
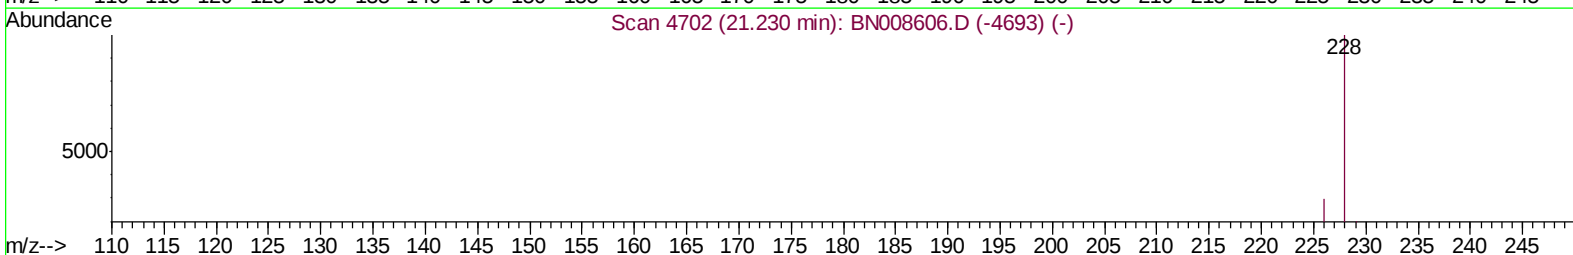
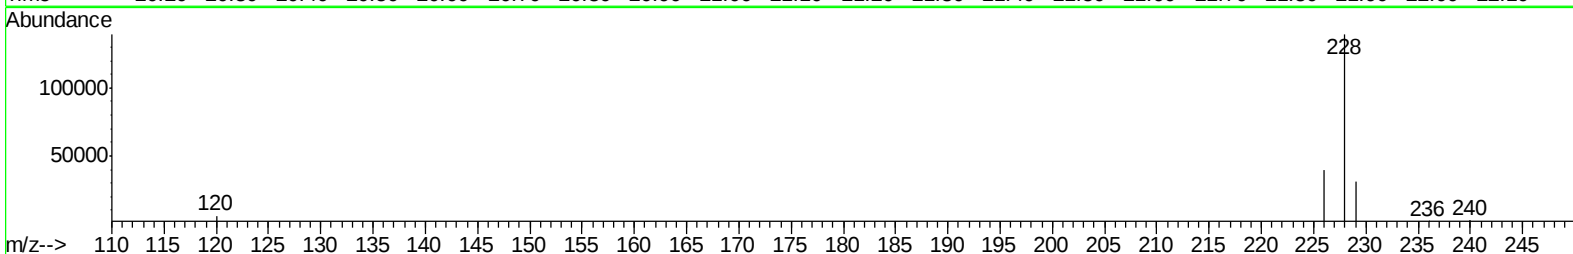


Data File : BN008616.D
Acq On : 18 Nov 2019 22:31
Operator : JU
Sample : K5678-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Nov 19 01:52:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

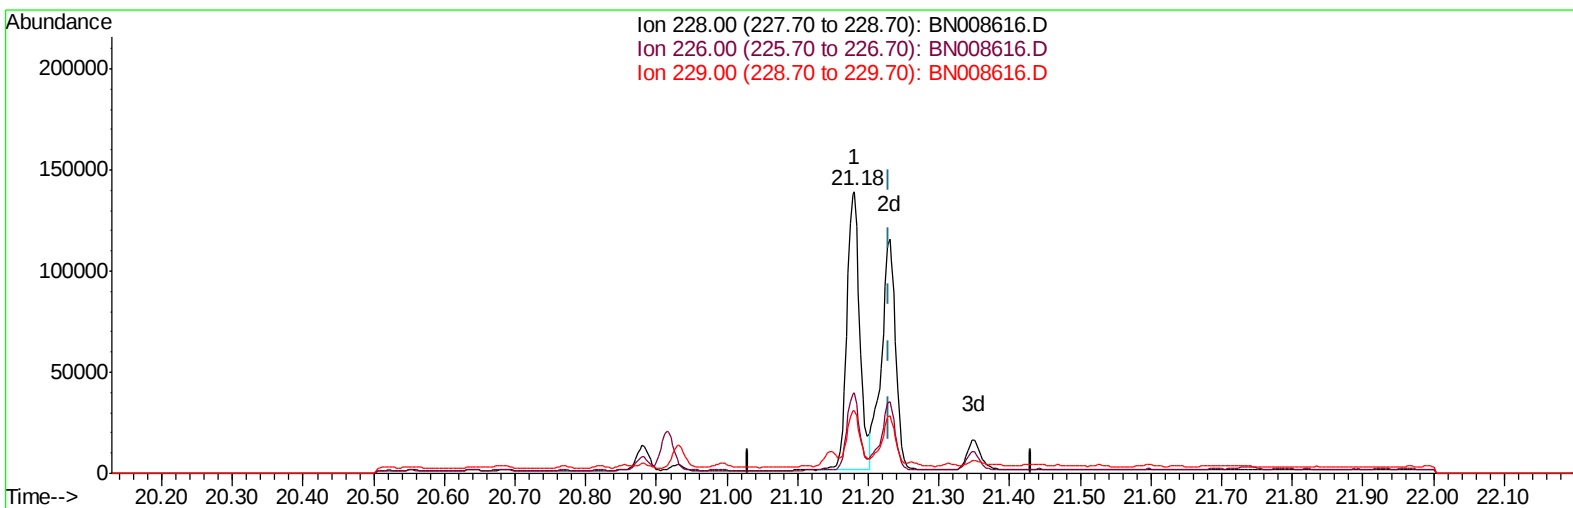

TIC: BN008616.D

(19) Chrysene

21.180min (-0.050) 4.13ng/ul

response 174240

Ion	Exp%	Act%
228.00	100	100
226.00	30.60	28.54
229.00	19.40	22.33
0.00	0.00	0.00