
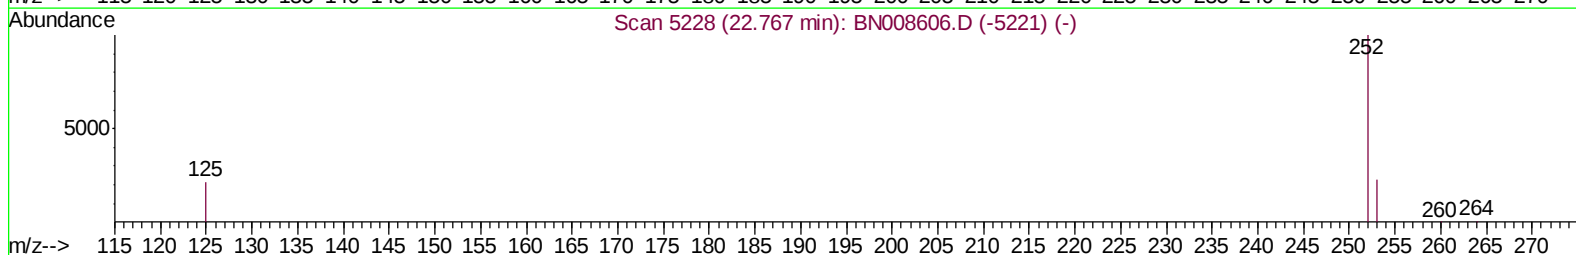
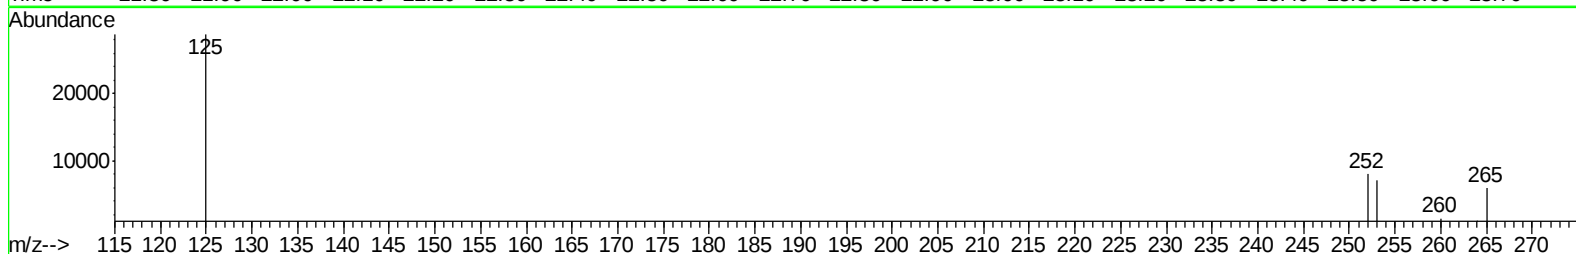


Data File : BN008617.D
Acq On : 18 Nov 2019 23:07
Operator : JU
Sample : K5678-17MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 19 03:09:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

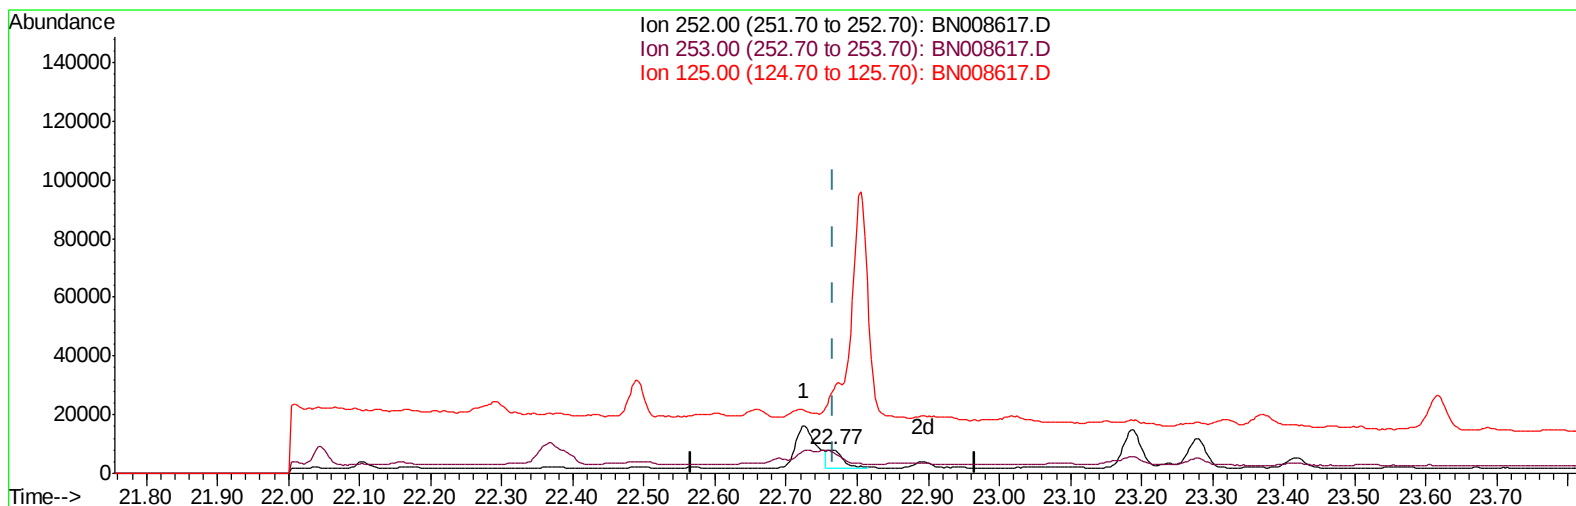

TIC: BN008617.D

(22) Benzo(k)fluoranthene

22.767min (-0.000) 0.20ng/ul m

response 9683

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	88.25#
125.00	18.70	357.76#
0.00	0.00	0.00