
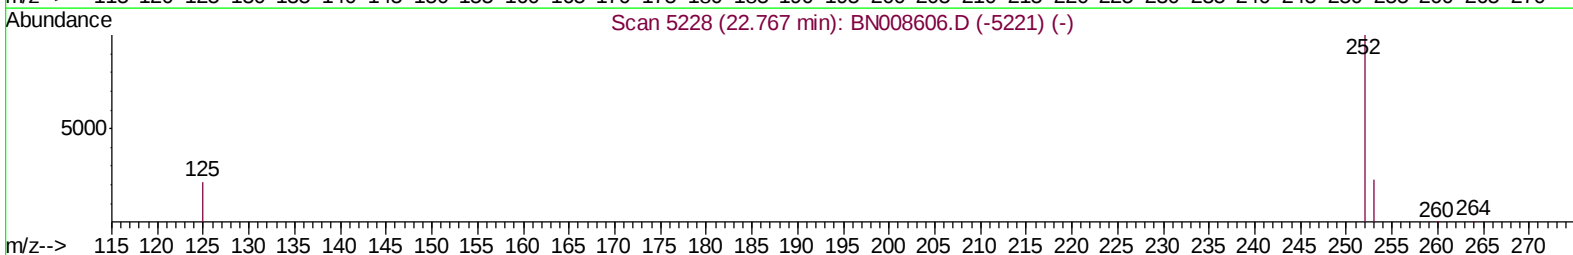
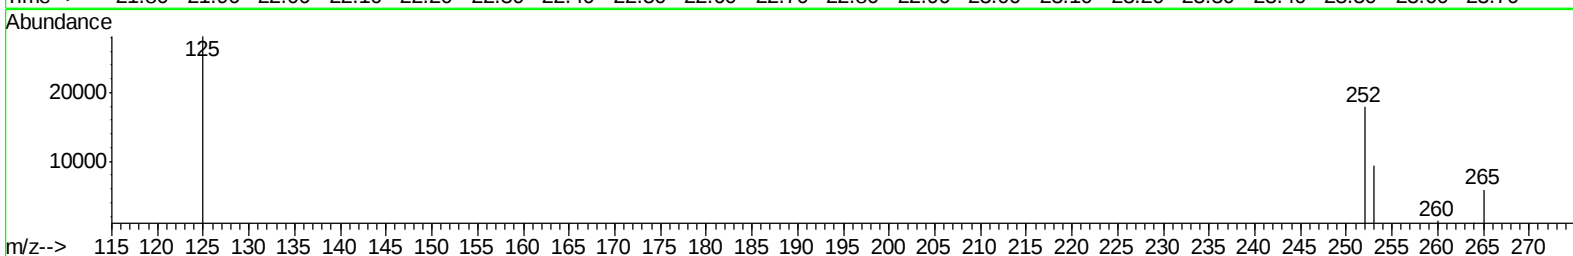


Data File : BN008618.D
Acq On : 18 Nov 2019 23:44
Operator : JU
Sample : K5678-18MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Nov 19 03:13:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

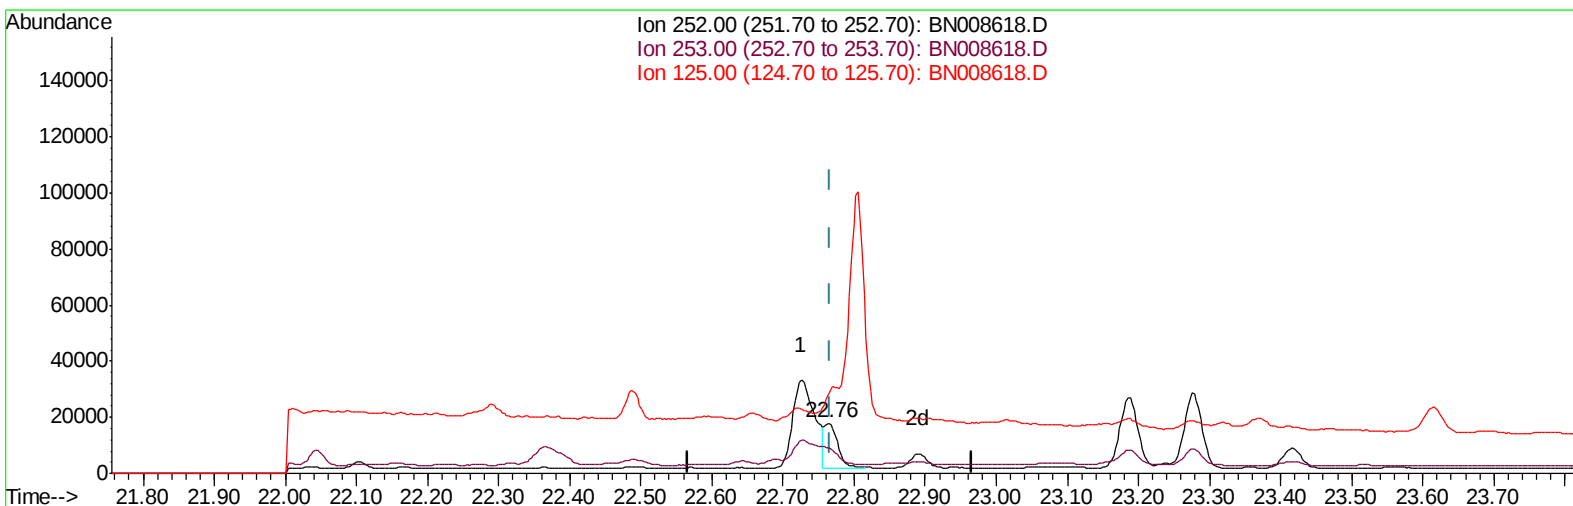

TIC: BN008618.D

(22) Benzo(k)fluoranthene

22.764min (-0.003) 0.41ng/ul m

response 20825

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	52.22#
125.00	18.70	157.73#
0.00	0.00	0.00