
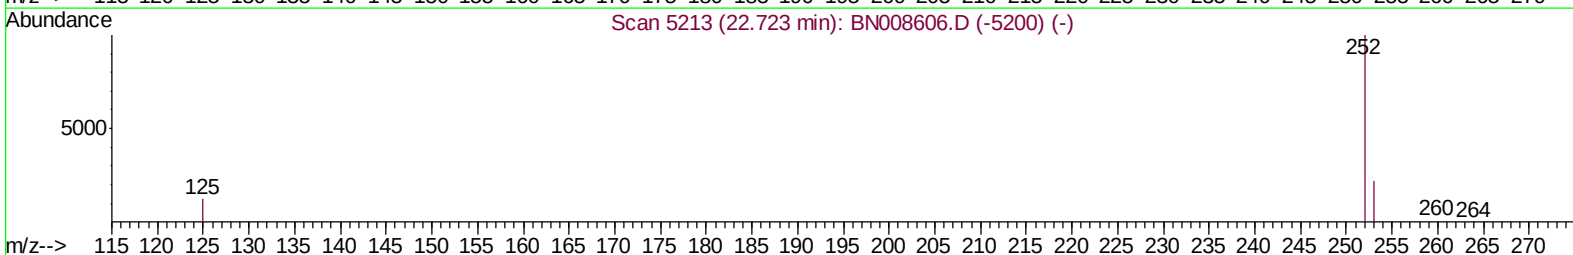
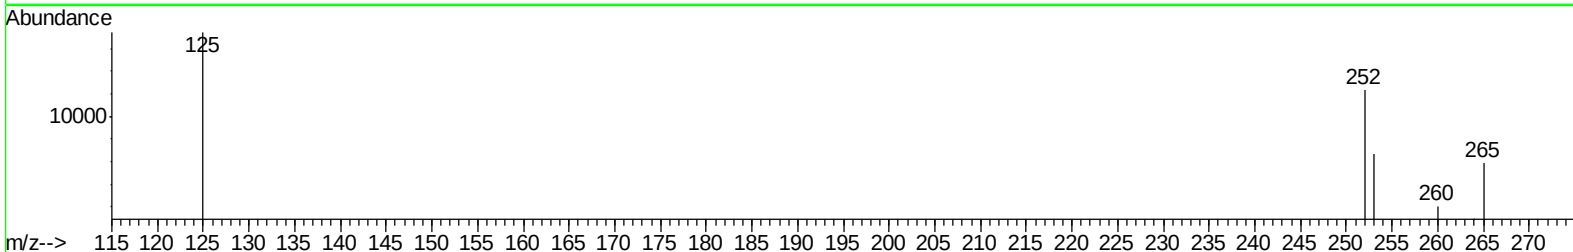


Data File : BN008619.D
Acq On : 19 Nov 2019 00:20
Operator : JU
Sample : K5678-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 19 03:19:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

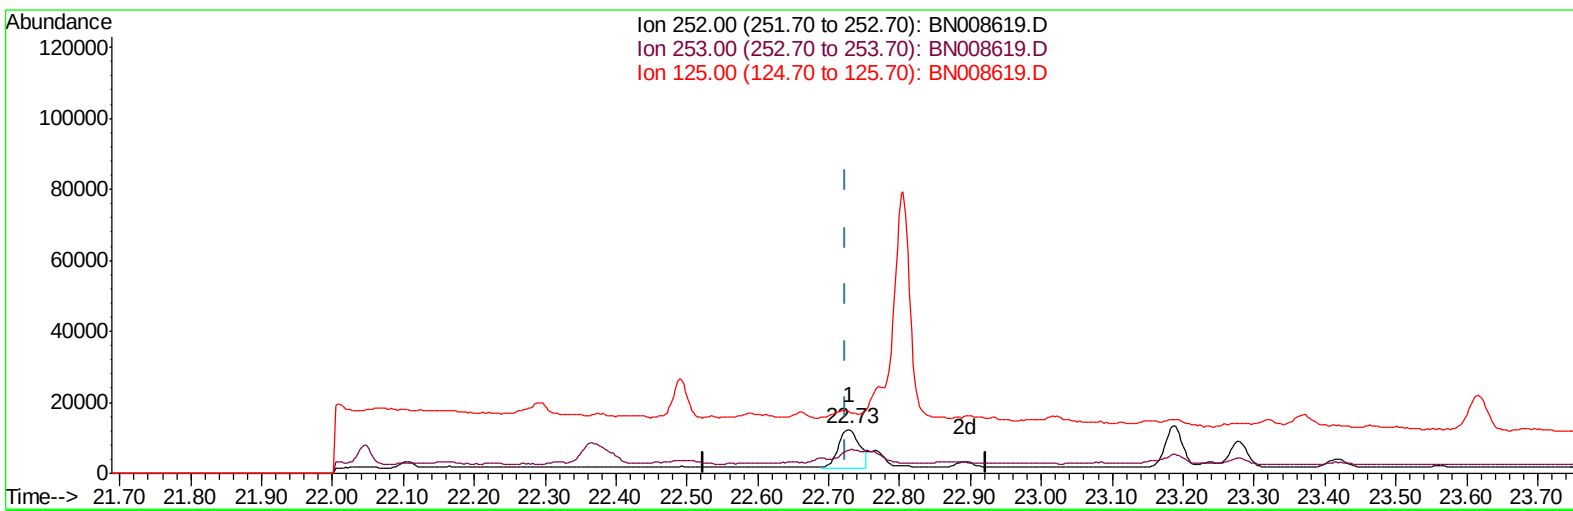

TIC: BN008619.D

(21) Benzo(b)fluoranthene

22.729min (+0.006) 0.46ng/ul m

response 22401

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	53.83#
125.00	15.00	140.84#
0.00	0.00	0.00