
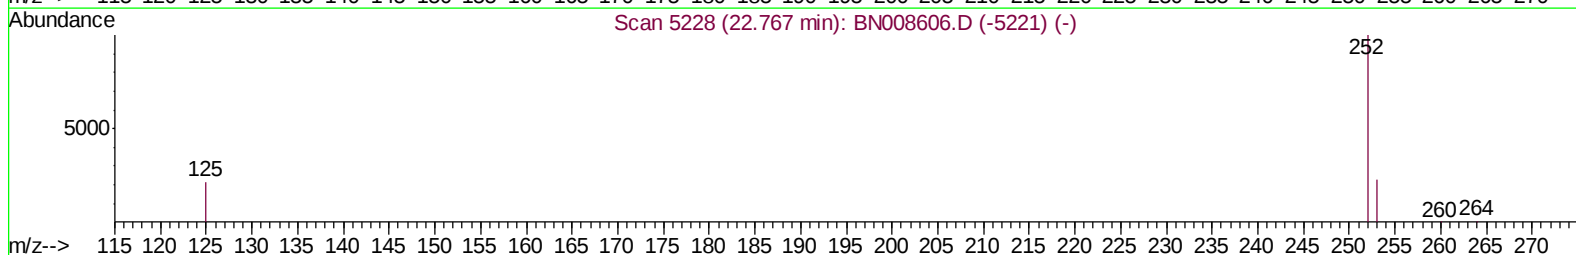
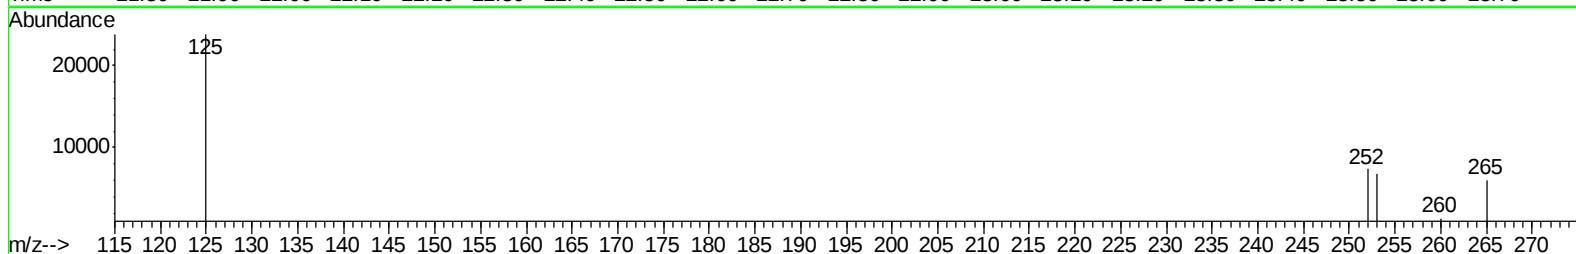


Data File : BN008620.D
Acq On : 19 Nov 2019 00:56
Operator : JU
Sample : K5678-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Nov 19 01:53:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

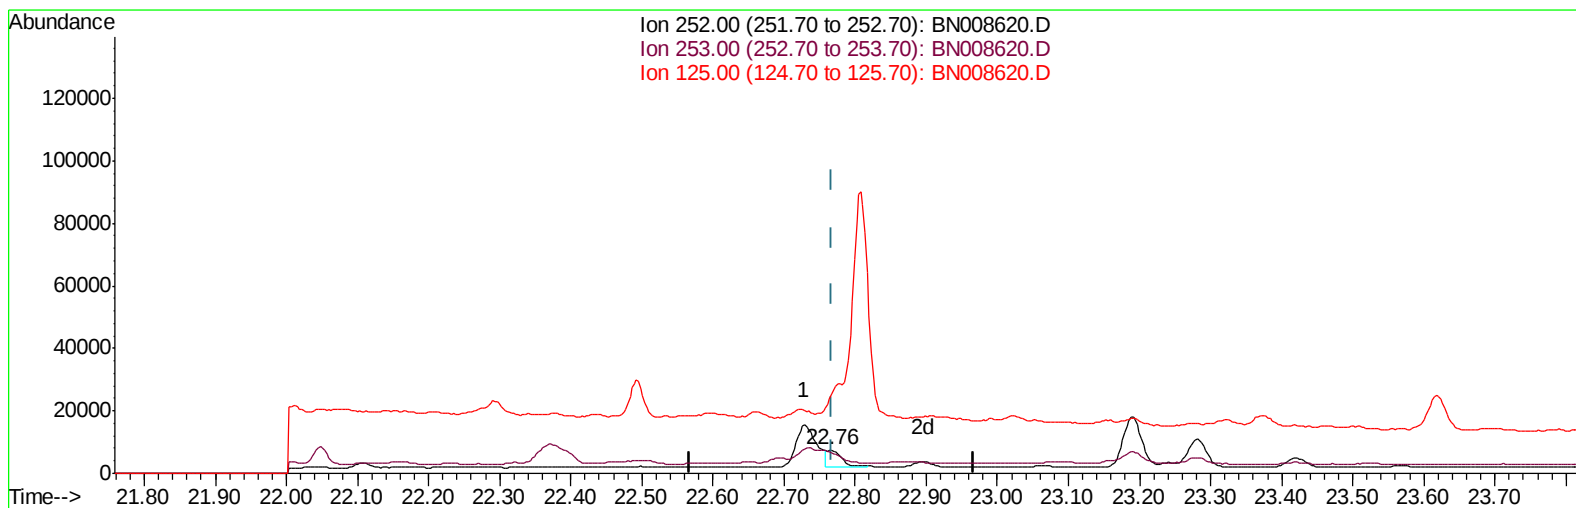

TIC: BN008620.D

(22) Benzo(k)fluoranthene

22.764min (-0.003) 0.17ng/ul m

response 8090

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	92.70#
125.00	18.70	321.77#
0.00	0.00	0.00