
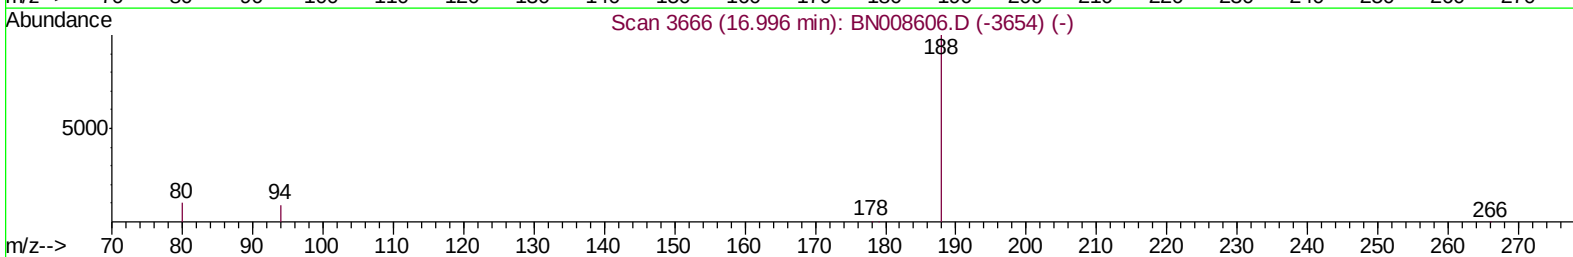
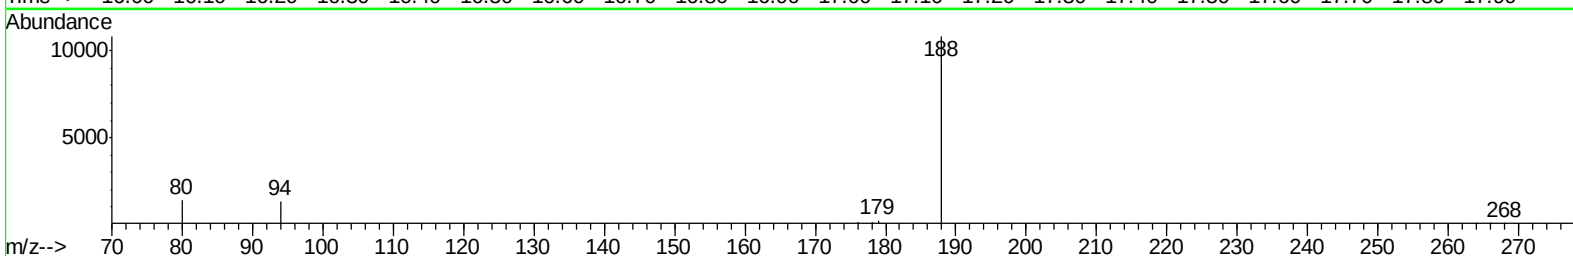


Data File : BN008621.D  
Acq On : 19 Nov 2019 01:32  
Operator : JU  
Sample : K5678-21  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Nov 19 03:24:00 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 19 01:47:58 2019  
Response via : Initial Calibration

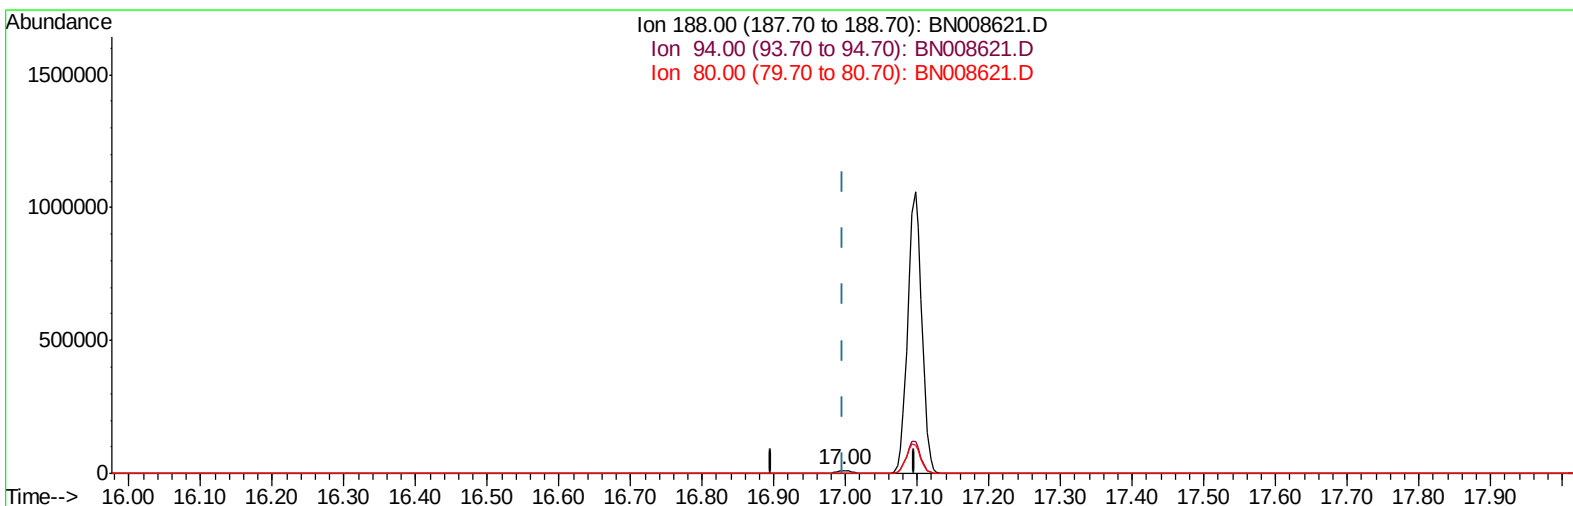

TIC: BN008621.D

(10) Phenanthrene-d10 (I)

16.996min (-0.000) 0.40ng/ul m

response 14906

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 188.00 | 100   | 100   |
| 94.00  | 10.60 | 12.43 |
| 80.00  | 11.80 | 12.98 |
| 0.00   | 0.00  | 0.00  |