
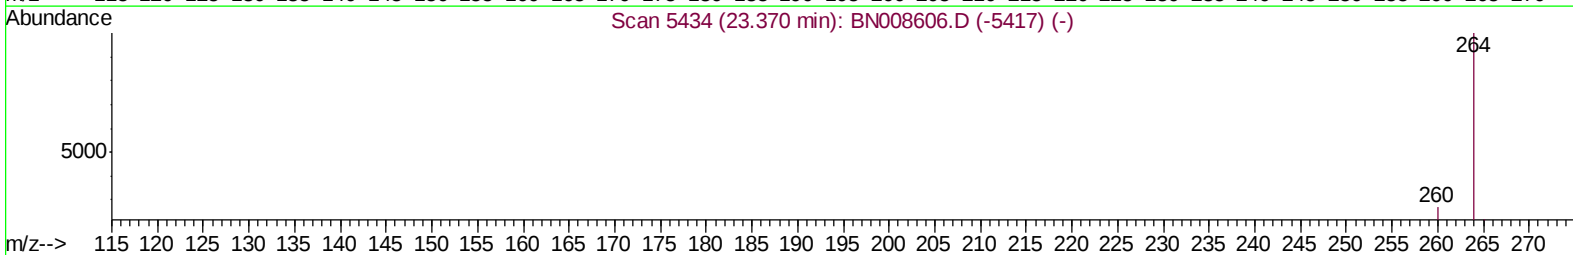
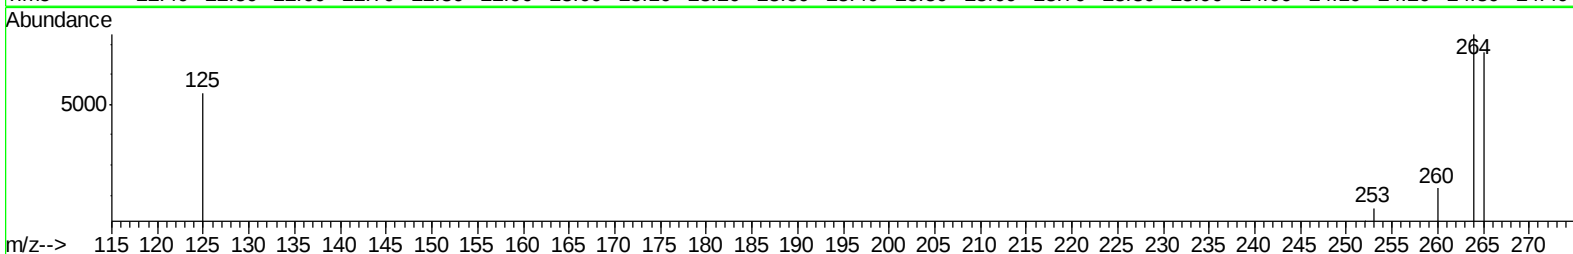


Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Nov 19 03:25:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

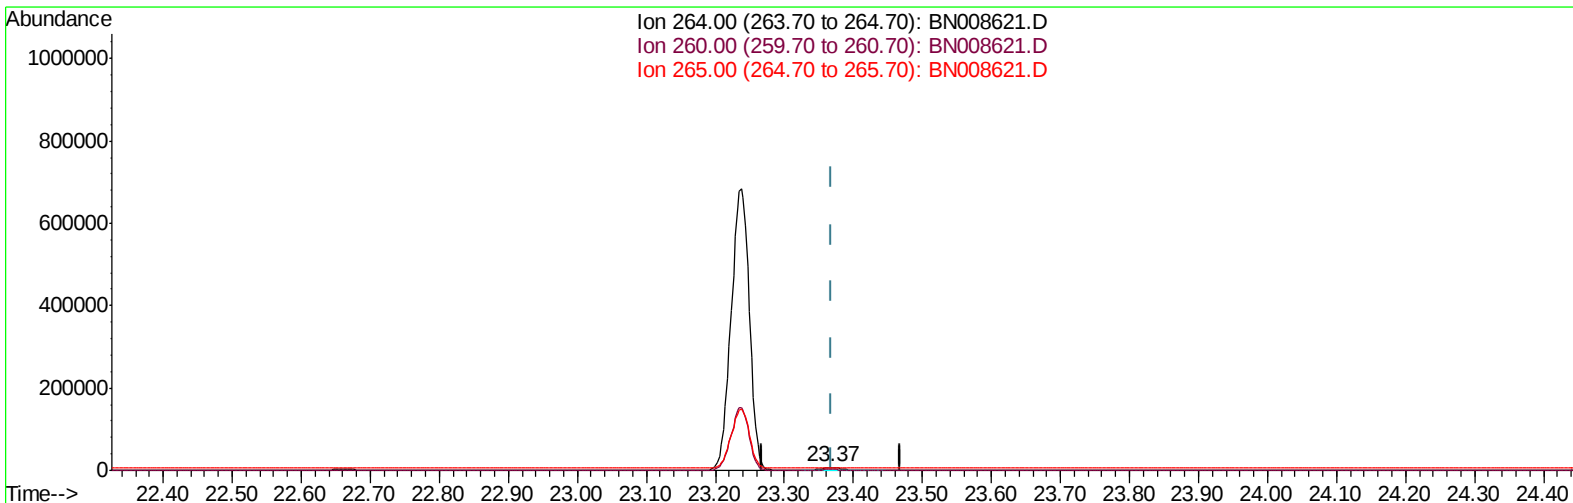

TIC: BN008621.D

(20) Perylene-d12 (I)

23.366min (-0.003) 0.40ng/ul

response 12603

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	30.48
265.00	69.30	91.86#
0.00	0.00	0.00