

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111819\
Quantitation Report (QT Reviewed)


Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMM1

Manual Integrations
APPROVED

mohammad
11/19/2019 2:45:43 PM

Quant Time: Nov 19 03:26:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

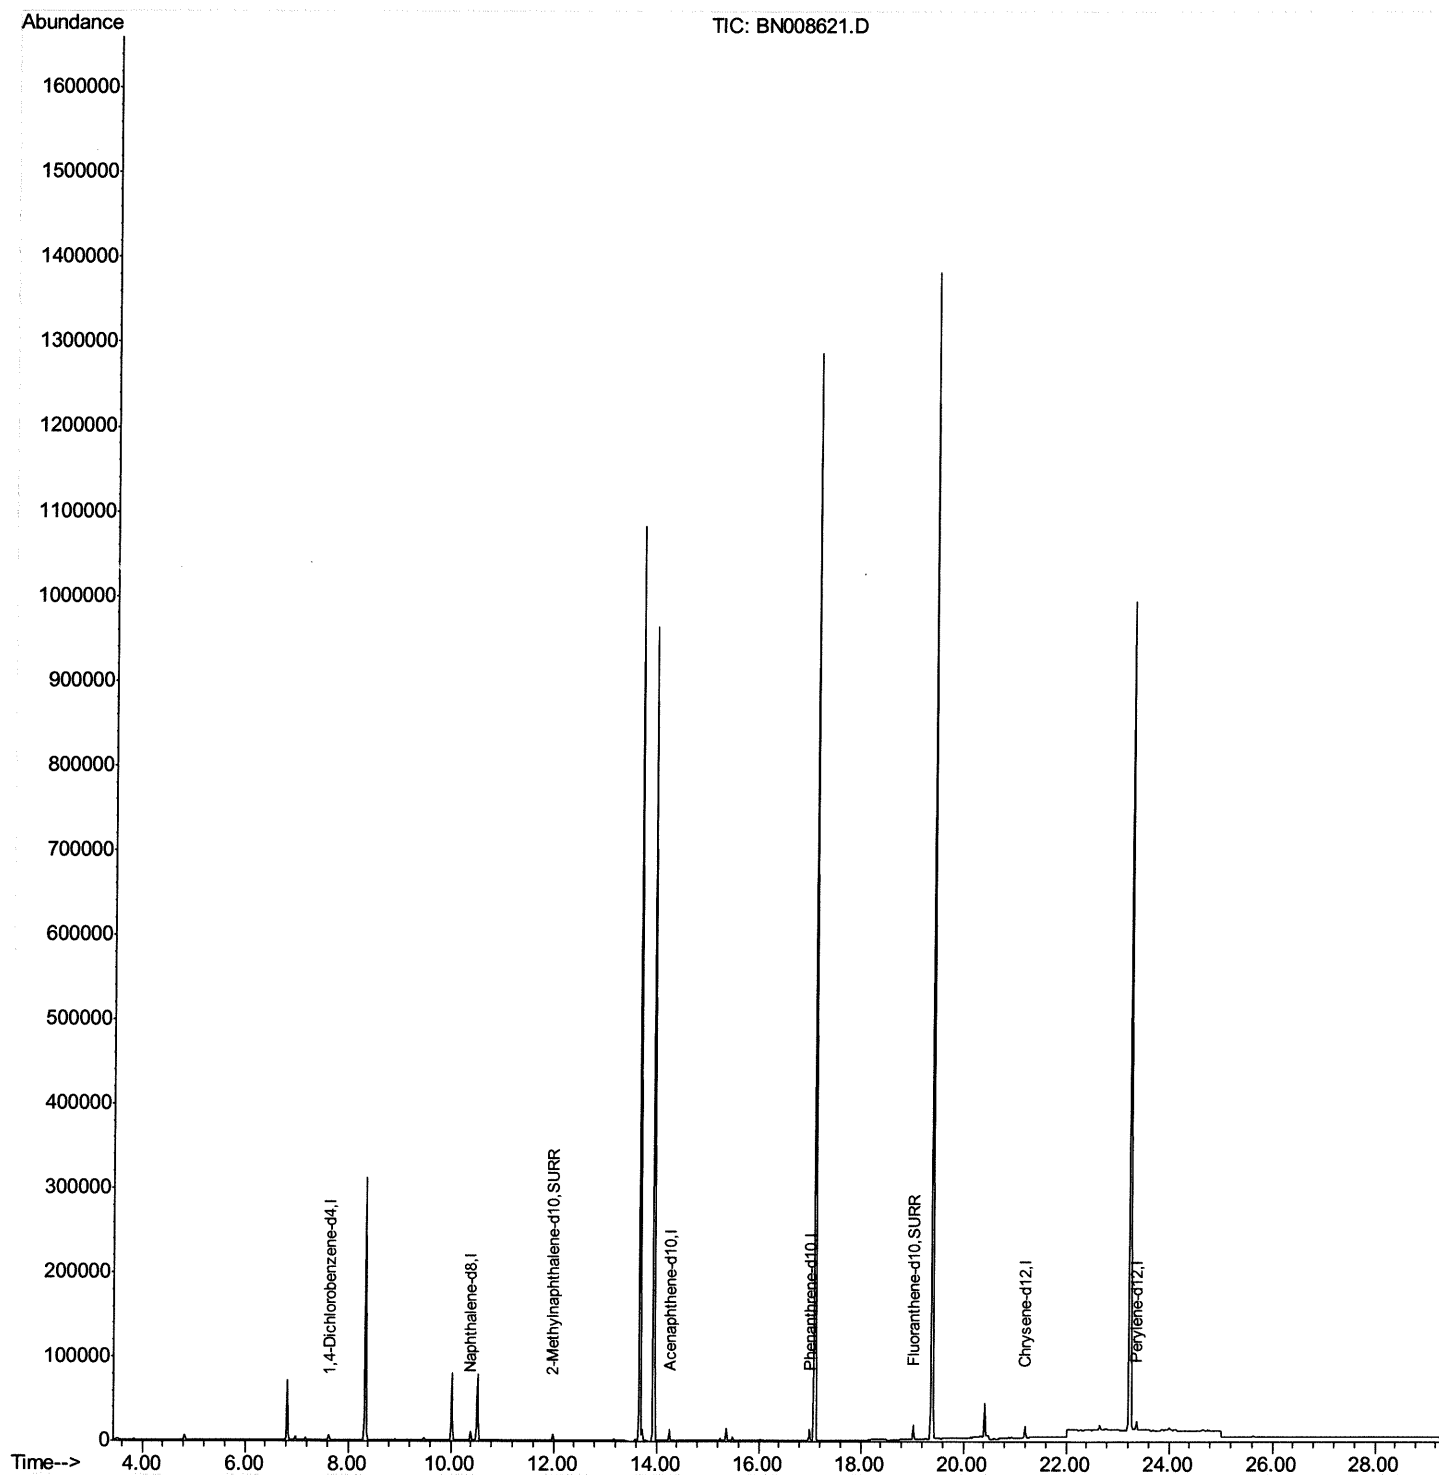

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111819\
Quantitation Report (Qedit)




Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMM1

Manual Integrations
APPROVED

mohammad
11/19/2019 2:45:43 PM

Quant Time: Nov 19 03:24:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

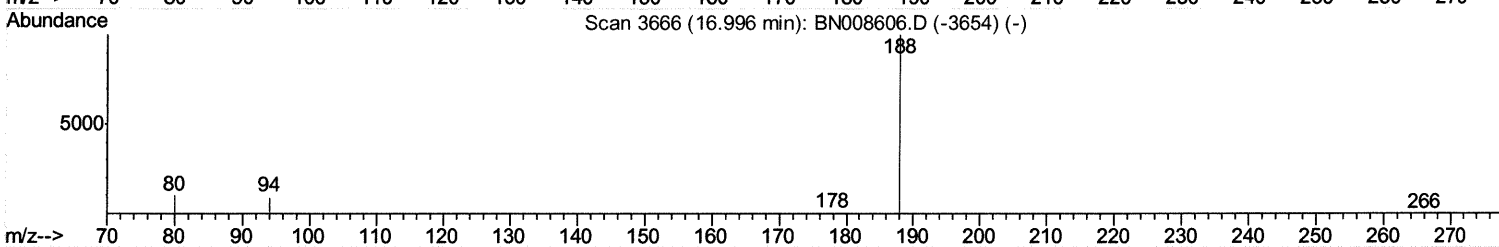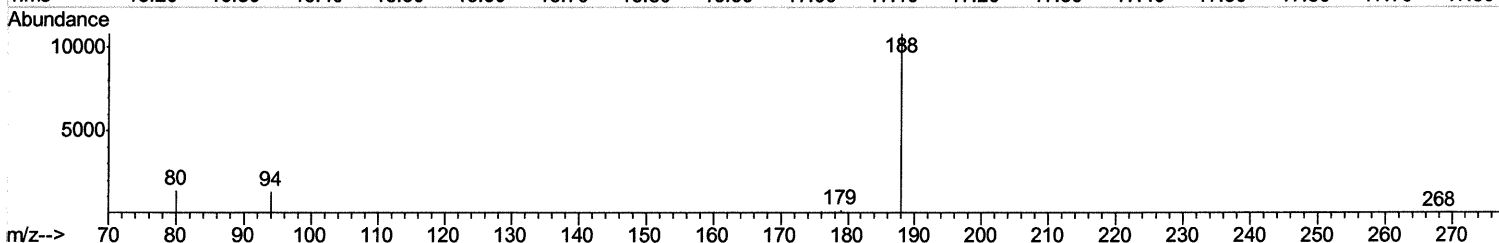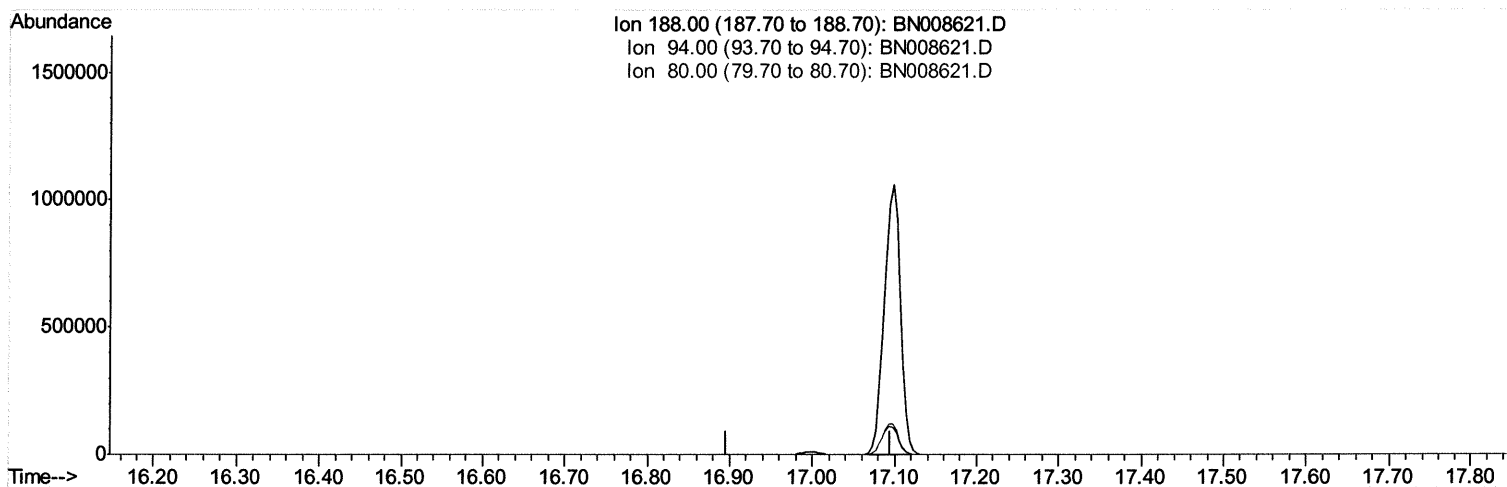

TIC: BN008621.D

(10) Phenanthrene-d10 (I)

16.996min (-16.996) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111819\
Quantitation Report (Qedit)




Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMM1

Manual Integrations
APPROVED

mohammad
11/19/2019 2:45:43 PM

Quant Time: Nov 19 03:24:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

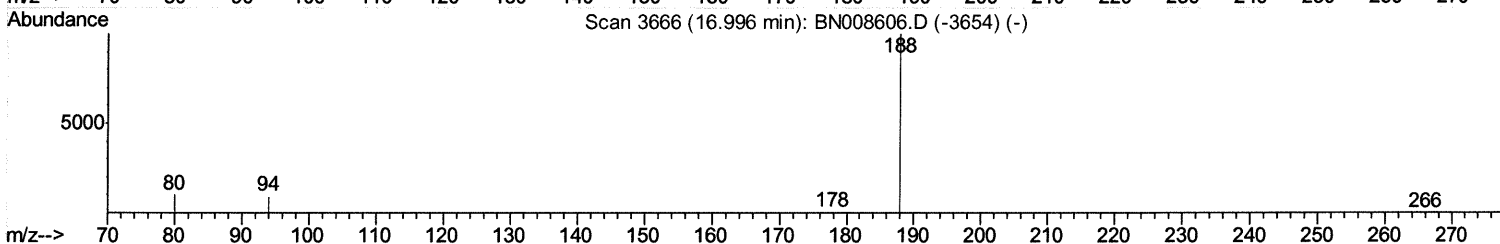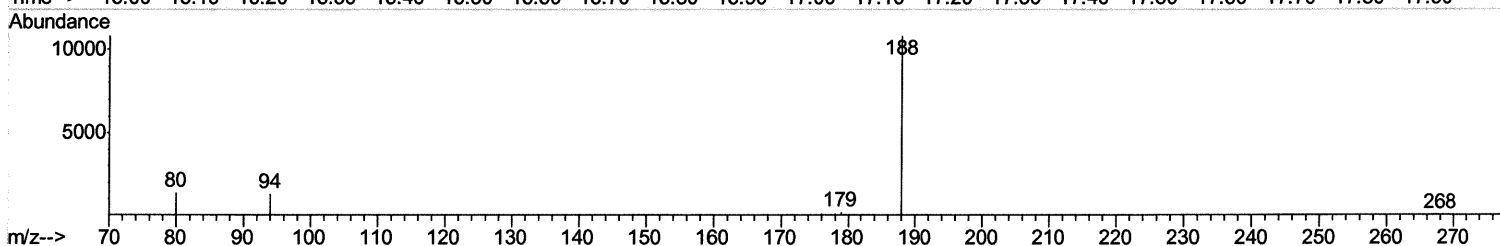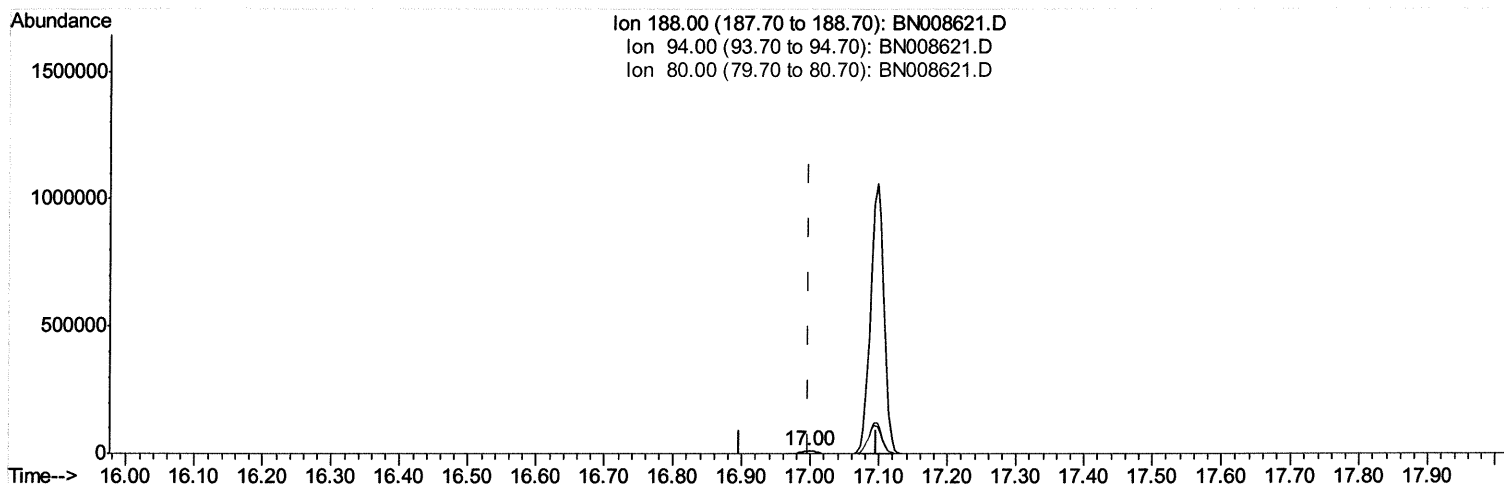

TIC: BN008621.D

(10) Phenanthrene-d10 (I)

16.996min (-0.000) 0.40ng/ul m

response 14906

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	12.43
80.00	11.80	12.98
0.00	0.00	0.00

344/24/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111819\
Quantitation Report (Qedit)




Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMM1

Manual Integrations
APPROVED

mohammad
11/19/2019 2:45:43 PM

Quant Time: Nov 19 03:25:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

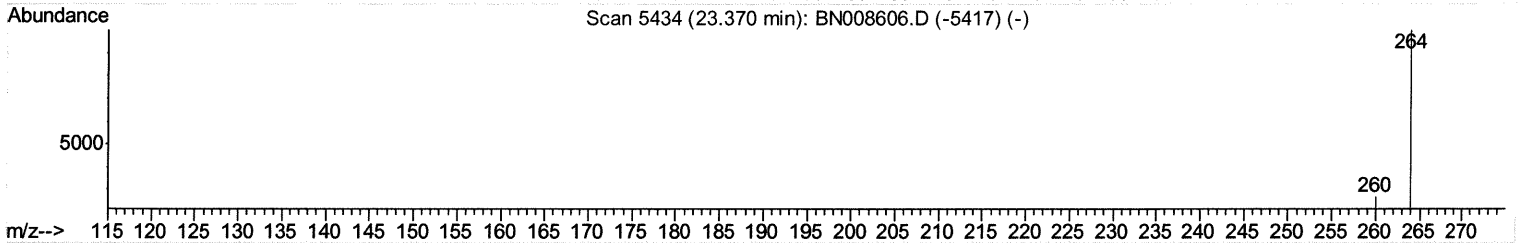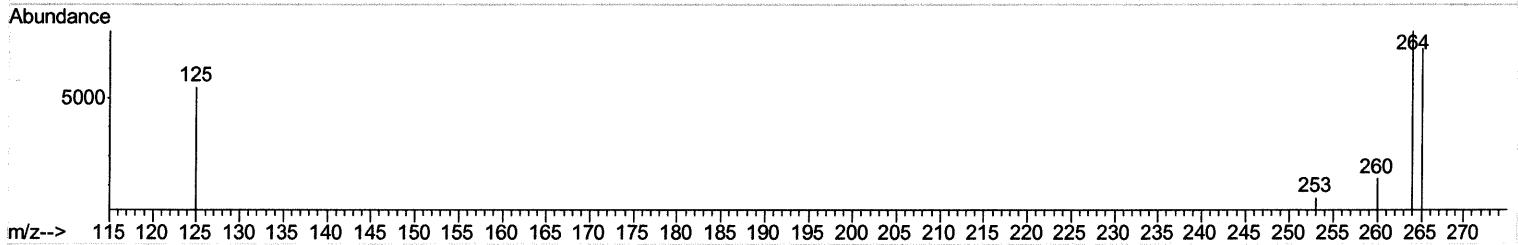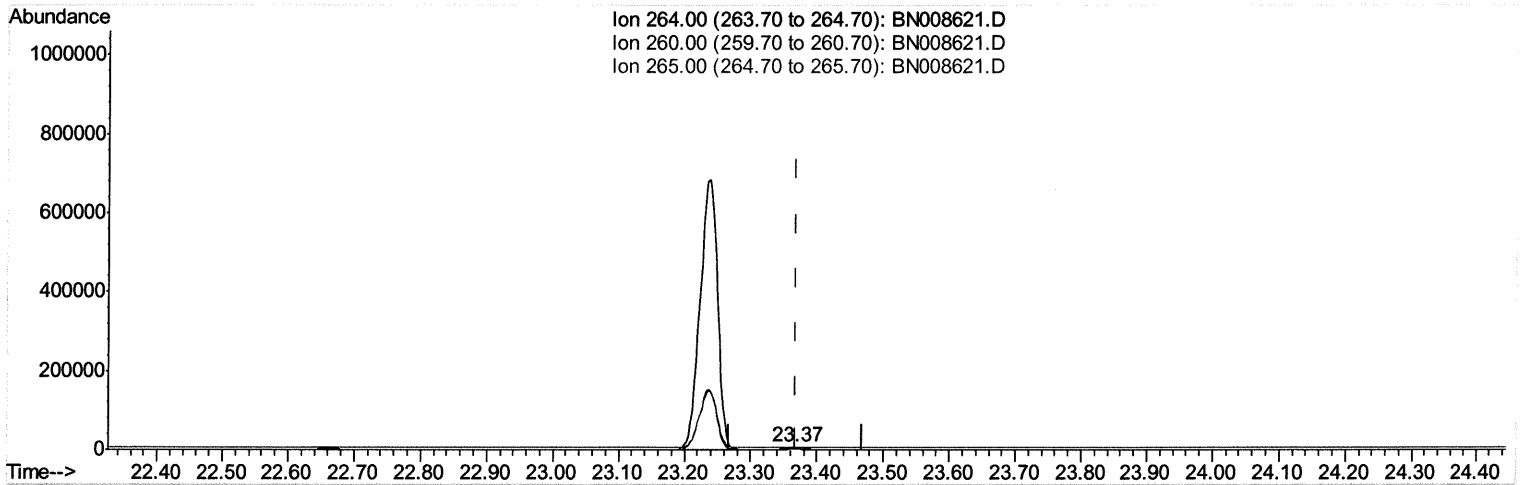

TIC: BN008621.D

(20) Perylene-d12 (I)

23.366min (-0.003) 0.40ng/ul

response 12603

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	30.48
265.00	69.30	91.86#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111819\
Quantitation Report (Qedit)




Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMM1

Manual Integrations
APPROVED

mohammad
11/19/2019 2:45:43 PM

Quant Time: Nov 19 03:25:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

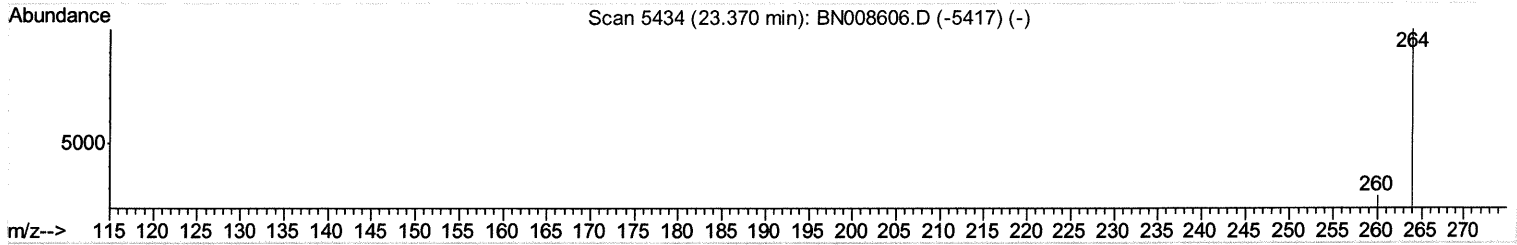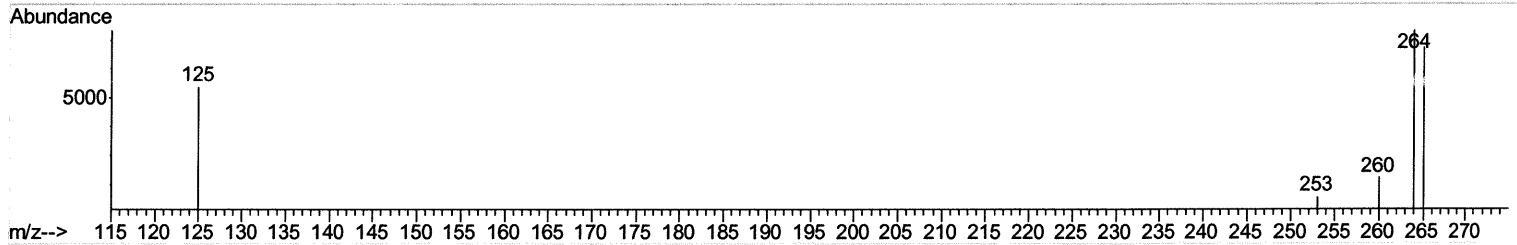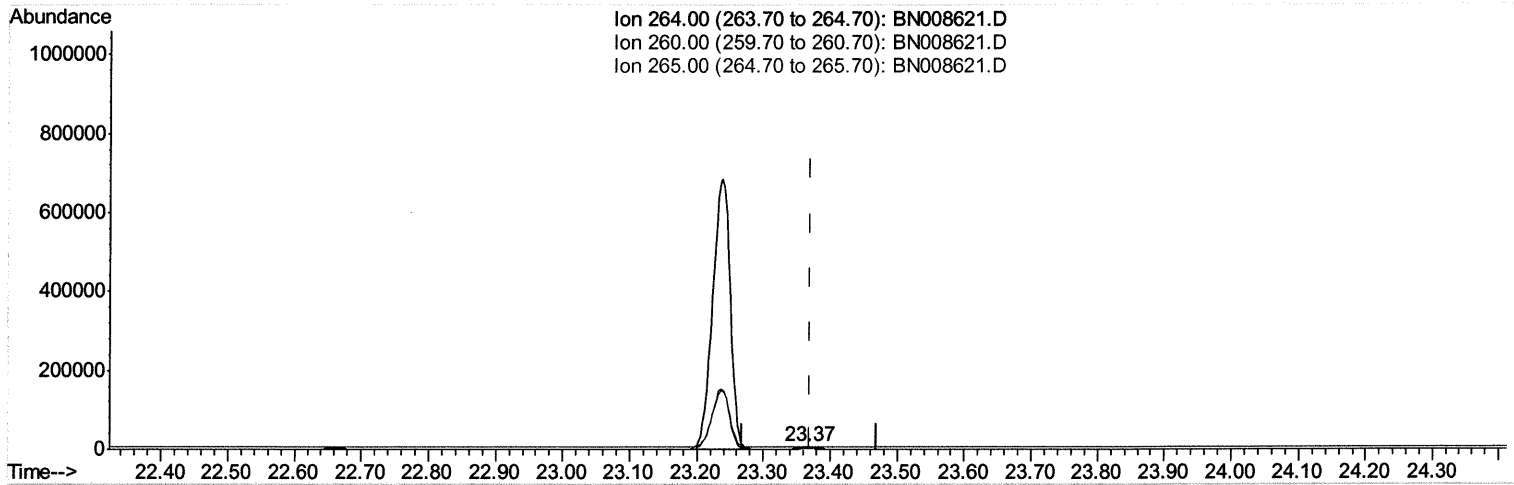

TIC: BN008621.D

(20) Perylene-d12 (I)

23.366min (-0.003) 0.40ng/ul m

response 12108

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	30.48
265.00	69.30	91.86#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111819\
Quantitation Report (QT Reviewed)

Data File : BN008621.D
Acq On : 19 Nov 2019 01:32
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMM1

Manual Integrations
APPROVED

mohammad
11/19/2019 2:45:43 PM

Quant Time: Nov 19 03:26:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3308	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	12363	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	7169	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	14906m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	12111	0.40	ng/ul	0.00
20) Perylene-d12	23.37	264	12108m	0.40	ng/ul	0.00

Handwritten notes: >JU 11/21/19 and >JU 11/21/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152	8912	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.03	212	19873	0.44	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed