

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
 Data File : BN012607.D
 Acq On : 18 Nov 2020 23:06
 Operator : CG/JU
 Sample : L4726-22
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGG2

Quant Time: Nov 19 03:46:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	132162	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	519874	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	338414	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	729945	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	756712	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	840728	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	20344	5.49	ng/uL	0.00
5) Phenol-d5	6.63	99	67540	5.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	205139	28.96	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	215474	22.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	125531	12.78	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	126524	29.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	146126	30.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	231608	25.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	20098	2.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	930641	33.67	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1095148	33.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	19784	3.82	ng/ul	0.00
58) Fluorene-d10	15.10	176	810770	33.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	164248	32.98	ng/ul	0.00
71) Anthracene-d10	16.96	188	1412164	38.08	ng/ul	0.00
79) Pyrene-d10	19.26	212	1589446	40.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.05	264	1862799	40.54	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.57	163	52077	1.871	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111820\
Data File : BN012607.D
Acq On : 18 Nov 2020 23:06
Operator : CG/JU
Sample : L4726-22
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGG2

Quant Time: Nov 19 03:46:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 18 14:31:59 2020
Response via : Initial Calibration

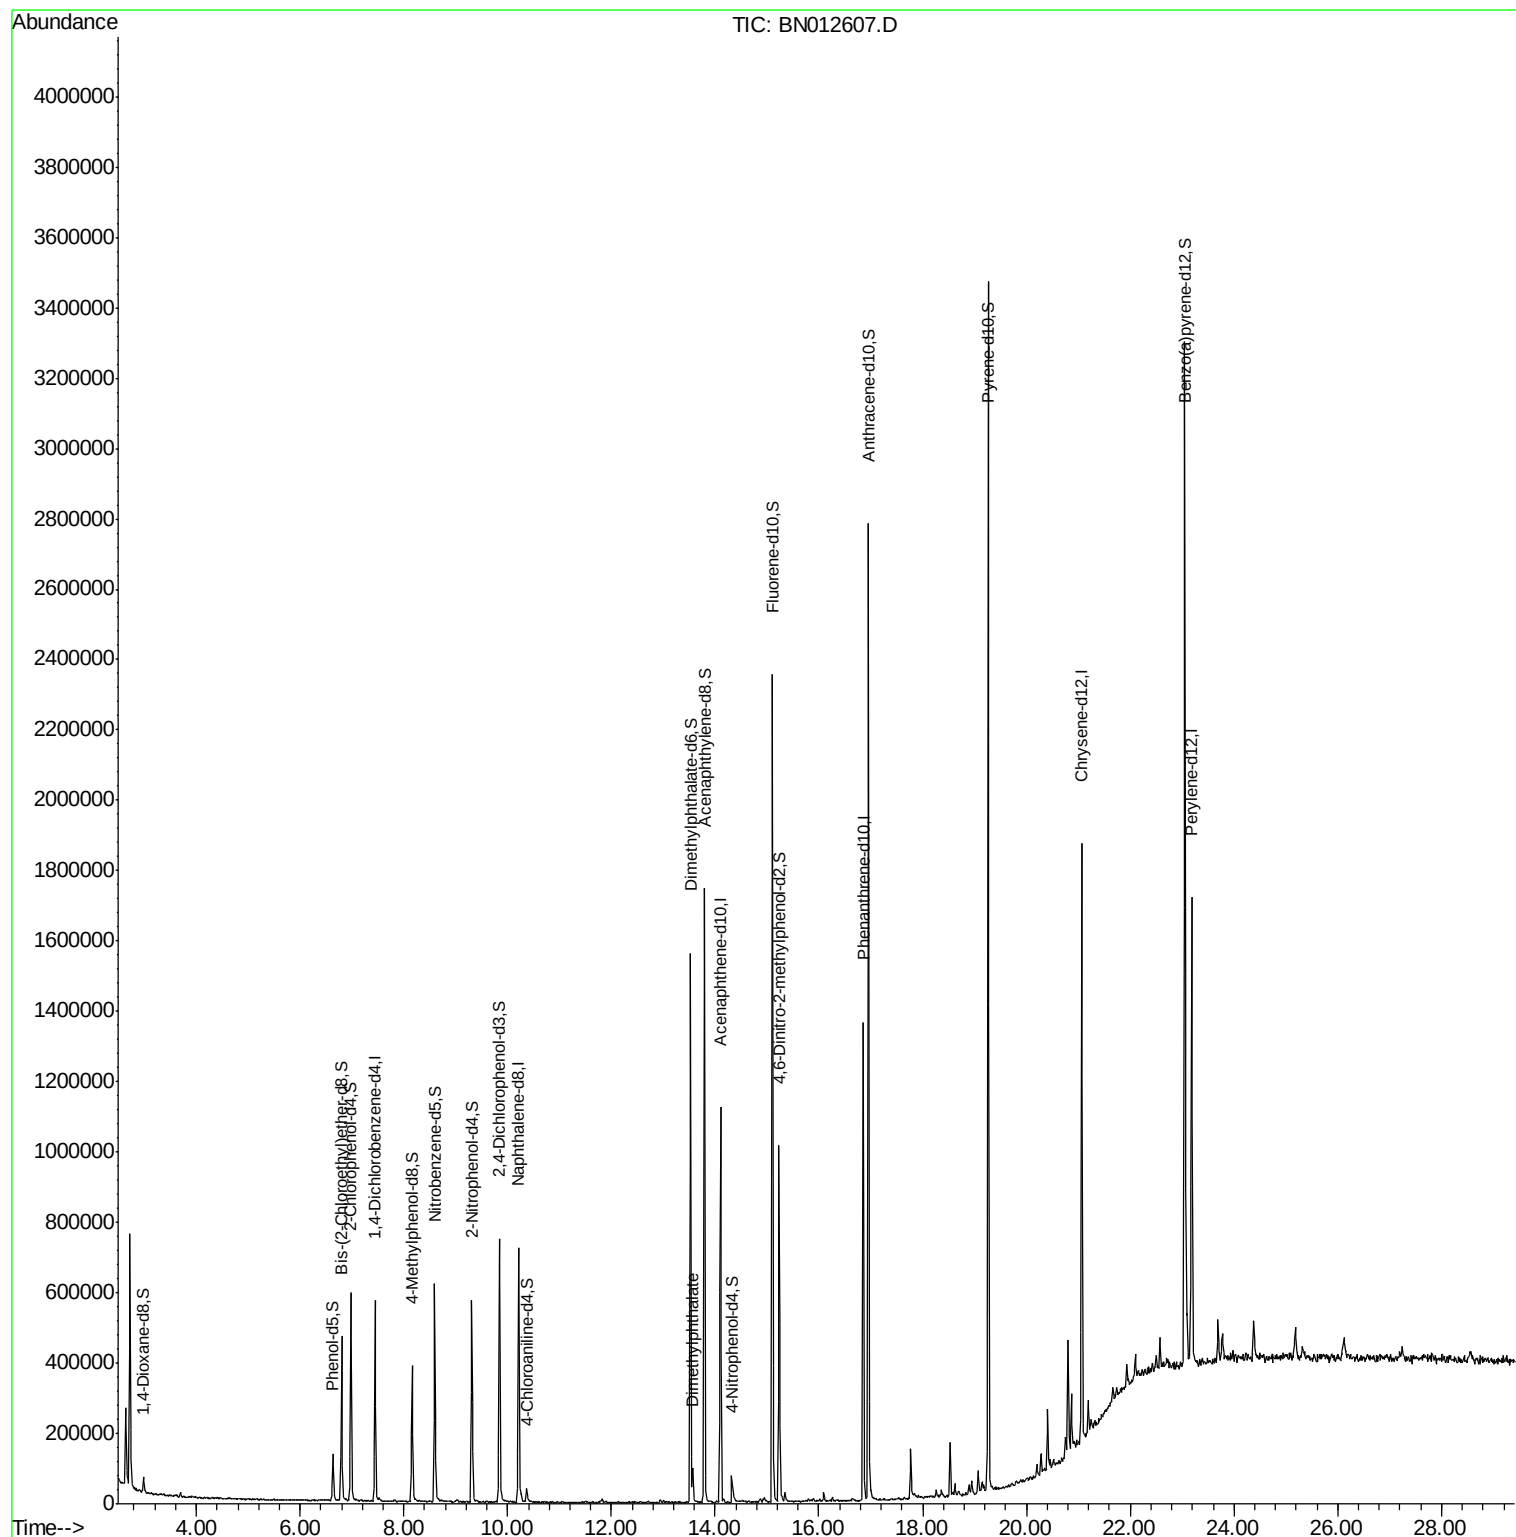

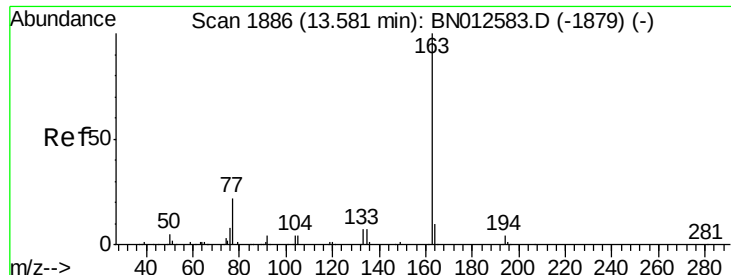

#45

Dimethylphthalate

Concen: 1.871 ng/ul

RT: 13.57 min Scan# 1884

Delta R.T. -0.01 min

Lab File: BN012607.D

Acq: 18 Nov 2020 23:06

Instrument :

BNA_N

ClientSampleId :

DBG2


Tot Ion:163 Resp: 52077

Ion Ratio Lower Upper

163 100

194 4.1 3.0 4.4

164 11.4 8.6 13.0

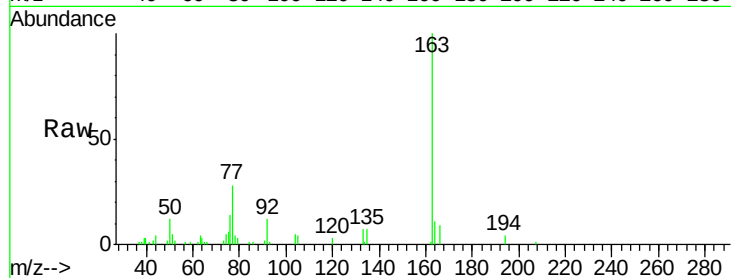

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

