

#45

Dimethylphthalate

Concen: 3.195 ng/ul

RT: 13.57 min Scan# 1885

Delta R.T. 0.00 min

Lab File: BN012615.D

Acq: 19 Nov 2020 04:32

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 95756

Ion Ratio Lower Upper




163 100

194 3.9 3.0 4.4

164 8.9 8.6 13.0

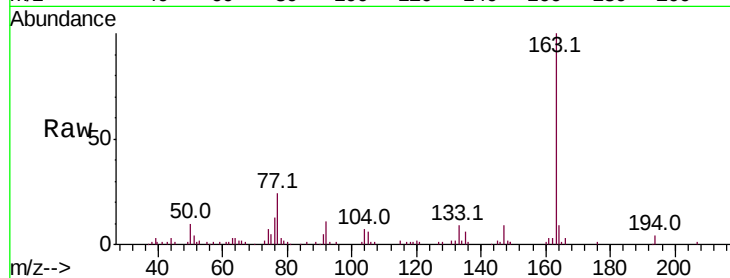

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

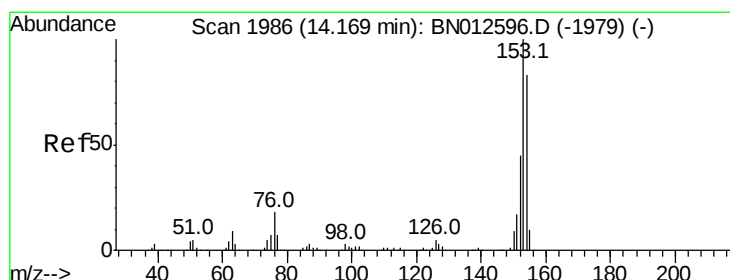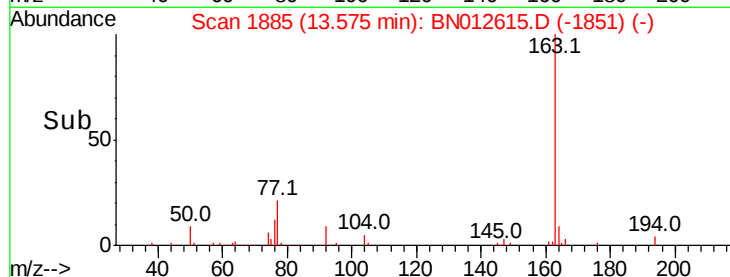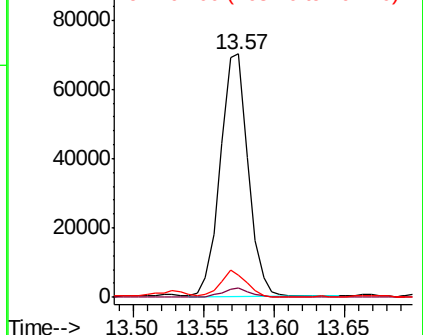

#50

Acenaphthene

Concen: 52.860 ng/ul

RT: 14.17 min Scan# 1986

Delta R.T. 0.00 min

Lab File: BN012615.D

Acq: 19 Nov 2020 04:32


Tgt Ion:153 Resp: 1373034

Ion Ratio Lower Upper

153 100

152 46.8 37.1 55.7

154 89.7 69.7 104.5

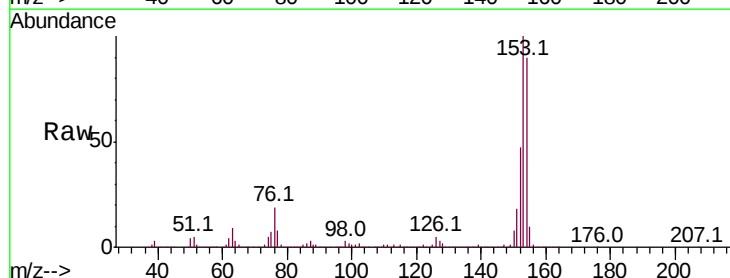

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

