
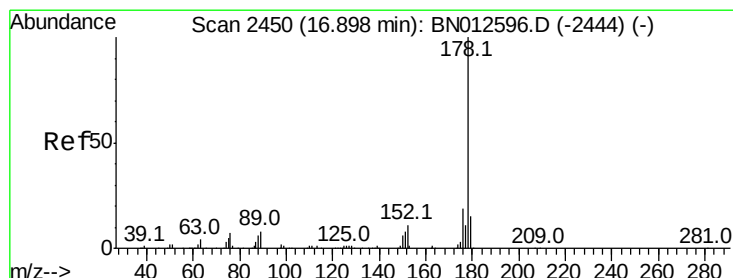
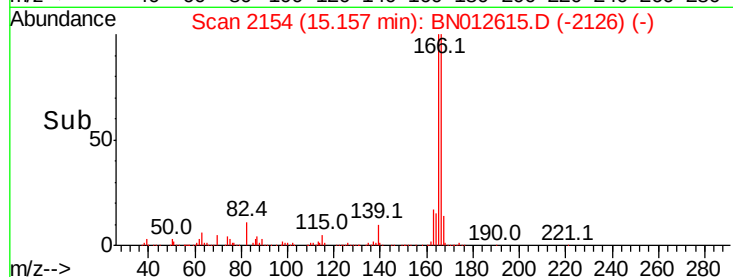
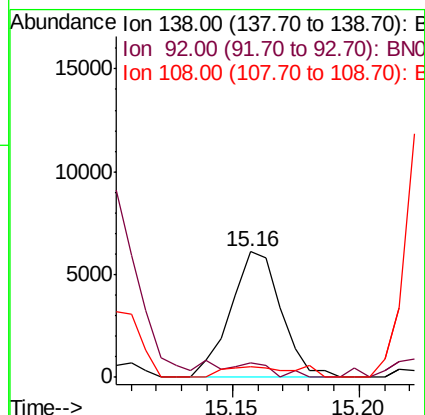


#61
4-Nitroaniline
Concen: 1.431 ng/ul
RT: 15.16 min Scan# 2154
Delta R.T. -0.04 min
Lab File: BN012615.D
Acq: 19 Nov 2020 04:32

Instrument :
BNA_N
ClientSampleId :

Tot Ion:138 Resp: 8481
Ion Ratio Lower Upper
138 100
92 11.5 47.0 70.4#
108 8.6 79.8 119.6#

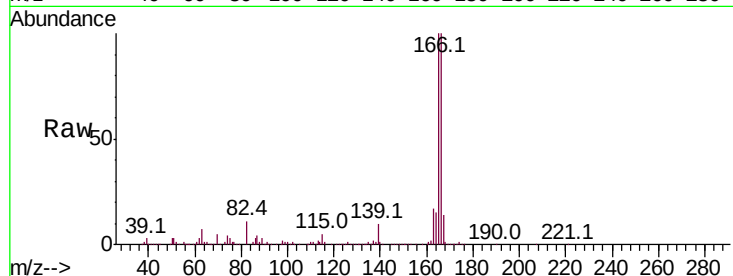

#70
Phenanthrene
Concen: 9.014 ng/ul
RT: 16.90 min Scan# 2450
Delta R.T. 0.00 min
Lab File: BN012615.D
Acq: 19 Nov 2020 04:32

Tgt Ion:178 Resp: 462128
Ion Ratio Lower Upper
178 100
179 14.5 13.1 19.7
176 18.0 15.4 23.0

