

#15

N-Nitroso-di-n-propylamine

Concen: 34.174 ng/ul

RT: 8.25 min Scan# 980

Delta R.T. -0.01 min

Lab File: BN012616.D

Acq: 19 Nov 2020 05:09

Instrument :

BNA_N

ClientSampleId :

Tot Ion: 70 Resp: 307164


Ion	Ratio	Lower	Upper
70	100		
42	64.2	50.0	75.0
101	9.2	7.5	11.3
130	20.0	17.6	26.4

70 100

42 64.2 50.0 75.0

101 9.2 7.5 11.3

130 20.0 17.6 26.4

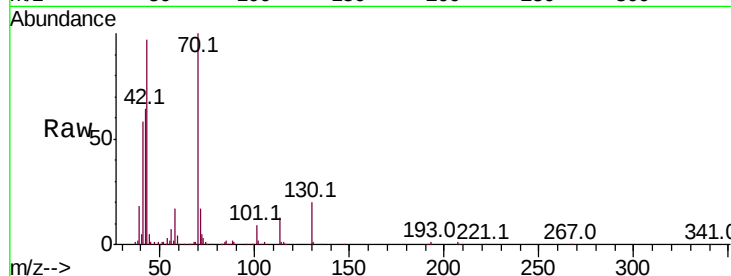




Abundance Ion 70.00 (69.70 to 70.70): BN0

Ion 42.00 (41.70 to 42.70): BN0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

Time-->

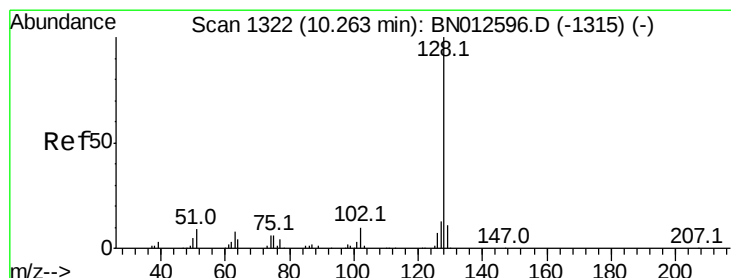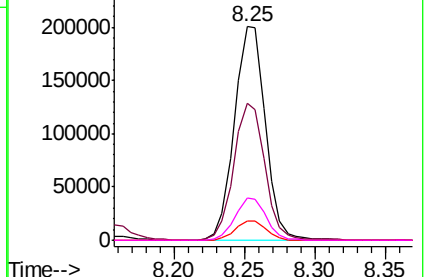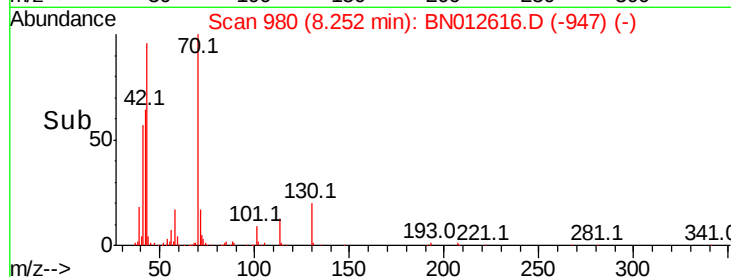

#28

Naphthalene

Concen: 277.764 ng/ul

RT: 10.27 min Scan# 1323

Delta R.T. 0.01 min

Lab File: BN012616.D

Acq: 19 Nov 2020 05:09


Tgt Ion:128 Resp:10359359

Ion	Ratio	Lower	Upper
128	100		
129	11.1	8.6	12.8
127	13.7	11.6	17.4

128 100

129 11.1 8.6 12.8

127 13.7 11.6 17.4

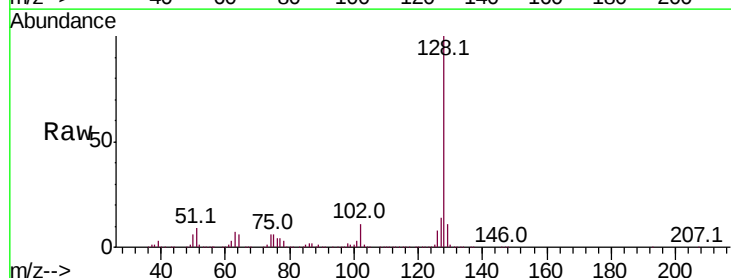

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

Time-->

