

#55

2,4-Dinitrotoluene

Concen: 36.651 ng/ul

RT: 14.49 min Scan# 2040

Delta R.T. 0.00 min

Lab File: BN012616.D

Acq: 19 Nov 2020 05:09

Instrument :

BNA_N

ClientSampleId :


Tot Ion:165 Resp: 378486

Ion Ratio Lower Upper

165 100

63 56.7 39.4 59.0




182 2.9 2.8 4.2

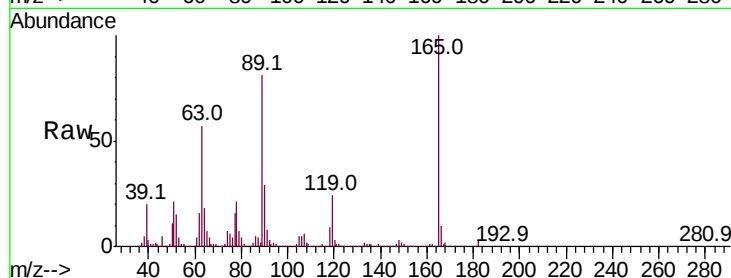

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BNO

Ion 182.00 (181.70 to 182.70): E

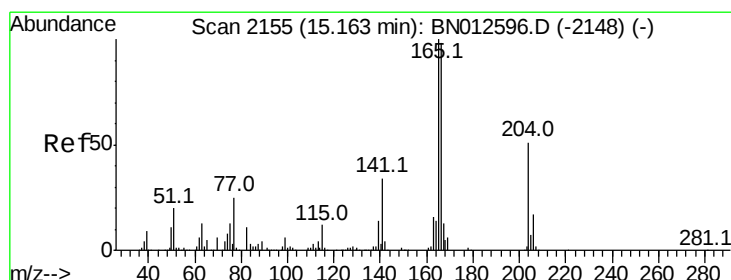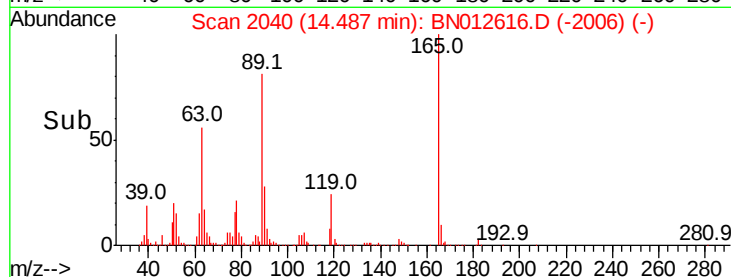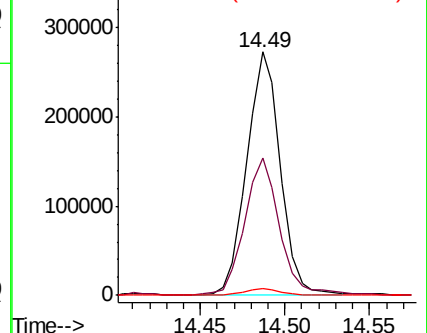

#59

Fluorene

Concen: 19.012 ng/ul

RT: 15.16 min Scan# 2154

Delta R.T. -0.01 min

Lab File: BN012616.D

Acq: 19 Nov 2020 05:09


Tgt Ion:166 Resp: 670762

Ion Ratio Lower Upper

166 100

165 101.5 83.3 124.9

167 14.3 11.0 16.6

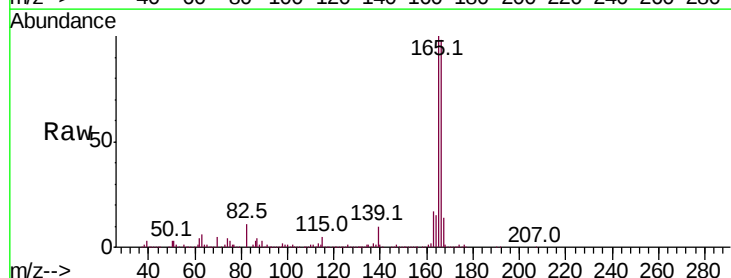

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

