





#61
4-Nitroaniline
Concen: 1.245 ng/ul
RT: 15.16 min Scan# 2154
Delta R.T. -0.04 min
Lab File: BN012616.D
Acq: 19 Nov 2020 05:09

Instrument :
BNA_N
ClientSampled :

Tot Ion:138 Resp: 8652
Ion Ratio Lower Upper
138 100
92 14.5 47.0 70.4#
108 12.5 79.8 119.6#

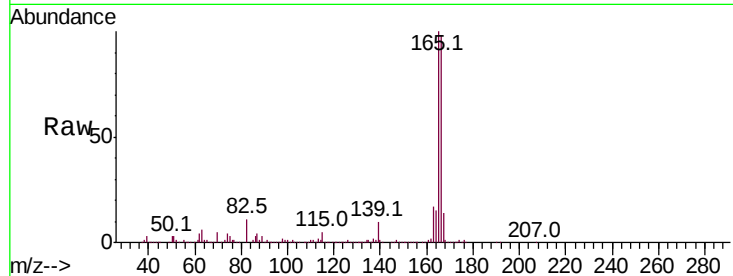


Abundance Ion 138.00 (137.70 to 138.70): E
Ion 92.00 (91.70 to 92.70): BNO
Ion 108.00 (107.70 to 108.70): E

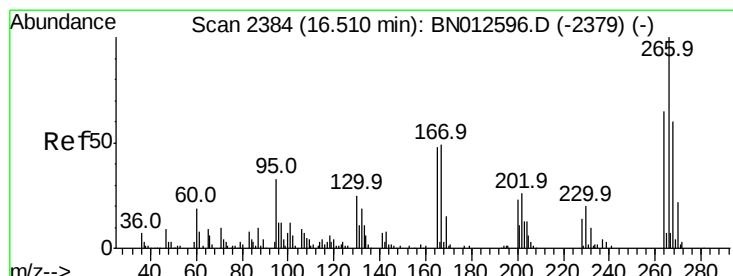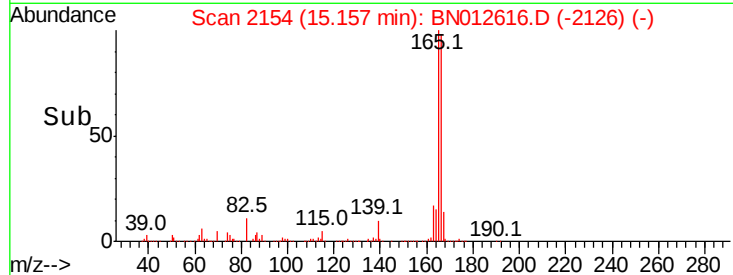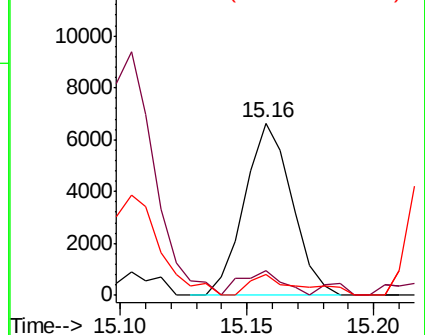

#69
Pentachlorophenol
Concen: 37.819 ng/ul
RT: 16.51 min Scan# 2384
Delta R.T. -0.01 min
Lab File: BN012616.D
Acq: 19 Nov 2020 05:09

Tgt Ion:266 Resp: 283796
Ion Ratio Lower Upper
266 100
264 61.8 55.0 82.6
268 65.8 56.9 85.3

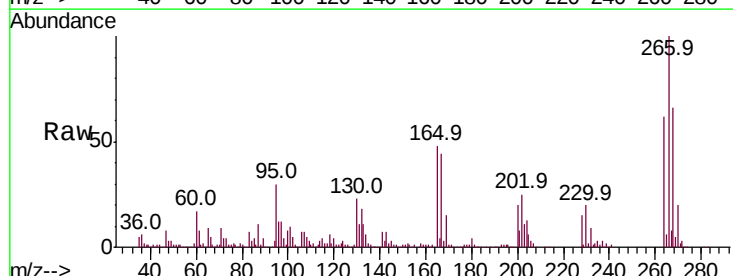

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

