

#15

N-Nitroso-di-n-propylamine

Concen: 34.856 ng/ul

RT: 8.25 min Scan# 980

Delta R.T. -0.01 min

Lab File: BN012617.D

Acq: 19 Nov 2020 05:45

Instrument :

BNA_N

ClientSampled :

Tot Ion: 70 Resp: 248348


Ion	Ratio	Lower	Upper
70	100		
42	63.1	50.0	75.0
101	9.7	7.5	11.3
130	20.5	17.6	26.4

70 100

42 63.1 50.0 75.0

101 9.7 7.5 11.3

130 20.5 17.6 26.4

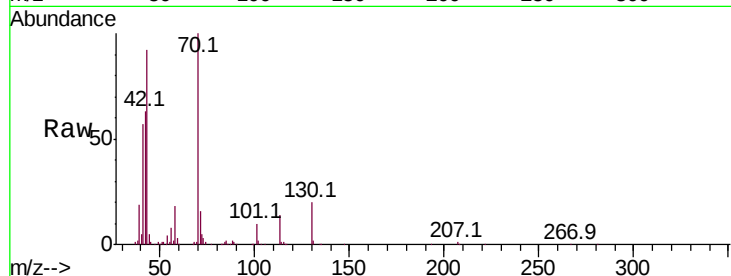




Abundance

Ion 70.00 (69.70 to 70.70): BN012596.D (-974) (-)

Ion 42.00 (41.70 to 42.70): BN012596.D (-974) (-)

Ion 101.00 (100.70 to 101.70): BN012596.D (-974) (-)

Ion 130.00 (129.70 to 130.70): BN012596.D (-974) (-)

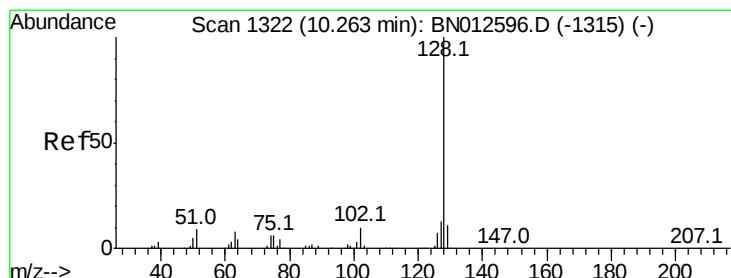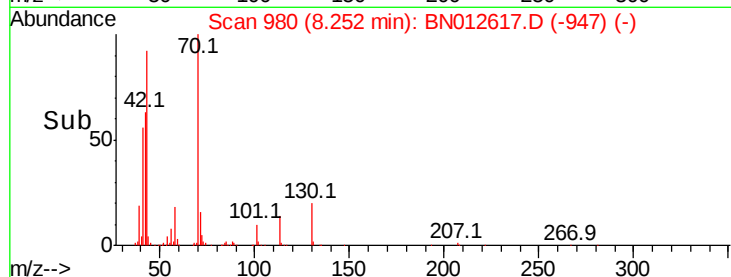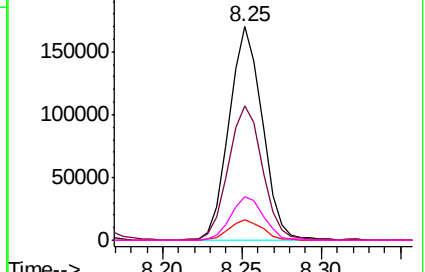

#28

Naphthalene

Concen: 277.567 ng/ul

RT: 10.27 min Scan# 1323

Delta R.T. 0.01 min

Lab File: BN012617.D

Acq: 19 Nov 2020 05:45


Tgt Ion: 128 Resp: 8463941

Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.6	12.8
127	13.2	11.6	17.4

128 100

129 10.9 8.6 12.8

127 13.2 11.6 17.4

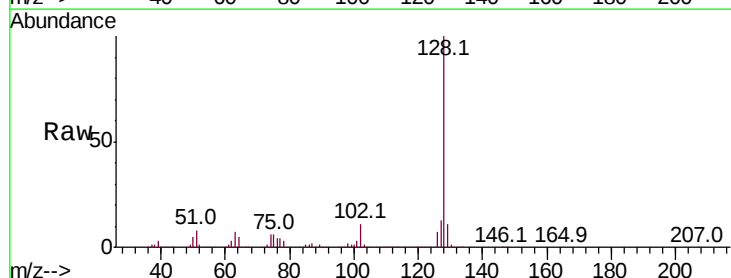

Abundance

Ion 128.00 (127.70 to 128.70): BN012596.D (-1315) (-)

Ion 129.00 (128.70 to 129.70): BN012596.D (-1315) (-)

Ion 127.00 (126.70 to 127.70): BN012596.D (-1315) (-)

