
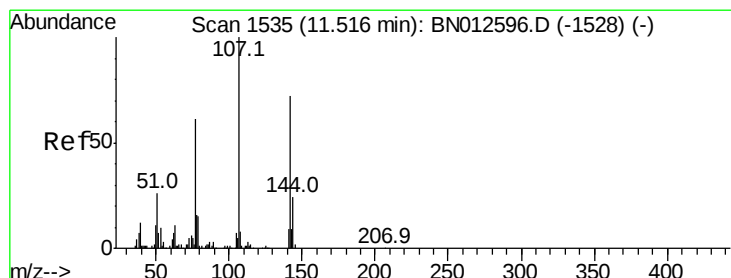
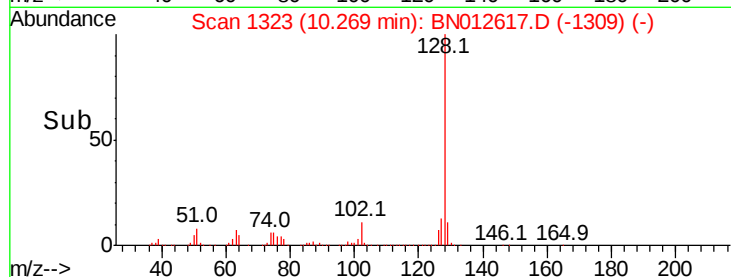
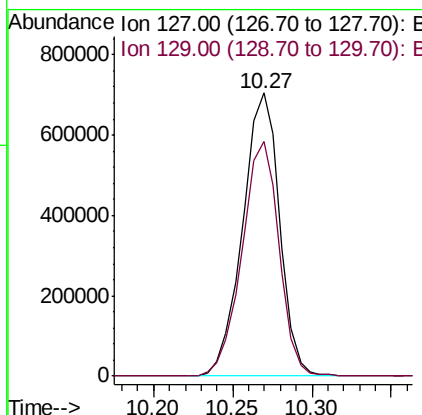


#30
 4-Chloroaniline
 Concen: 131.569 ng/ul
 RT: 10.27 min Scan# 1323
 Delta R.T. -0.12 min
 Lab File: BN012617.D
 Acq: 19 Nov 2020 05:45

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:127 Resp: 1143415
 Ion Ratio Lower Upper
 127 100
 129 82.9 25.5 38.3#

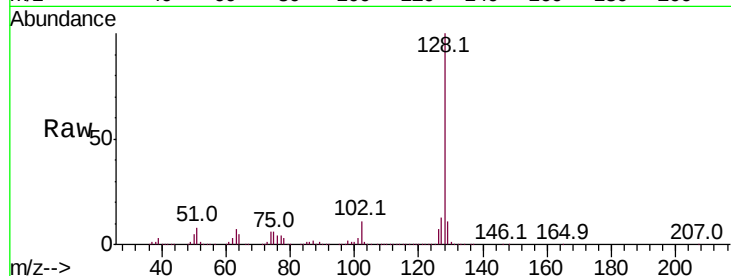

#33
 4-Chloro-3-methylphenol
 Concen: 28.416 ng/ul
 RT: 11.51 min Scan# 1534
 Delta R.T. -0.01 min
 Lab File: BN012617.D
 Acq: 19 Nov 2020 05:45

Tgt Ion:107 Resp: 289927
 Ion Ratio Lower Upper
 107 100
 144 24.6 20.0 30.0
 142 75.3 60.2 90.4

