
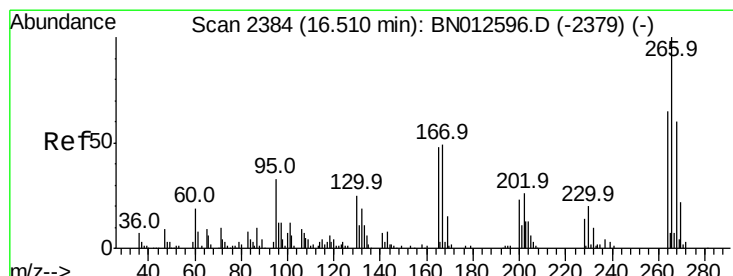
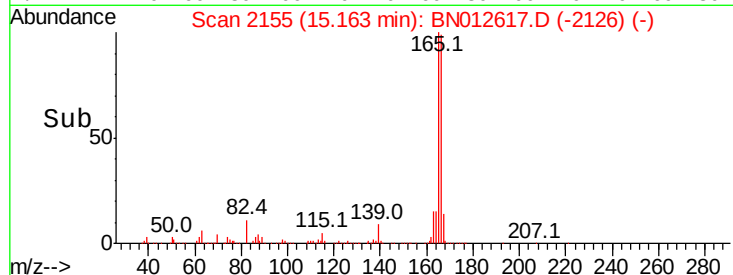
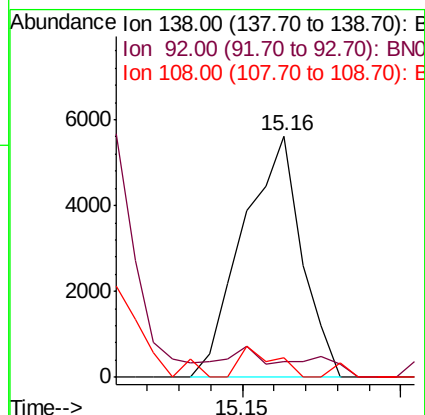


#61
4-Nitroaniline
Concen: 1.261 ng/ul
RT: 15.16 min Scan# 2155
Delta R.T. -0.03 min
Lab File: BN012617.D
Acq: 19 Nov 2020 05:45

Instrument :
BNA_N
ClientSampleId :

Tot Ion:138 Resp: 7235
Ion Ratio Lower Upper
138 100
92 6.3 47.0 70.4#
108 8.0 79.8 119.6#

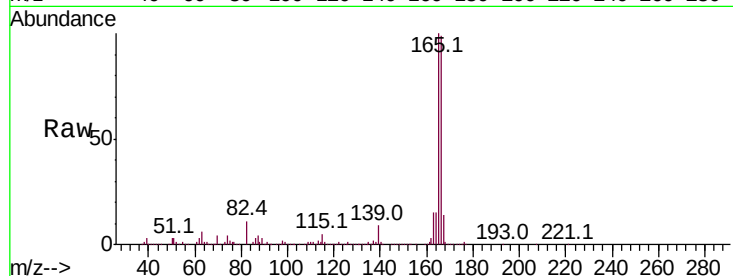

#69
Pentachlorophenol
Concen: 39.264 ng/ul
RT: 16.51 min Scan# 2384
Delta R.T. -0.01 min
Lab File: BN012617.D
Acq: 19 Nov 2020 05:45

Tgt Ion:266 Resp: 244681
Ion Ratio Lower Upper
266 100
264 56.6 55.0 82.6
268 60.7 56.9 85.3

