

#69

Pentachlorophenol

Concen: 2.386 ng/ul

RT: 16.51 min Scan# 2384

Delta R.T. -0.01 min

Lab File: BN012618.D

Acq: 19 Nov 2020 06:21

Instrument :

BNA_N

ClientSampleId :


Tot Ion:266 Resp: 21296

Ion Ratio Lower Upper

266 100

264 55.1 55.0 82.6




268 68.8 56.9 85.3

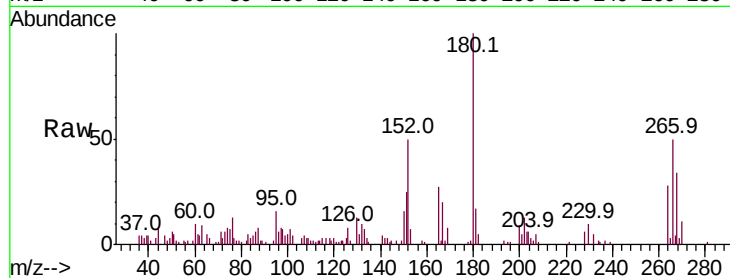

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

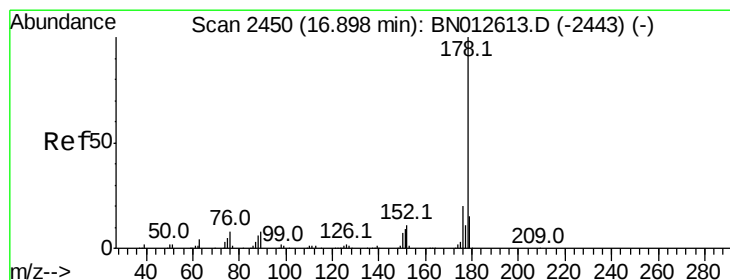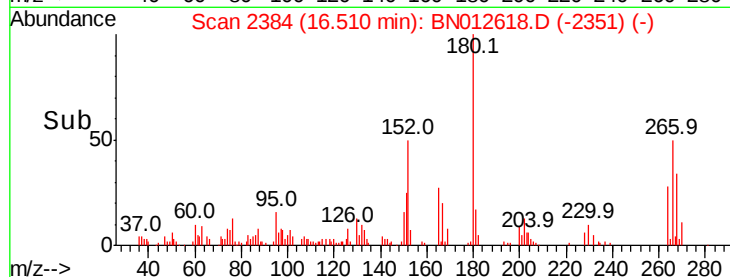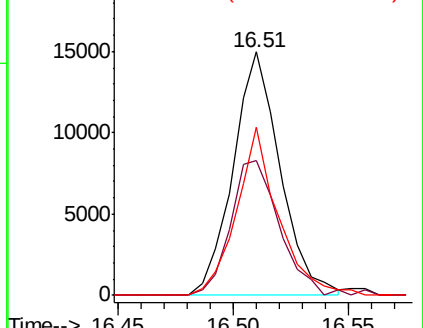

#70

Phenanthrene

Concen: 3.563 ng/ul

RT: 16.90 min Scan# 2450

Delta R.T. 0.00 min

Lab File: BN012618.D

Acq: 19 Nov 2020 06:21


Tgt Ion:178 Resp: 247574

Ion Ratio Lower Upper

178 100

179 14.8 13.1 19.7

176 20.1 15.4 23.0

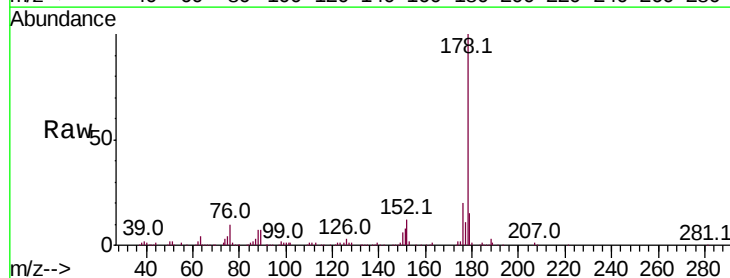

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

