


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111820\
Data File : BN012600.D
Acq On : 18 Nov 2020 18:54
Operator : CG/JU
Sample : L4726-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGF5

Manual Integrations
APPROVED

mohammad
11/20/2020 11:29:50 AM

Quant Time: Nov 19 04:23:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 18 14:31:59 2020
Response via : Initial Calibration

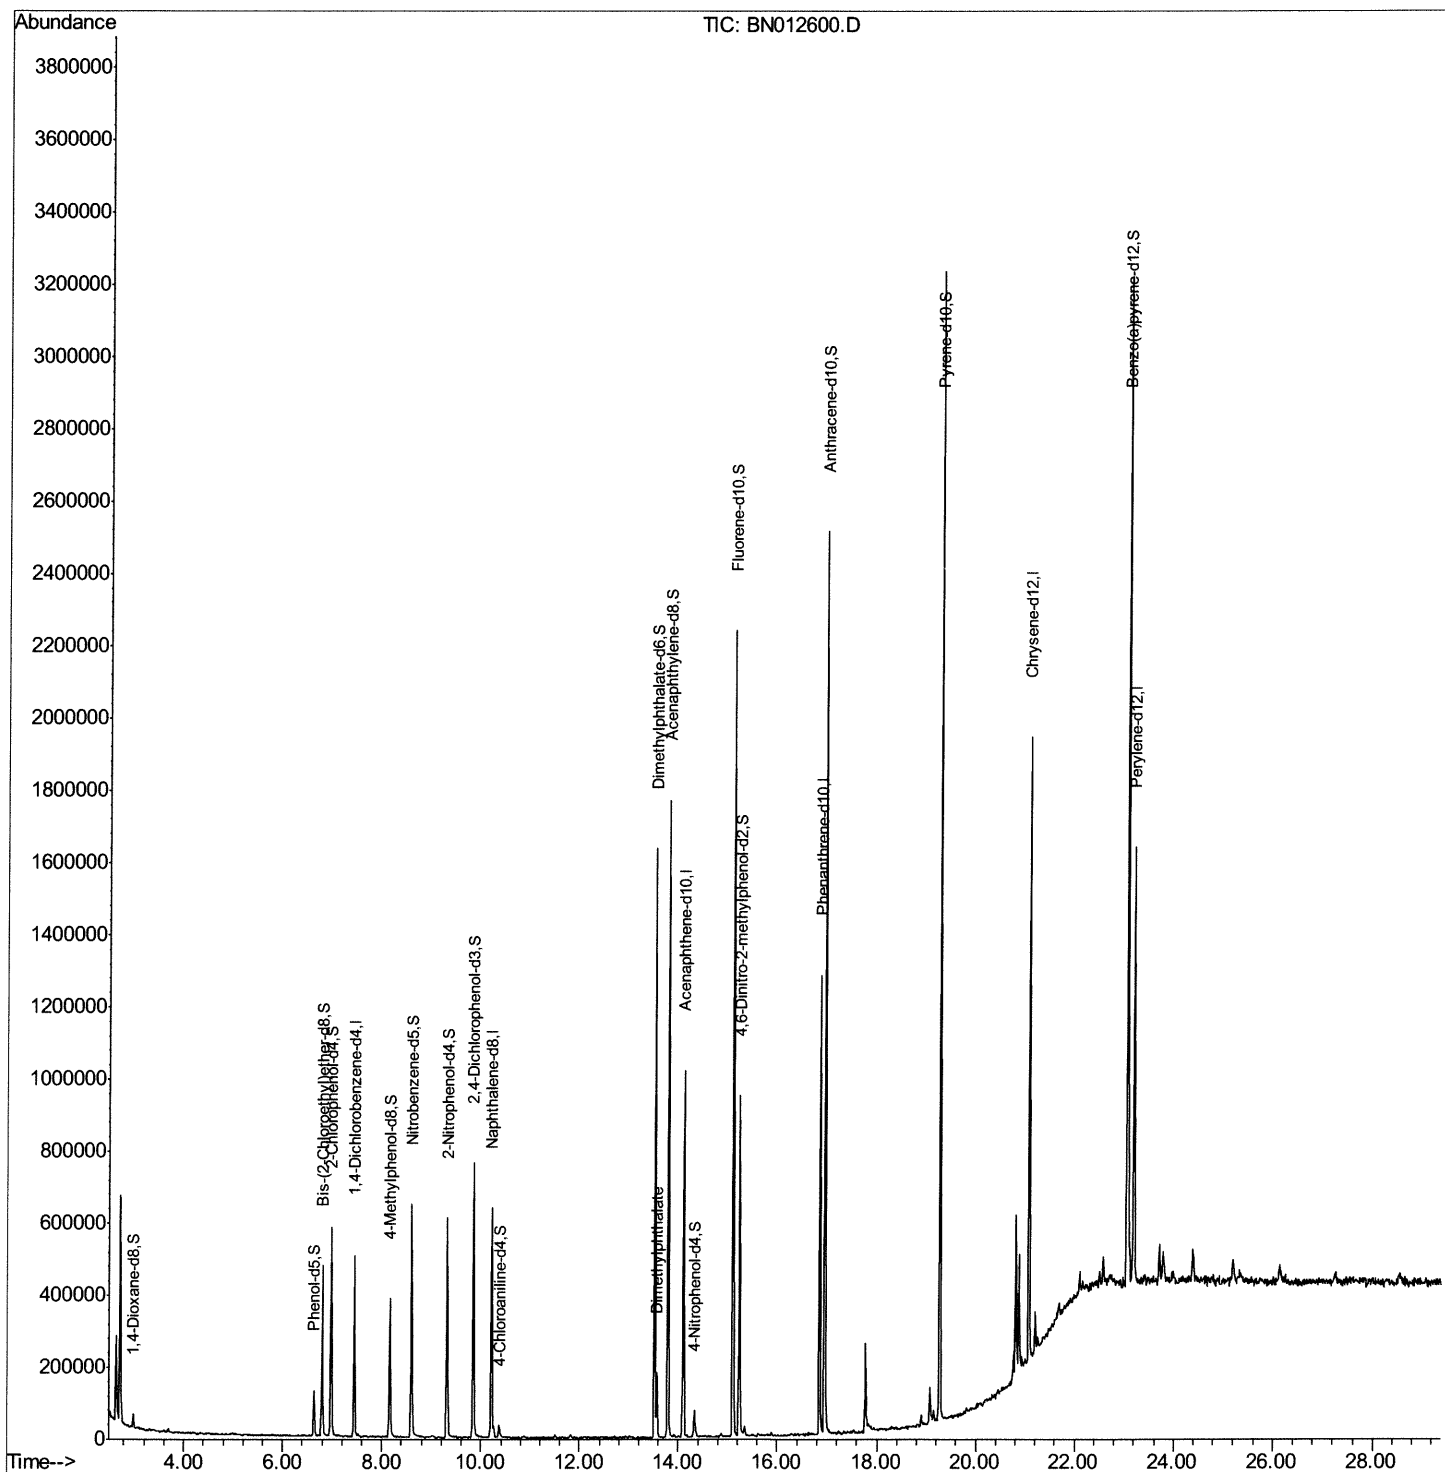

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111820\
 Data File : BN012600.D
 Acq On : 18 Nov 2020 18:54
 Operator : CG/JU
 Sample : L4726-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGF5

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:29:50 AM

Quant Time: Nov 19 03:45:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

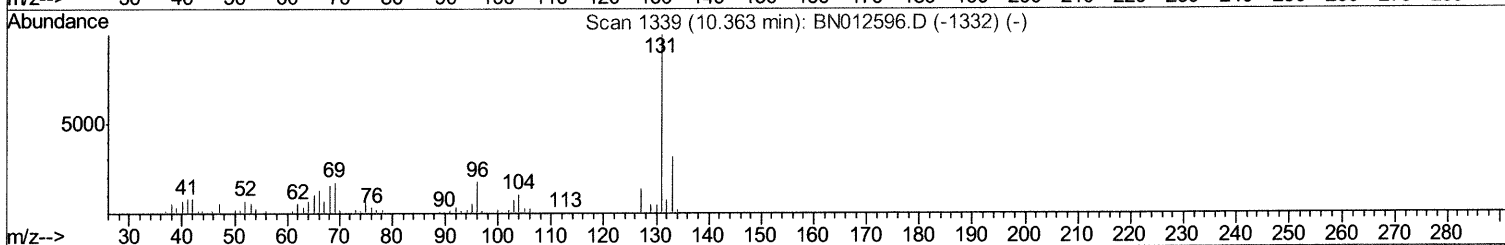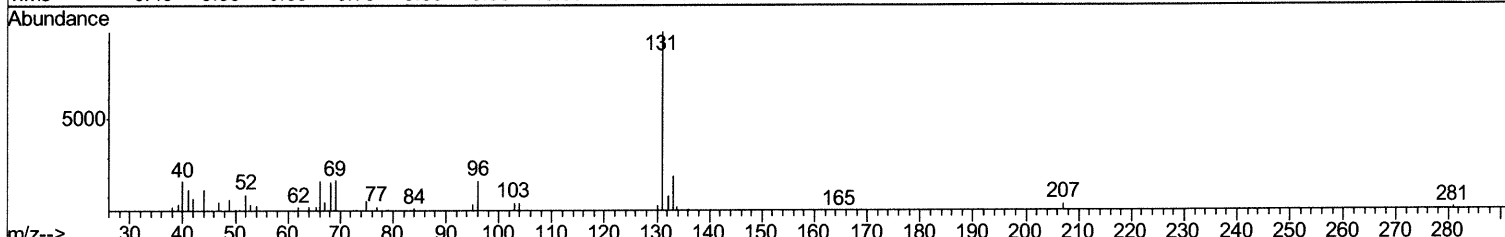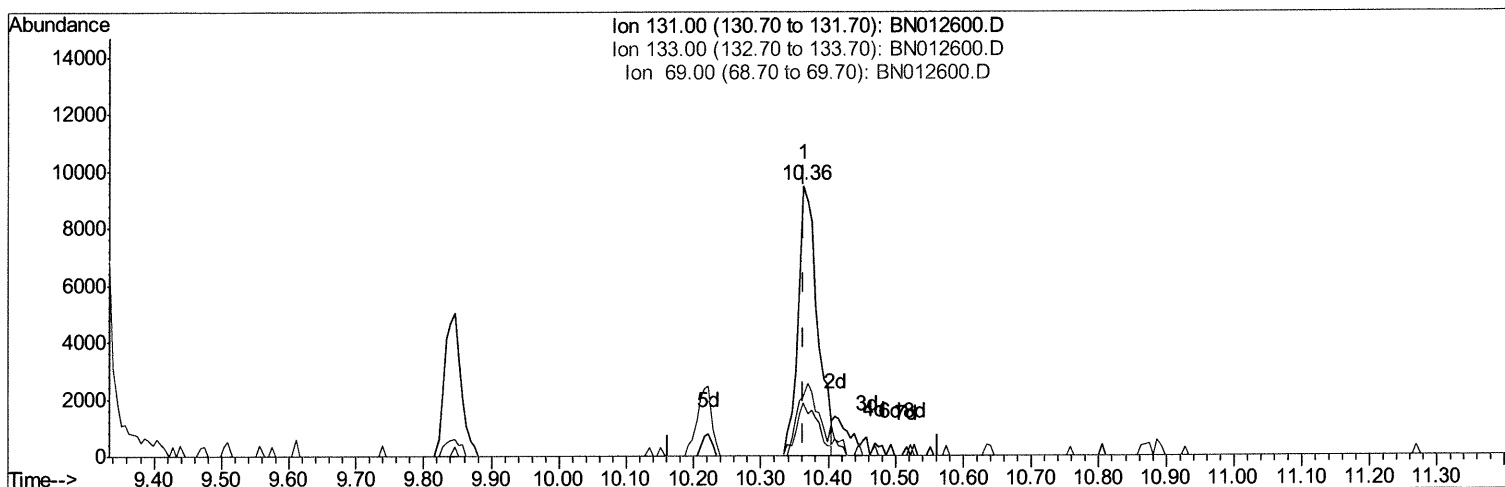

TIC: BN012600.D

(29) 4-Chloroaniline-d4 (S)

10.363min (+0.000) 2.29ng/ul

response 18871

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	22.01#
69.00	22.10	19.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
 Data File : BN012600.D
 Acq On : 18 Nov 2020 18:54
 Operator : CG/JU
 Sample : L4726-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGF5

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:29:50 AM

Quant Time: Nov 19 03:45:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

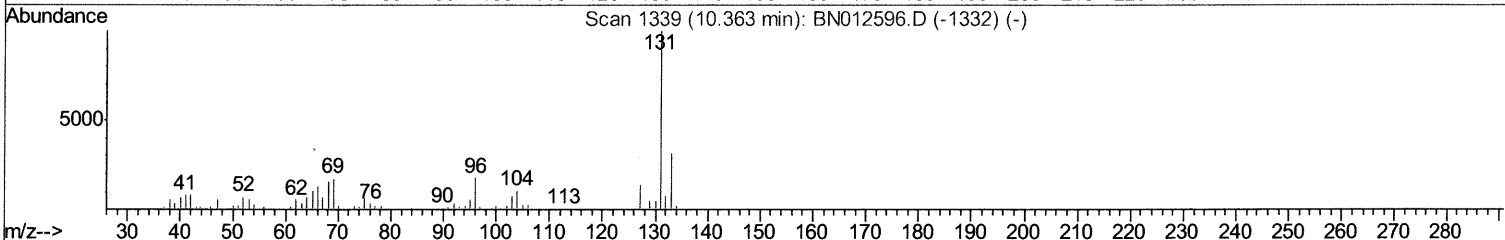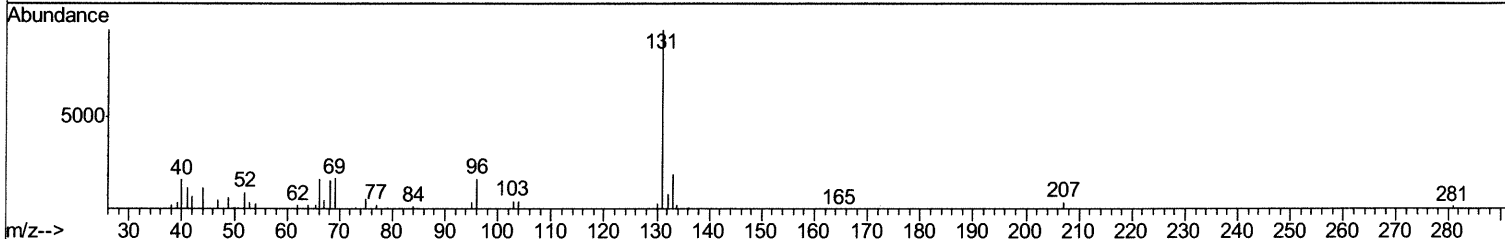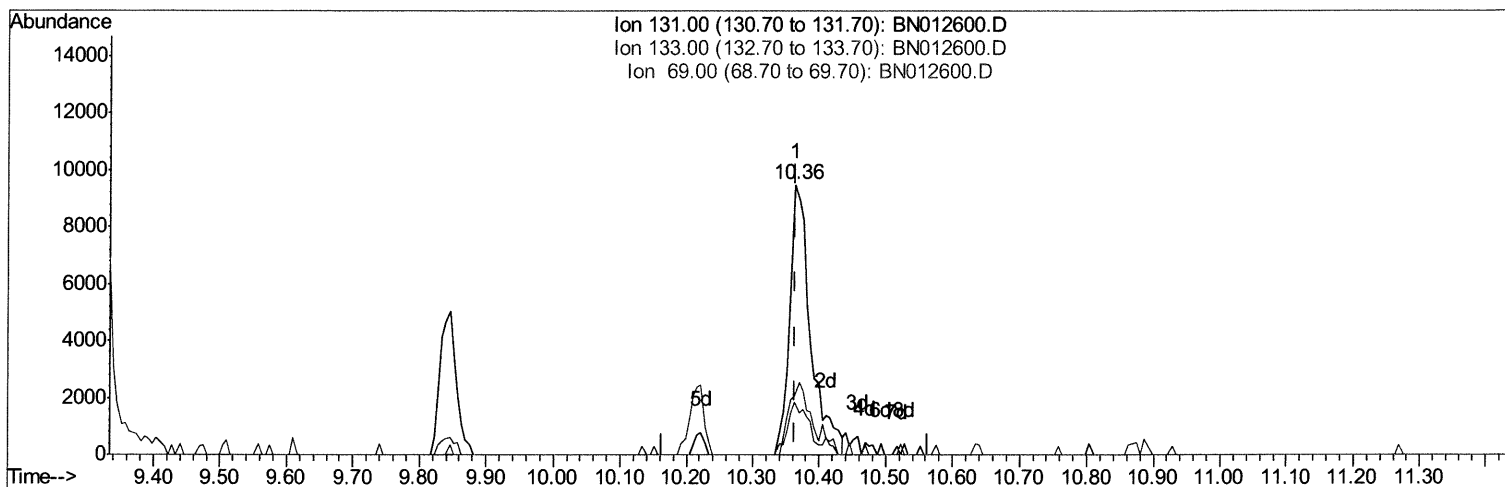

TIC: BN012600.D

(29) 4-Chloroaniline-d4 (S)

10.363min (+0.000) 2.51ng/ul m 12/02/2024

response 20655

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	22.01#
69.00	22.10	19.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
 Data File : BN012600.D
 Acq On : 18 Nov 2020 18:54
 Operator : CG/JU
 Sample : L4726-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGF5

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:29:50 AM

Quant Time: Nov 19 04:23:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	120476	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	481338	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	304165	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	659297	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	707723	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	783029	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	18199	5.38	ng/uL	0.00
5) Phenol-d5	6.63	99	60905	5.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	205174	31.78	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	211835	24.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	130015	14.52	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	130715	33.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	151564	34.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	252013	30.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	20655m	2.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	970357	39.06	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1100521	37.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	19220	4.13	ng/ul	0.00
58) Fluorene-d10	15.10	176	789267	36.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	151831	33.76	ng/ul	0.00
71) Anthracene-d10	16.96	188	1317912	39.35	ng/ul	0.00
79) Pyrene-d10	19.26	212	1484451	40.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	1738224	40.62	ng/ul	0.00

Target Compounds				Ovalue
45) Dimethylphthalate	13.57	163	97823	3.909 ng/ul# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed