

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111820\
 Data File : BN012623.D
 Acq On : 19 Nov 2020 09:21
 Operator : CG/JU
 Sample : L4753-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGG6

Quant Time: Nov 19 10:55:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	145980	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	568522	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	365618	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	772570	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	840334	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	911236	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	20321	4.96	ng/uL	0.00
5) Phenol-d5	6.63	99	75955	5.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	227014	29.02	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	237243	22.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	147774	13.62	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	142169	30.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	163124	31.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	259953	26.40	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	28294	2.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	1009277	33.80	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1198538	33.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	27091	4.85	ng/ul	0.00
58) Fluorene-d10	15.10	176	862004	32.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	174162	33.05	ng/ul	0.00
71) Anthracene-d10	16.95	188	1498628	38.18	ng/ul	0.00
79) Pyrene-d10	19.26	212	1703480	38.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2076159	41.69	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.57	163	30097	1.001	ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
Data File : BN012623.D
Acq On : 19 Nov 2020 09:21
Operator : CG/JU
Sample : L4753-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGG6

Quant Time: Nov 19 10:55:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 18 14:31:59 2020
Response via : Initial Calibration

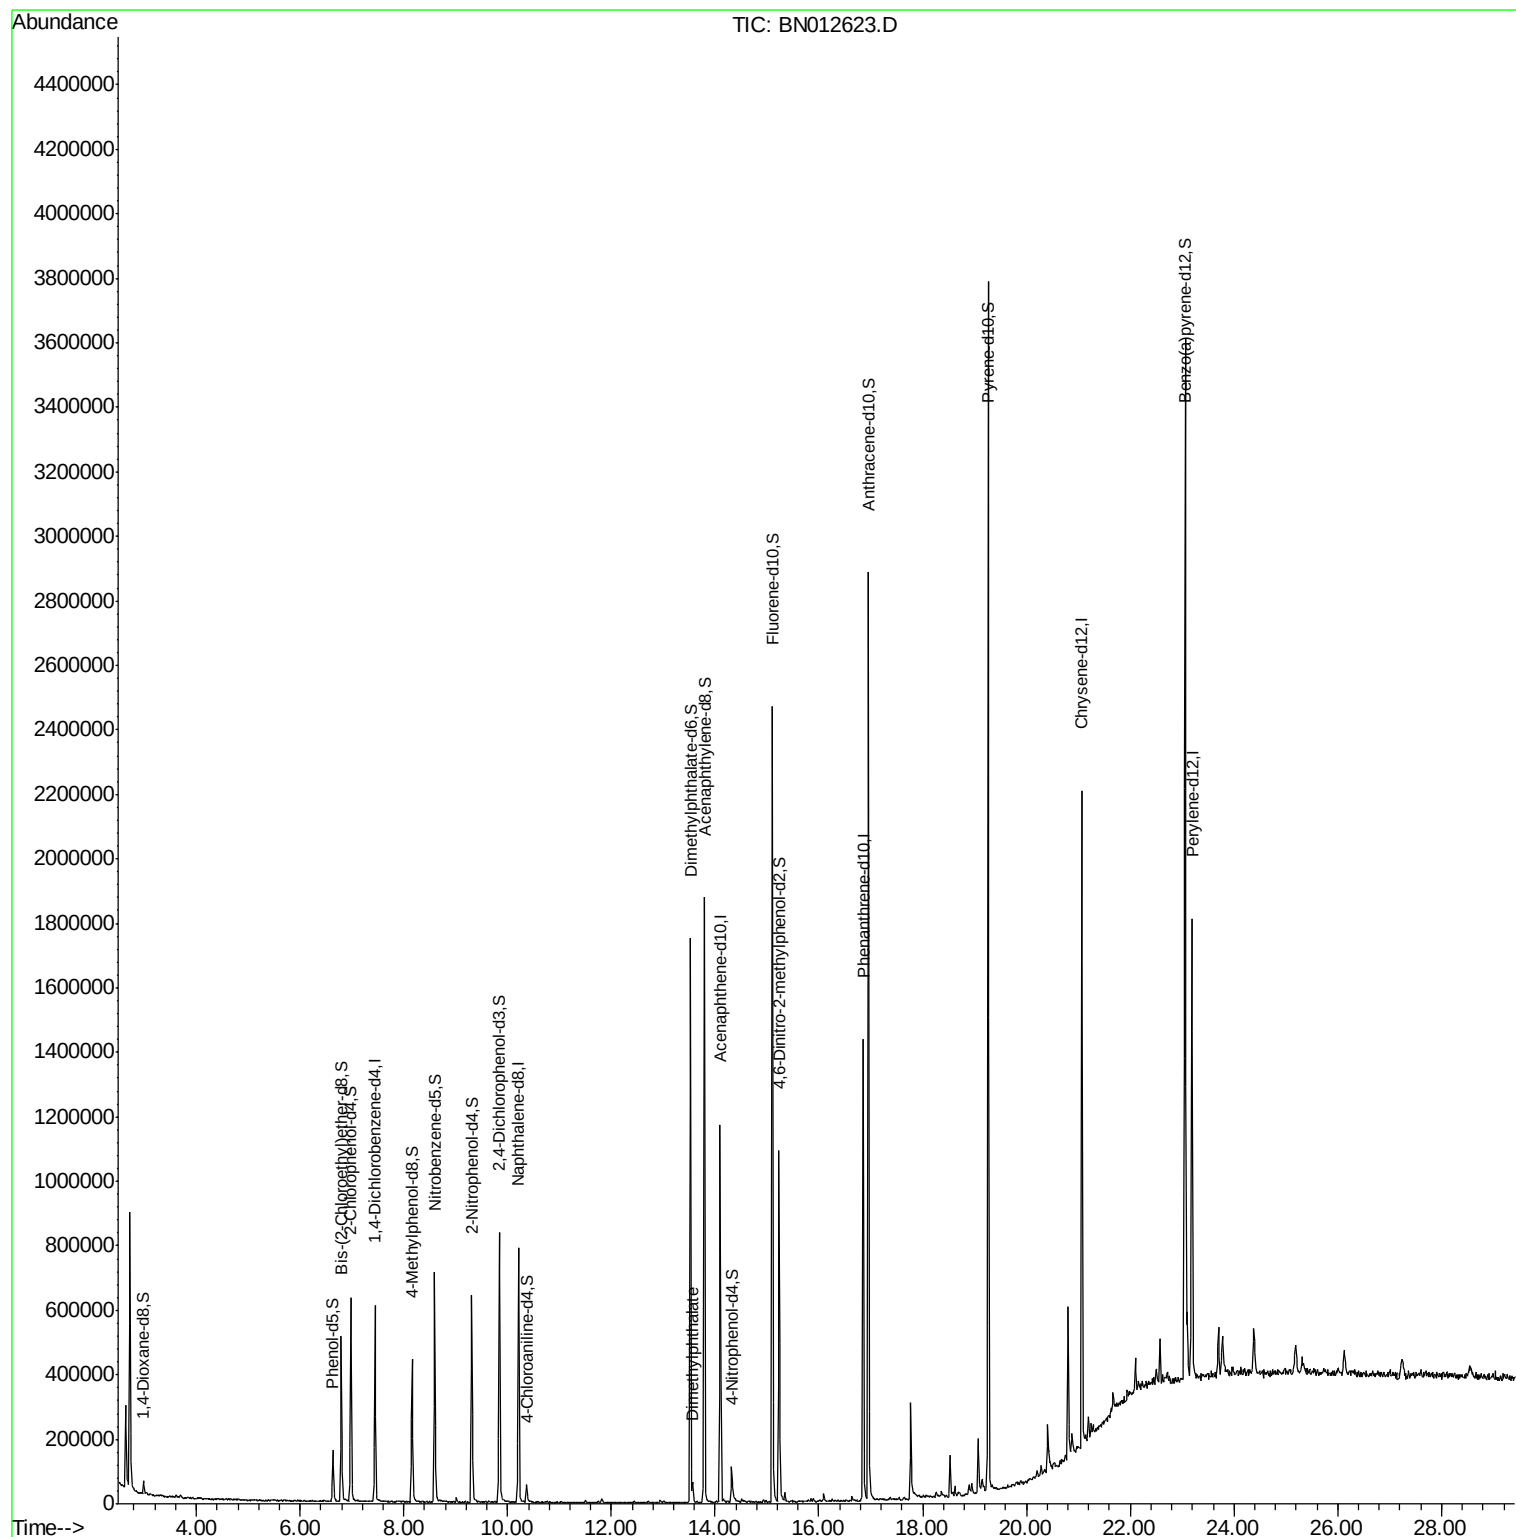

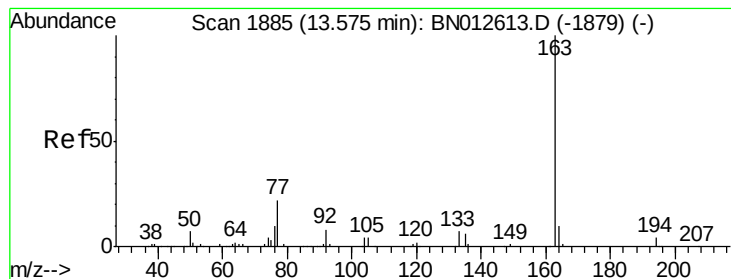

#45

Dimethylphthalate

Concen: 1.001 ng/ul

RT: 13.57 min Scan# 1884

Delta R.T. -0.01 min

Lab File: BN012623.D

Acq: 19 Nov 2020 09:21

Instrument :

BNA_N

ClientSampleId :

DBG6


Tot Ion:163 Resp: 30097

Ion Ratio Lower Upper

163 100

194 5.6 3.0 4.4#

164 10.4 8.6 13.0

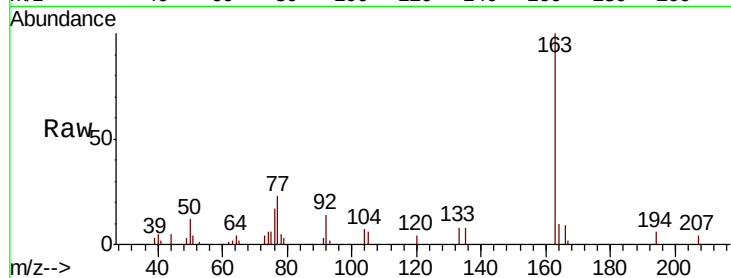

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

