

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
 Data File : BN012627.D
 Acq On : 19 Nov 2020 11:45
 Operator : CG/JU
 Sample : L4753-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGG7

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:30:46 AM

Quant Time: Nov 19 12:58:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	175166	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	698891	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	448527	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	961399	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1032335	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1179385	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	26113	5.31	ng/uL	0.00
5) Phenol-d5	6.63	99	84269	5.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	275554	29.35	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	289192	23.21	ng/ul	-0.01
13) 4-Methylphenol-d8	8.15	113	176406	13.55	ng/ul	-0.01
19) Nitrobenzene-d5	8.59	128	171585m	29.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	192157	30.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	309686	25.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	27063	2.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1199323	32.74	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1451884	33.21	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	26983	3.93	ng/ul	0.00
58) Fluorene-d10	15.10	176	998733	30.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	202074	30.81	ng/ul	0.00
71) Anthracene-d10	16.96	188	1726432	35.35	ng/ul	0.00
79) Pyrene-d10	19.26	212	1964764	36.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2425522	37.63	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.57	163	136853	3.709	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111820\
Data File : BN012627.D
Acq On : 19 Nov 2020 11:45
Operator : CG/JU
Sample : L4753-07
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampled :
DBGG7

Manual Integrations
APPROVED

mohammad
11/20/2020 11:30:46 AM

Quant Time: Nov 19 12:58:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 18 14:31:59 2020
Response via : Initial Calibration

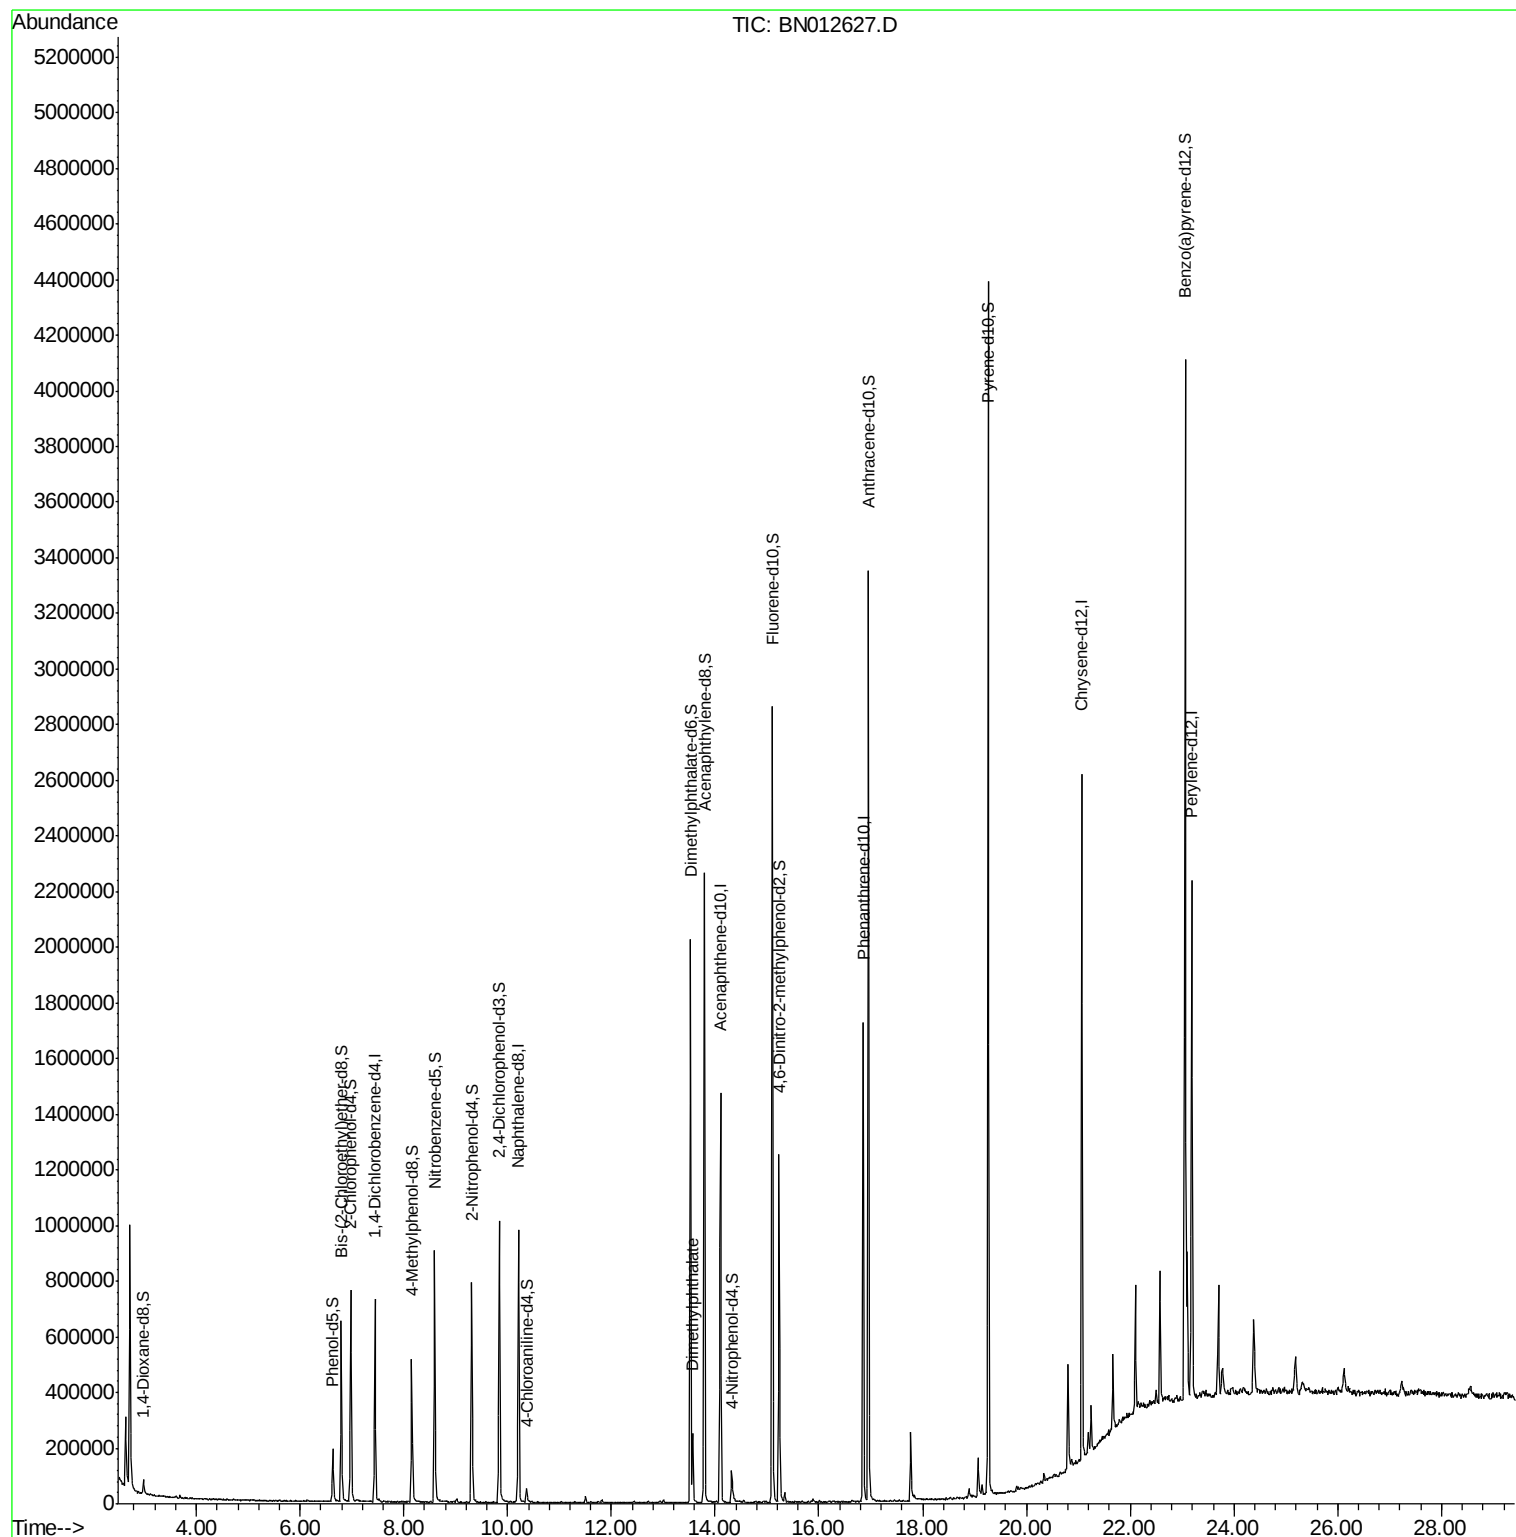

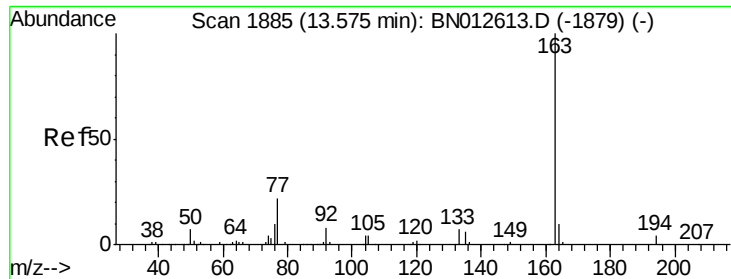


#45
 Dimethylphthalate
 Concen: 3.709 ng/ul
 RT: 13.57 min Scan# 1884
 Delta R.T. -0.01 min
 Lab File: BN012627.D
 Acq: 19 Nov 2020 11:45

Instrument :
 BNA_N
 ClientSampleId :
 DBGG7

Tot Ion:	163	Resp:	136853
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.0	4.4
164	9.5	8.6	13.0

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:30:46 AM

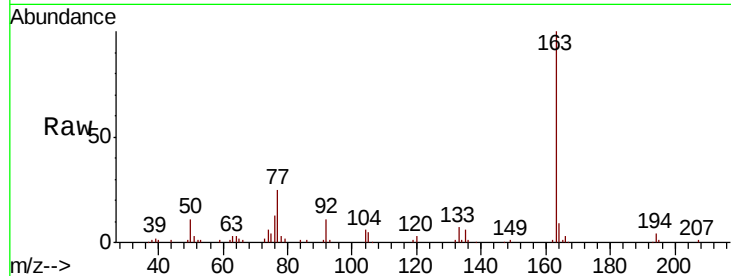

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

