

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
 Data File : BN012633.D
 Acq On : 19 Nov 2020 15:21
 Operator : CG/JU
 Sample : L4753-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGH3

Quant Time: Nov 19 15:52:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 14:31:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	149021	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	604578	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	396093	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	855266	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	905273	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1046194	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.98	96	21796	5.21	ng/uL	0.00
5) Phenol-d5	6.63	99	93214	6.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	275410	34.49	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	286125	26.99	ng/ul	-0.01
13) 4-Methylphenol-d8	8.16	113	180048	16.25	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	170877	34.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	197396	35.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	317117	30.29	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.36	131	32328	3.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	1251944	38.70	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1464190	37.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	34368	5.67	ng/ul	0.00
58) Fluorene-d10	15.10	176	1047621	36.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	220675	37.82	ng/ul	0.00
71) Anthracene-d10	16.95	188	1909289	43.94	ng/ul	0.00
79) Pyrene-d10	19.26	212	2159995	45.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2613269	45.71	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.57	163	248118	7.614	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
Data File : BN012633.D
Acq On : 19 Nov 2020 15:21
Operator : CG/JU
Sample : L4753-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGH3

Quant Time: Nov 19 15:52:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 18 14:31:59 2020
Response via : Initial Calibration

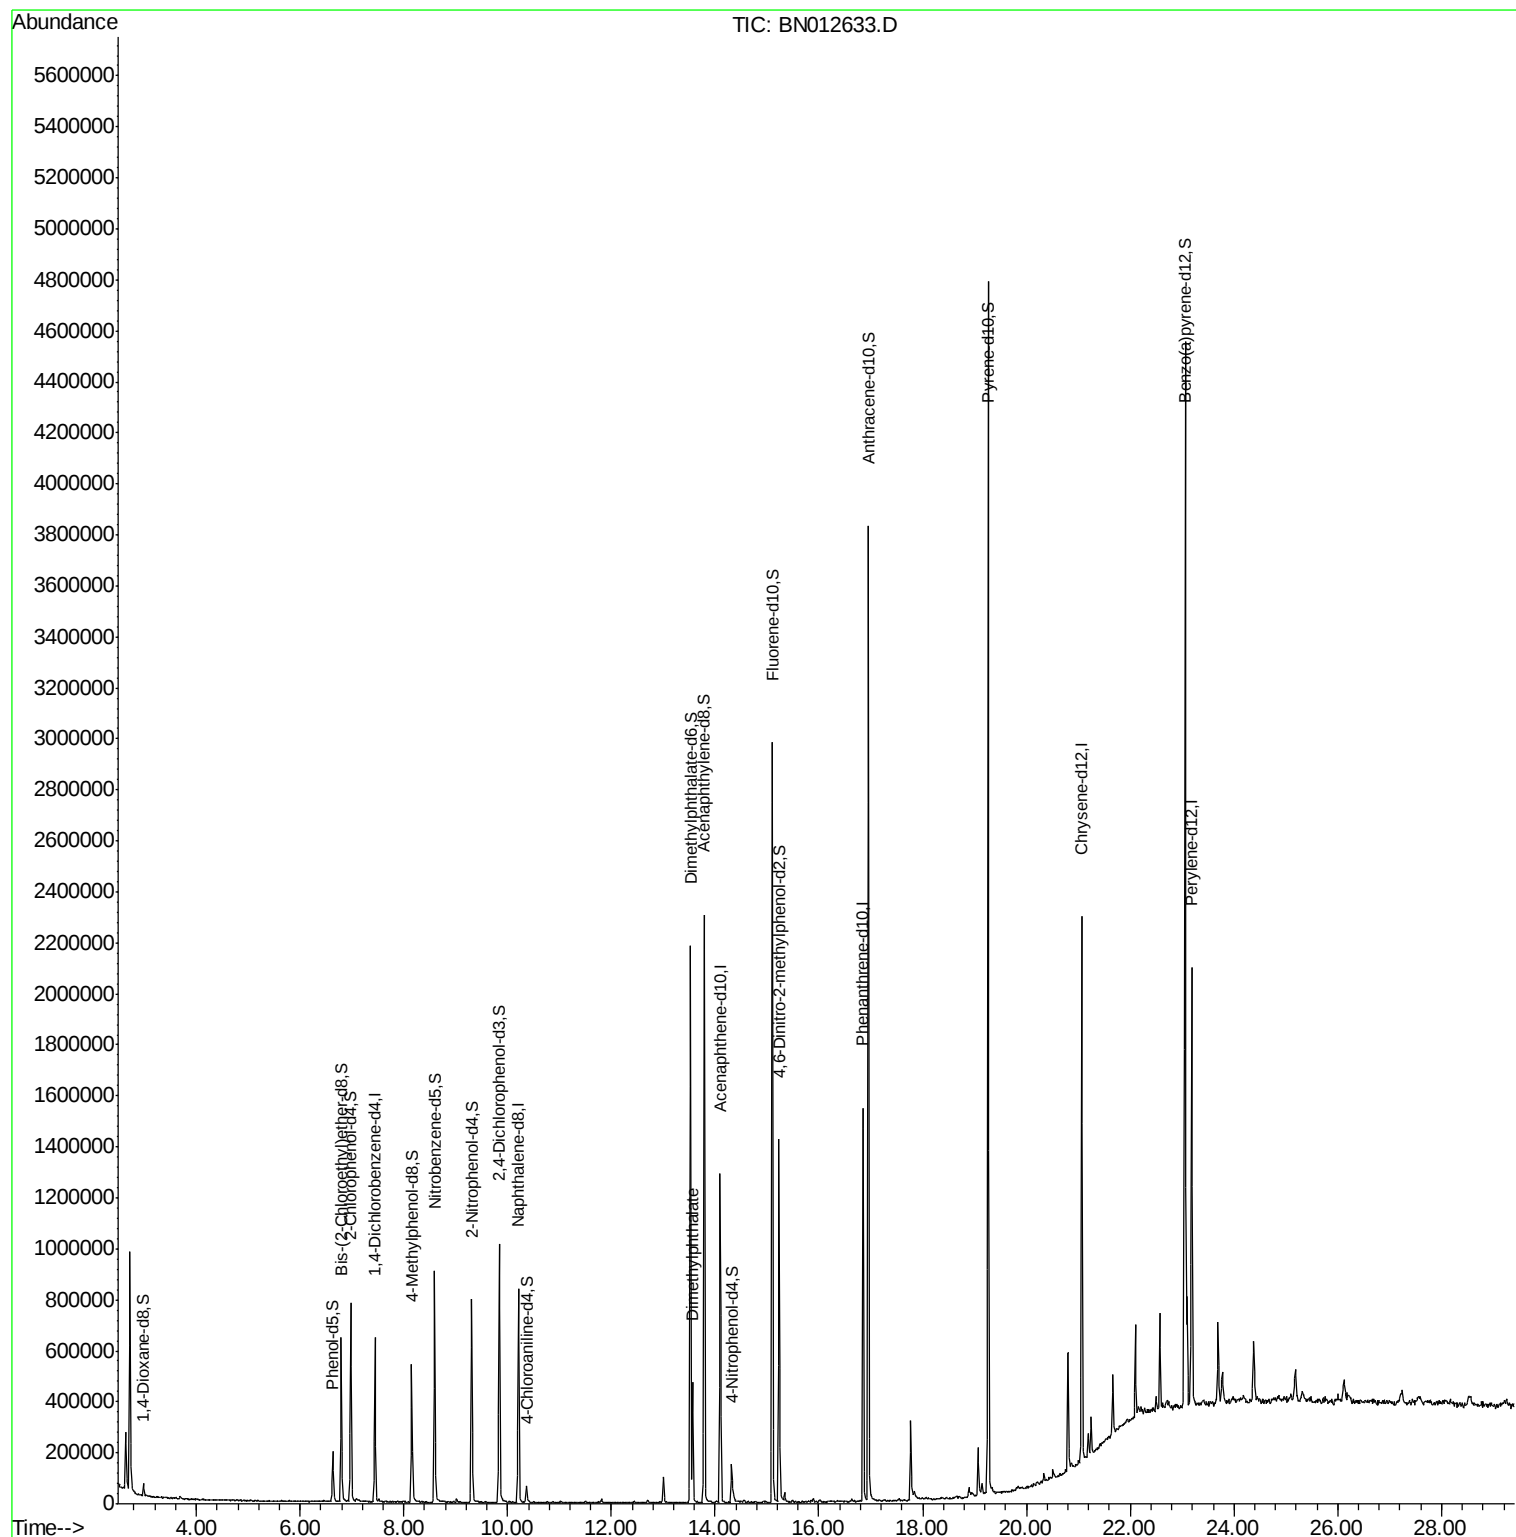

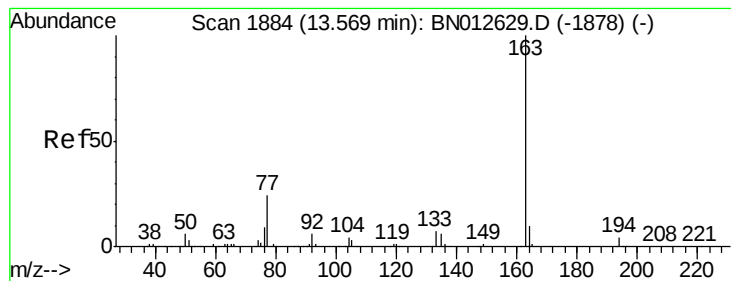

#45

Dimethylphthalate

Concen: 7.614 ng/ul

RT: 13.57 min Scan# 1884

Delta R.T. -0.01 min

Lab File: BN012633.D

Acq: 19 Nov 2020 15:21

Instrument :

BNA_N

ClientSampleId :

DBGH3

Tot Ion:163 Resp: 248118

Ion Ratio Lower Upper

163 100

194 3.6 3.0 4.4

164 10.5 8.6 13.0

