

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
 Data File : BN012641.D
 Acq On : 19 Nov 2020 20:08
 Operator : CG/JU
 Sample : L4726-08DL 2X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 DBGF3DL

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:31:11 AM

Quant Time: Nov 20 07:37:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 20 00:51:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	122776	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	480522	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	304980	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	706085	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	780738	20.00	ng/ul	-0.01
86) Perylene-d12	23.19	264	867669	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	2377	0.69	ng/uL	0.00
5) Phenol-d5	6.63	99	27530	2.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	89843	13.65	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	93420	10.70	ng/ul	-0.01
13) 4-Methylphenol-d8	8.15	113	54098	5.93	ng/ul	-0.01
19) Nitrobenzene-d5	8.59	128	54319m	13.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	57864	13.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	107457	12.91	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.52	166	440753	17.69	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	487139	16.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	10743m	2.30	ng/ul	0.00
58) Fluorene-d10	15.10	176	374587	17.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.23	200	64662	13.42	ng/ul	0.00
71) Anthracene-d10	16.95	188	636099	17.73	ng/ul	0.00
79) Pyrene-d10	19.26	212	763124	18.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.05	264	859019	18.12	ng/ul	-0.01

Target Compounds

					Ovalue	
28) Naphthalene	10.26	128	1141293	41.085	ng/ul	98
34) 2-Methylnaphthalene	11.88	142	43595	2.249	ng/ul	97
41) 1,1'-Biphenyl	12.92	154	33904	1.341	ng/ul	91
45) Dimethylphthalate	13.57	163	31306	1.248	ng/ul#	90
50) Acenaphthene	14.16	153	108160	4.974	ng/ul	98
54) Dibenzofuran	14.50	168	110367	3.661	ng/ul	95
56) 2,3,4,6-Tetrachlorophenol	14.73	232	5858	1.028	ng/ul#	82
59) Fluorene	15.16	166	44289	1.758	ng/ul	86
69) Pentachlorophenol	16.50	266	27853	4.995	ng/ul	90
75) Carbazole	17.26	167	597059	15.896	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111820\
Data File : BN012641.D
Acq On : 19 Nov 2020 20:08
Operator : CG/JU
Sample : L4726-08DL 2X
Misc :
ALS Vial : 50 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampled :
DBGF3DL

Quant Time: Nov 20 07:37:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 20 00:51:17 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
11/20/2020 11:31:11 AM

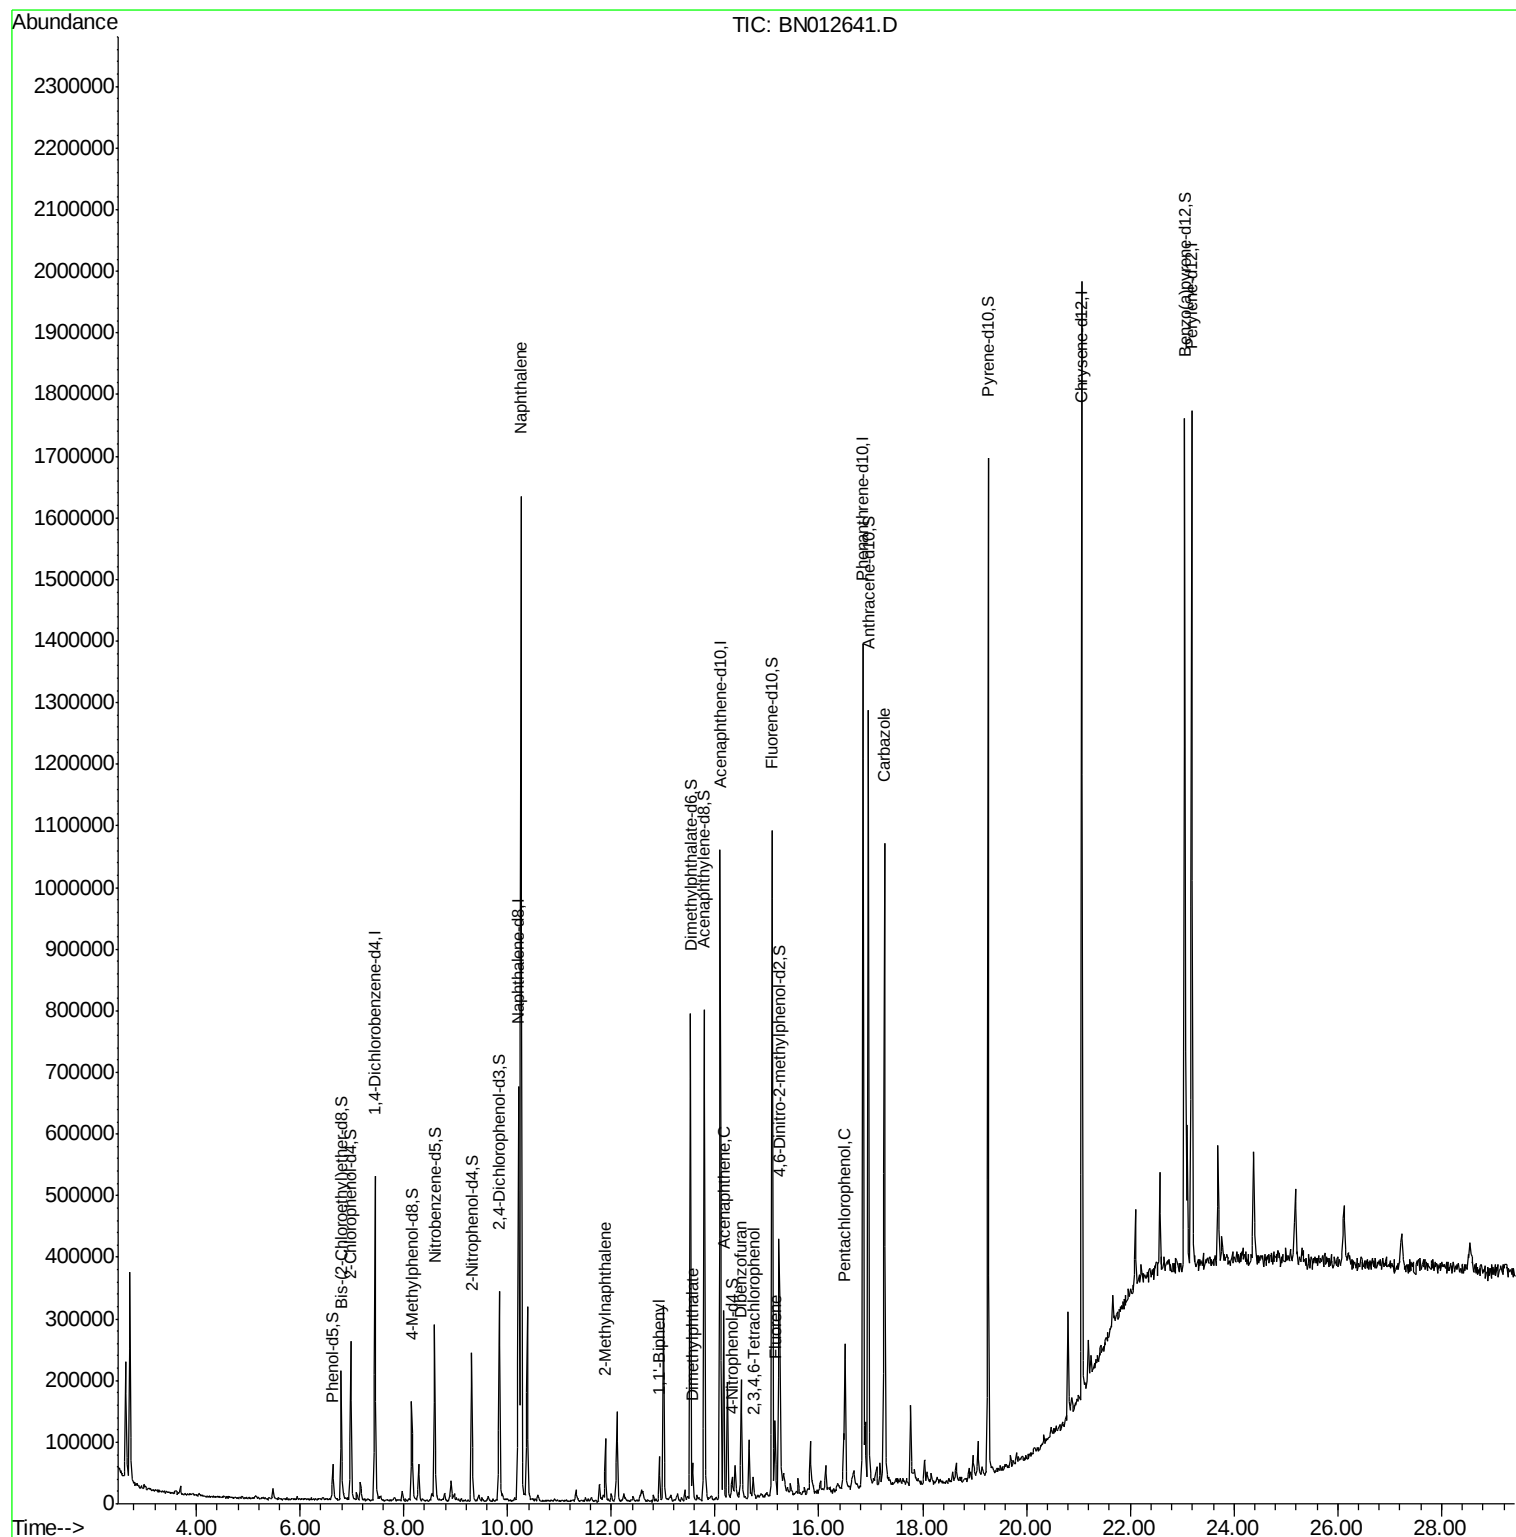







#28
Naphthalene
Concen: 41.085 ng/ul
RT: 10.26 min Scan# 1321
Delta R.T. -0.01 min
Lab File: BN012641.D
Acq: 19 Nov 2020 20:08

Instrument :
BNA_N
ClientSampleId :
DBGF3DL

Tot Ion	Ion	Ratio	Lower	Upper
128	100			
129	11.1	8.6	12.8	
127	13.7	11.6	17.4	




Manual Integrations
APPROVED


mohammad
11/20/2020 11:31:11 AM

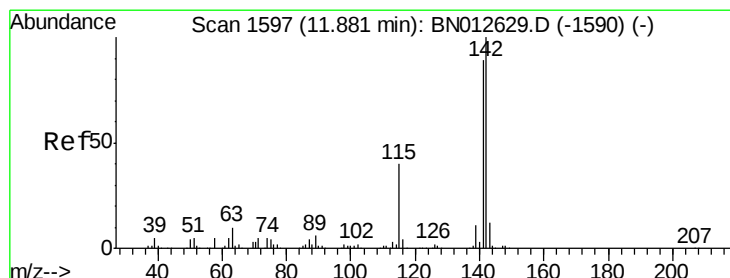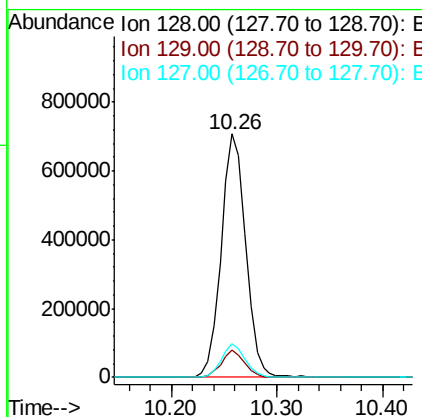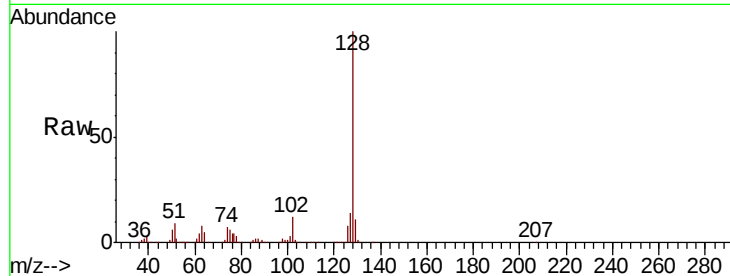

#34
2-Methylnaphthalene
Concen: 2.249 ng/ul
RT: 11.88 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BN012641.D
Acq: 19 Nov 2020 20:08

Tgt Ion	Ion	Ratio	Lower	Upper
142	100			
141	94.8	73.8	110.8	

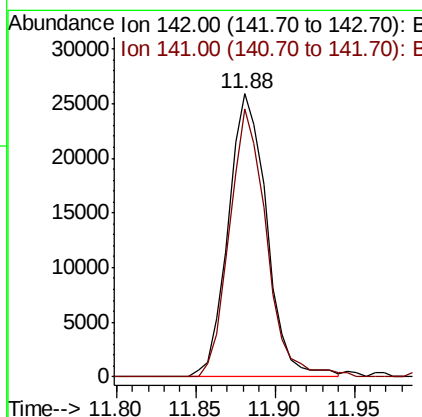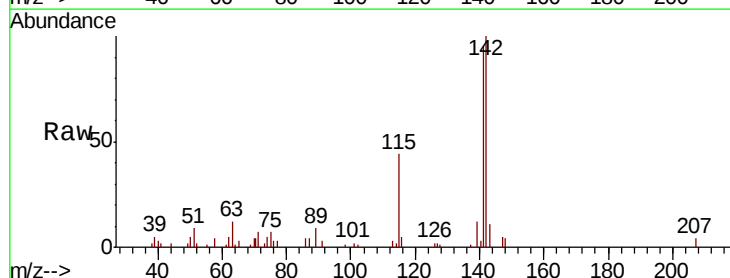

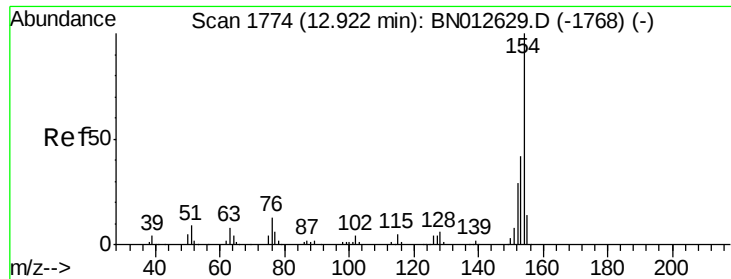





#41
 1,1'-Biphenyl
 Concen: 1.341 ng/ul
 RT: 12.92 min Scan# 1774
 Delta R.T. -0.01 min
 Lab File: BN012641.D
 Acq: 19 Nov 2020 20:08

Instrument :
 BNA_N
 ClientSampleID :
 DBGF3DL

Tot Ion	Ratio	Resp	Lower	Upper
154	100			
153	45.4	31.4	47.0	
76	9.8	9.3	13.9	




Manual Integrations
 APPROVED


mohammad
 11/20/2020 11:31:11 AM

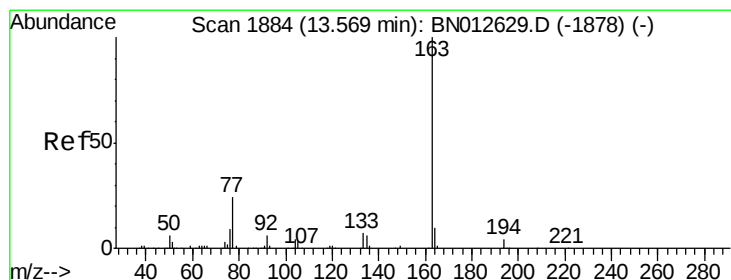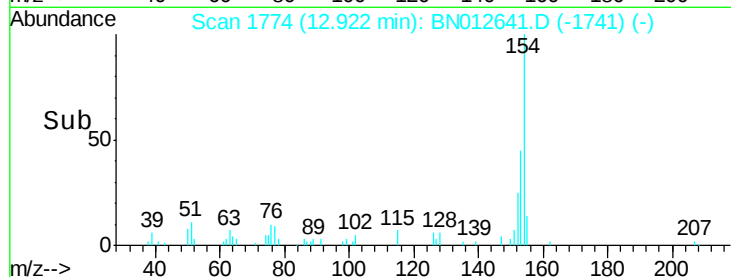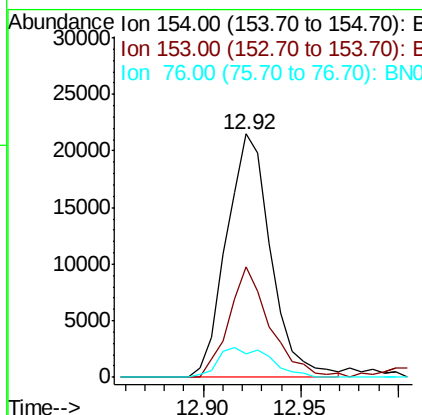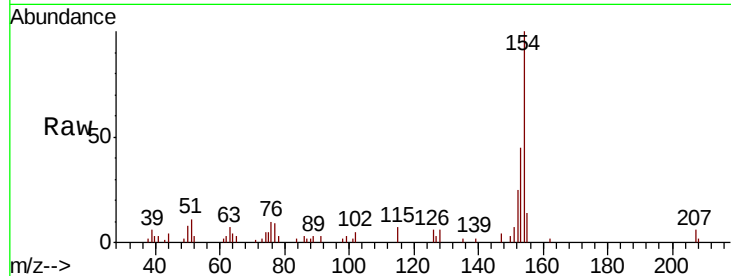

#45
 Dimethylphthalate
 Concen: 1.248 ng/ul
 RT: 13.57 min Scan# 1884
 Delta R.T. -0.01 min
 Lab File: BN012641.D
 Acq: 19 Nov 2020 20:08

Tgt Ion	Ratio	Resp	Lower	Upper
163	100			
194	7.0	3.0	4.4#	
164	7.1	8.6	13.0#	

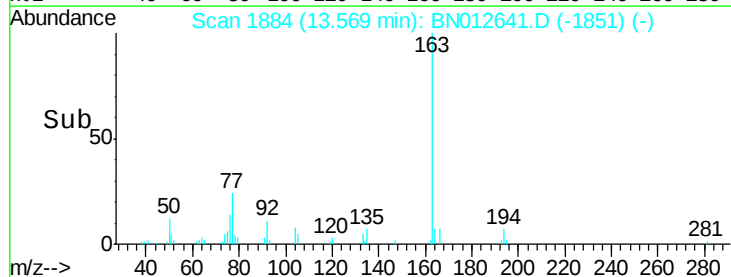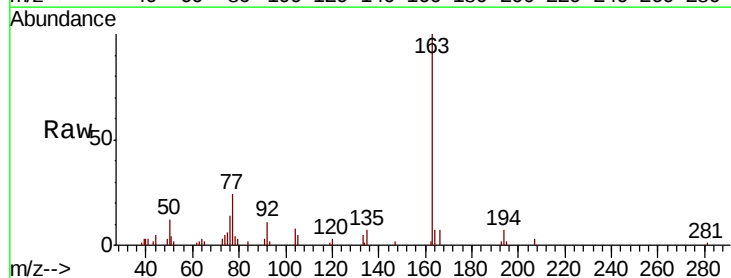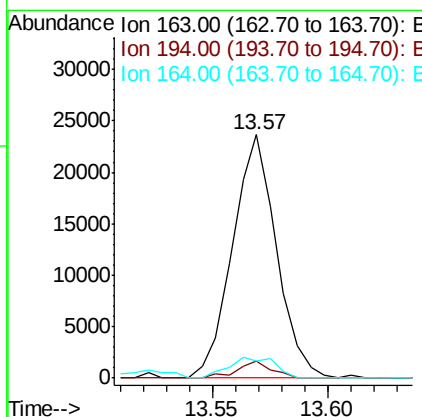



#50

Acenaphthene

Concen: 4.974 ng/ul

RT: 14.16 min Scan# 1985

Delta R.T. -0.01 min

Lab File: BN012641.D

Acq: 19 Nov 2020 20:08

Instrument :

BNA_N





ClientSampled :

DBGF3DL

Tot Ion:	153	Resp:	108160
Ion Ratio	Lower	Upper	
153	100		
152	46.8	37.1	55.7
154	84.6	69.7	104.5

Manual Integrations
APPROVED

mohammad
11/20/2020 11:31:11 AM

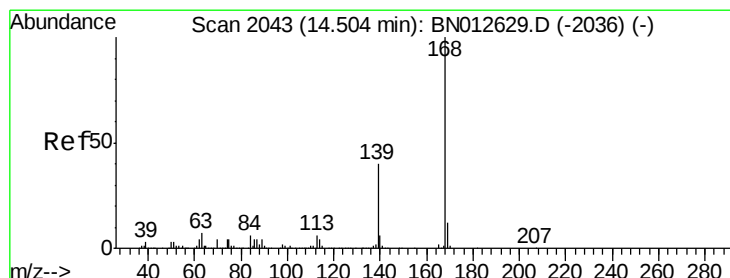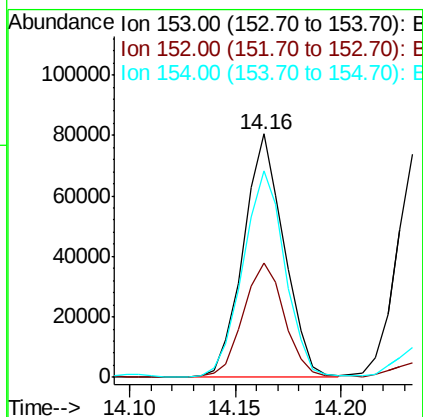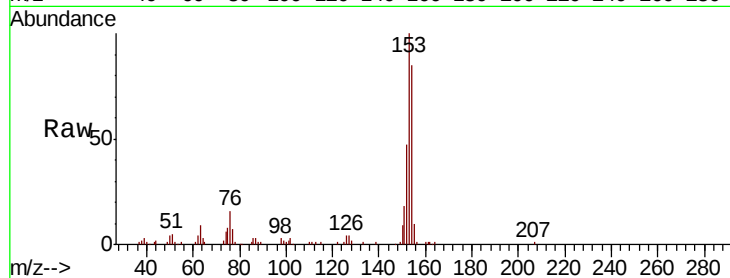

#54

Dibenzofuran

Concen: 3.661 ng/ul




RT: 14.50 min Scan# 2043


Delta R.T. -0.01 min

Lab File: BN012641.D

Acq: 19 Nov 2020 20:08

Tgt Ion:	168	Resp:	110367
Ion Ratio	Lower	Upper	
168	100		
139	41.1	30.5	45.7

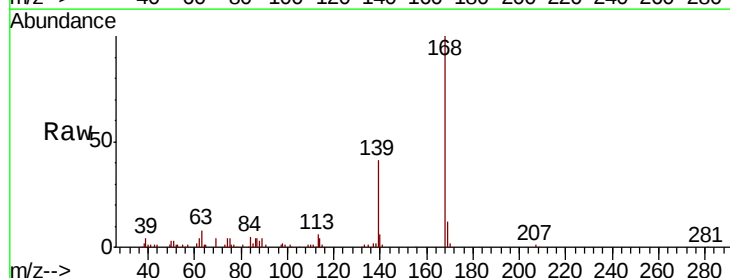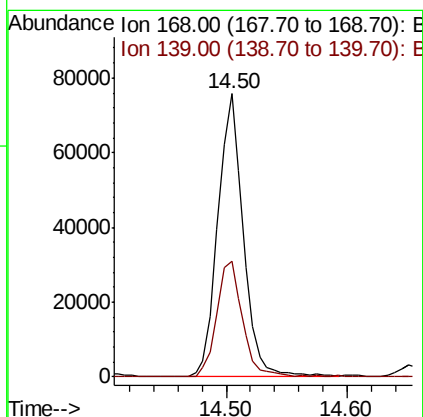







#56
2,3,4,6-Tetrachlorophenol
Concen: 1.028 ng/ul
RT: 14.73 min Scan# 2082
Delta R.T. -0.01 min
Lab File: BN012641.D
Acq: 19 Nov 2020 20:08

Instrument :
BNA_N
ClientSampleID :
DBGF3DL

Tot Ion	Ratio	Lower	Upper
232	100		
131	72.4	42.9	64.3#
130	0.0	2.5	3.7#
166	30.5	27.1	40.7




Manual Integrations
APPROVED


mohammad
11/20/2020 11:31:11 AM

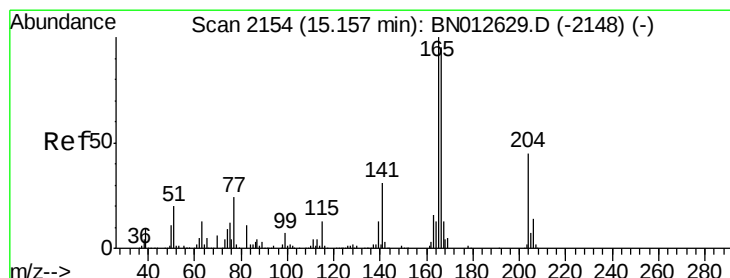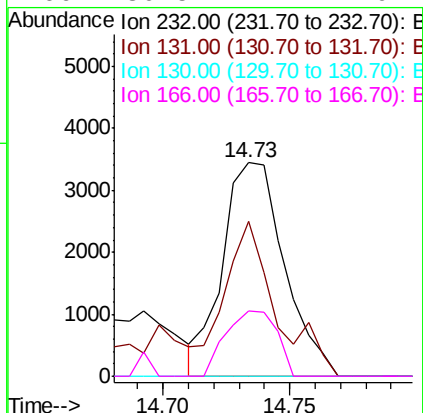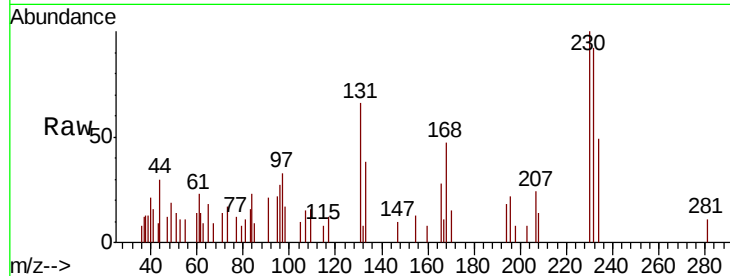

#59
Fluorene
Concen: 1.758 ng/ul
RT: 15.16 min Scan# 2154
Delta R.T. -0.01 min
Lab File: BN012641.D
Acq: 19 Nov 2020 20:08

Tgt Ion	Ratio	Lower	Upper
166	100		
165	88.3	83.3	124.9
167	14.8	11.0	16.6

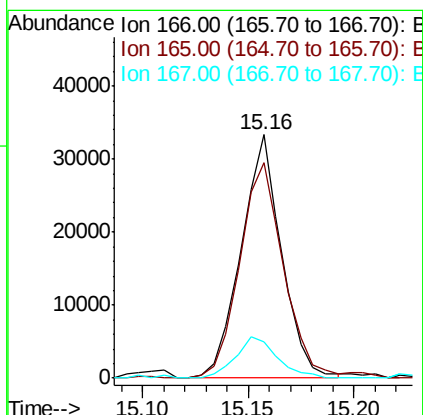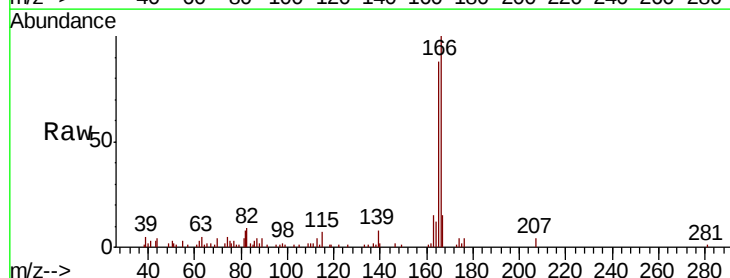







#69
 Pentachlorophenol
 Concen: 4.995 ng/ul
 RT: 16.50 min Scan# 2383
 Delta R.T. -0.01 min
 Lab File: BN012641.D
 Acq: 19 Nov 2020 20:08

Instrument :
 BNA_N
 ClientSampleID :
 DBGF3DL

Tot Ion	Ratio	Lower	Upper
266	100		
264	55.7	55.0	82.6
268	67.3	56.9	85.3

Manual Integrations
 APPROVED

mohammad
 11/20/2020 11:31:11 AM

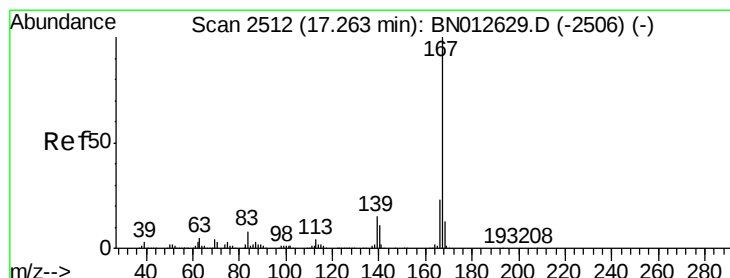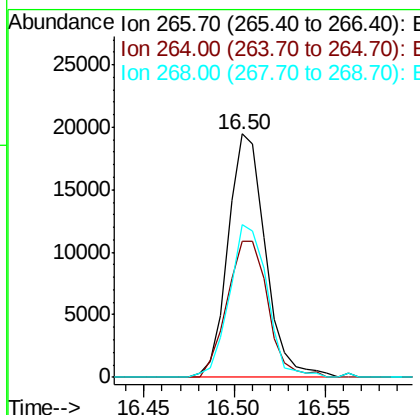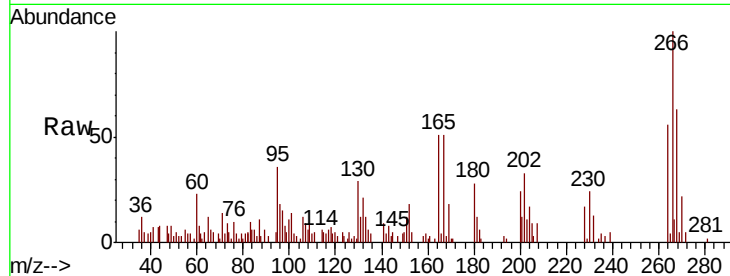

#75
 Carbazole
 Concen: 15.896 ng/ul
 RT: 17.26 min Scan# 2512
 Delta R.T. -0.01 min
 Lab File: BN012641.D
 Acq: 19 Nov 2020 20:08

Tgt Ion	Ratio	Lower	Upper
167	100		
166	22.0	17.8	26.8
139	14.4	10.4	15.6

