


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111919\
Data File : BN008631.D
Acq On : 19 Nov 2019 15:37
Operator : JU
Sample : PB124657BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK57

Manual Integrations
APPROVED

mohammad
11/21/2019 9:04:51 AM

Quant Time: Nov 19 16:20:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

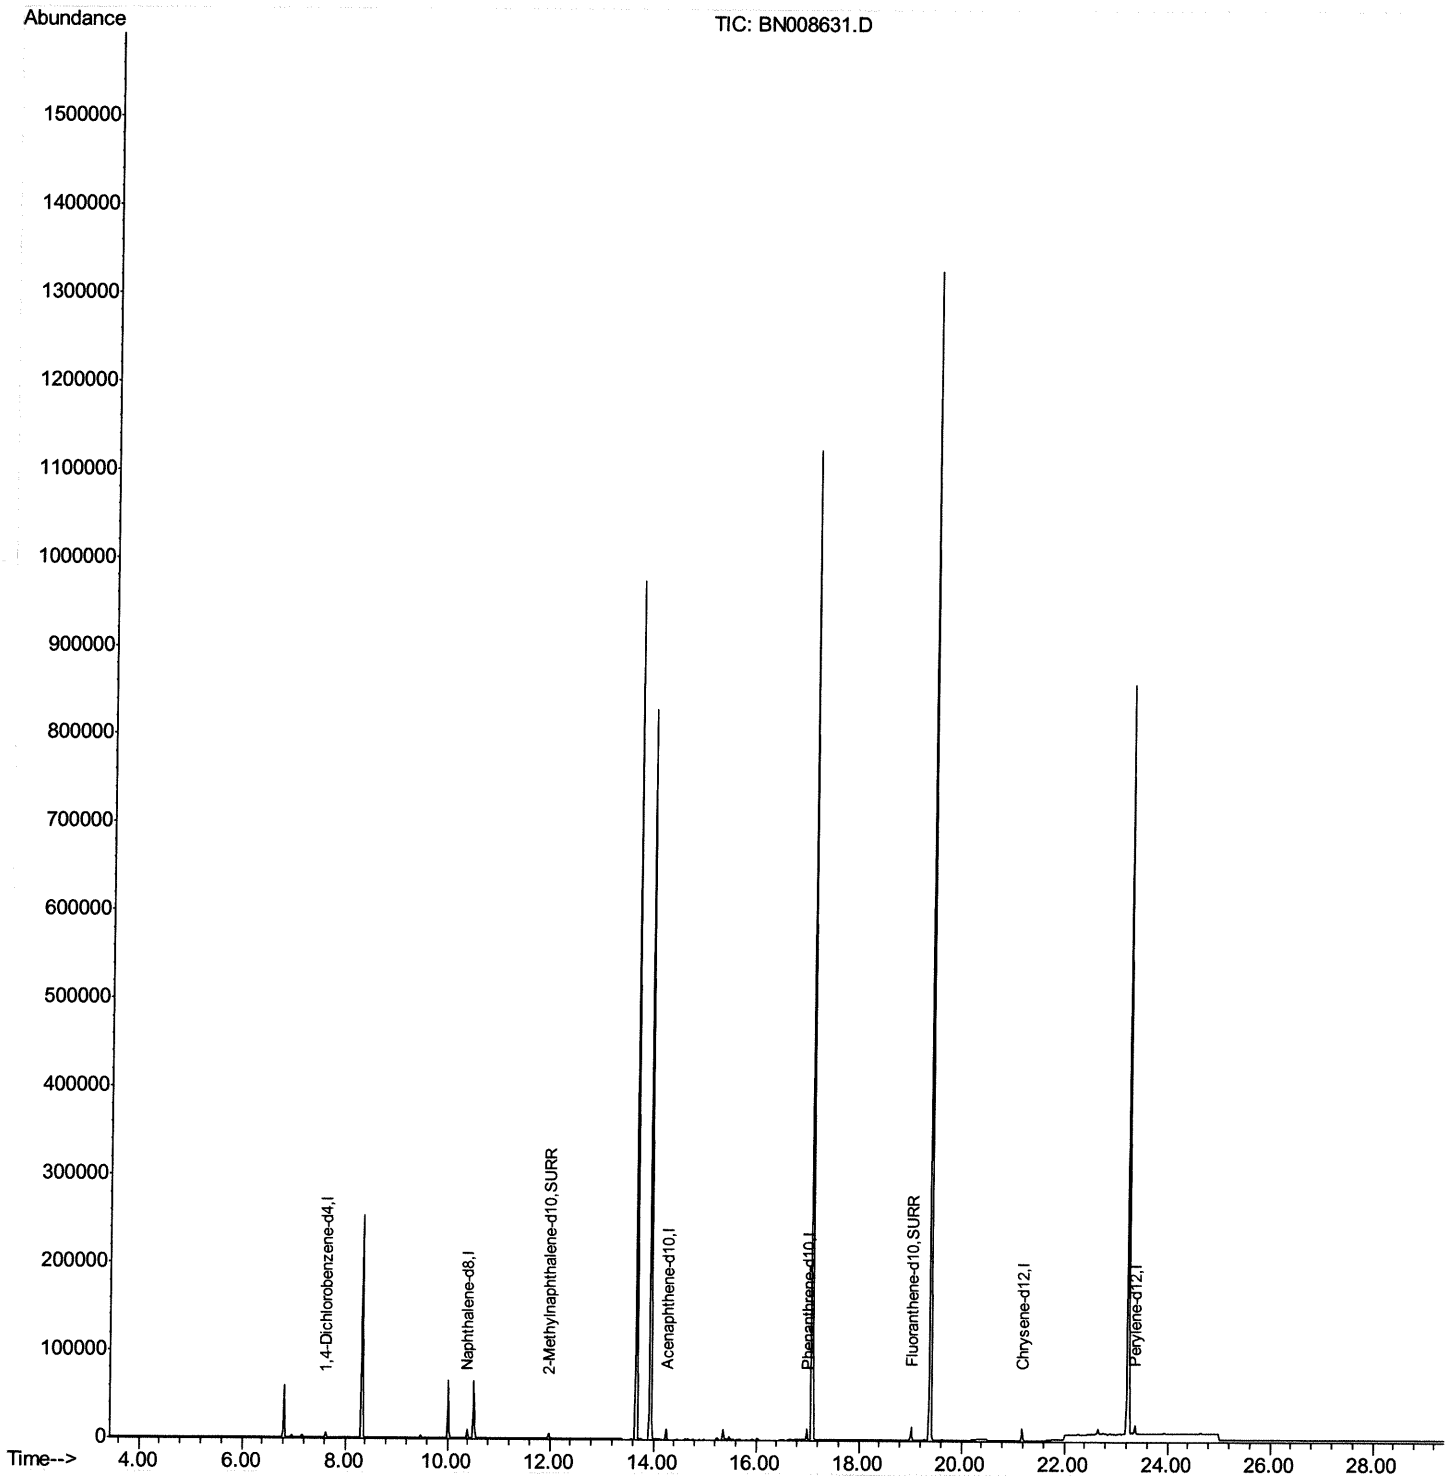

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111919\
 Data File : BN008631.D
 Acq On : 19 Nov 2019 15:37
 Operator : JU
 Sample : PB124657BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK57

Manual Integrations
 APPROVED

mohammad
 11/21/2019 9:04:51 AM

Quant Time: Nov 19 16:19:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 19 01:47:58 2019
 Response via : Initial Calibration

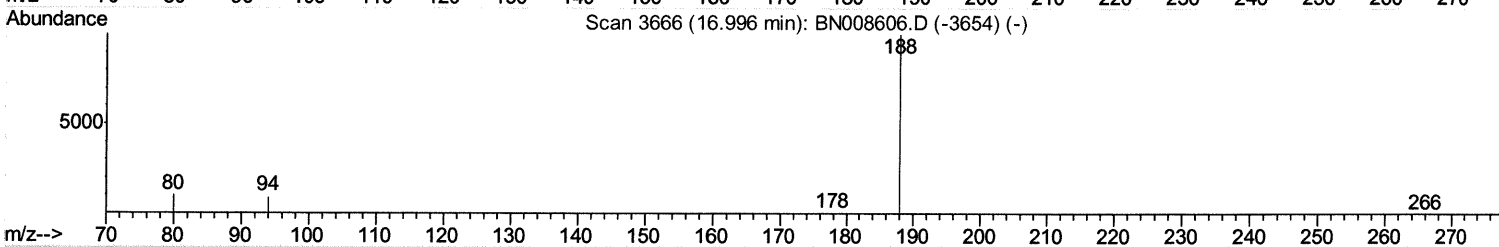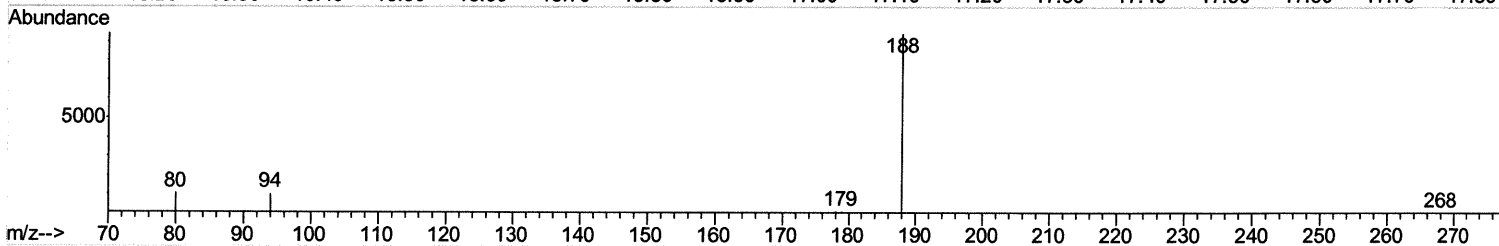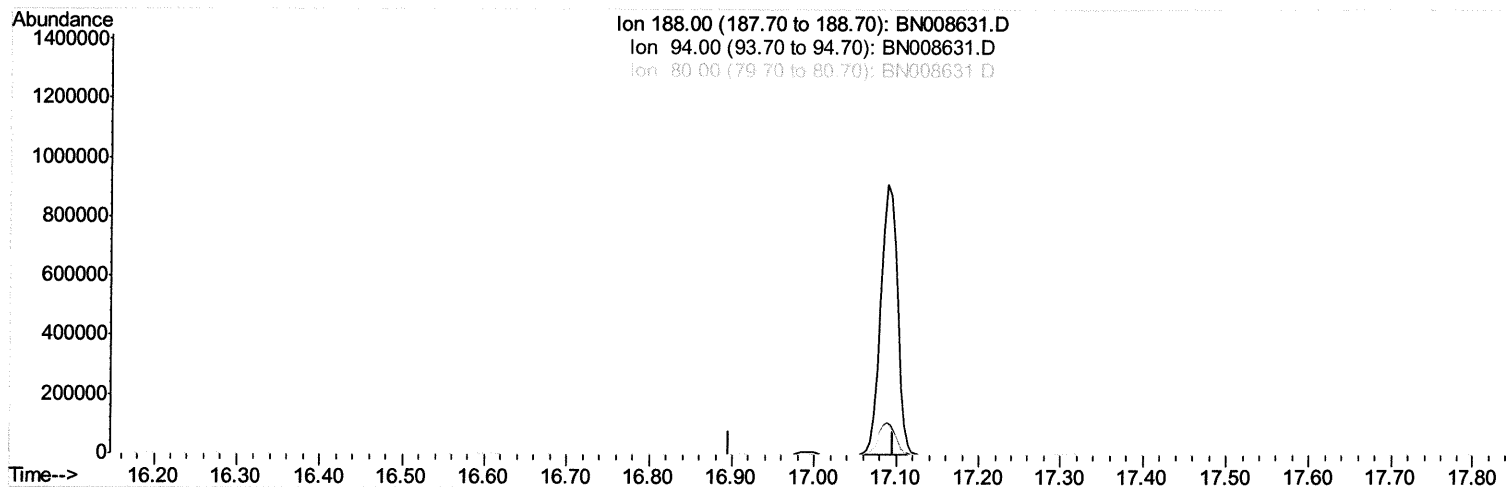

TIC: BN008631.D

(10) Phenanthrene-d10 (I)

16.996min (-16.996) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111919\
 Data File : BN008631.D
 Acq On : 19 Nov 2019 15:37
 Operator : JU
 Sample : PB124657BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK57

Manual Integrations
 APPROVED

mohammad
 11/21/2019 9:04:51 AM

Quant Time: Nov 19 16:19:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 19 01:47:58 2019
 Response via : Initial Calibration

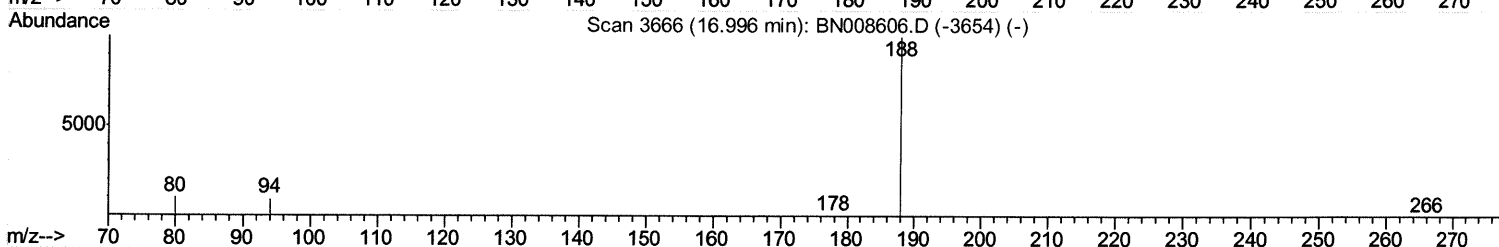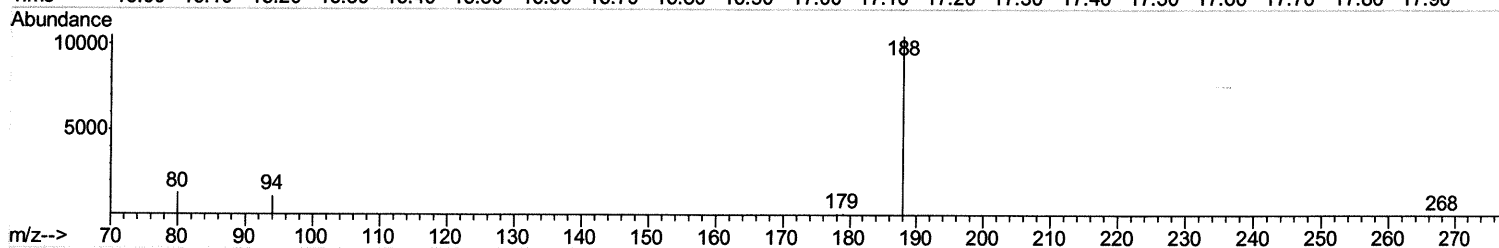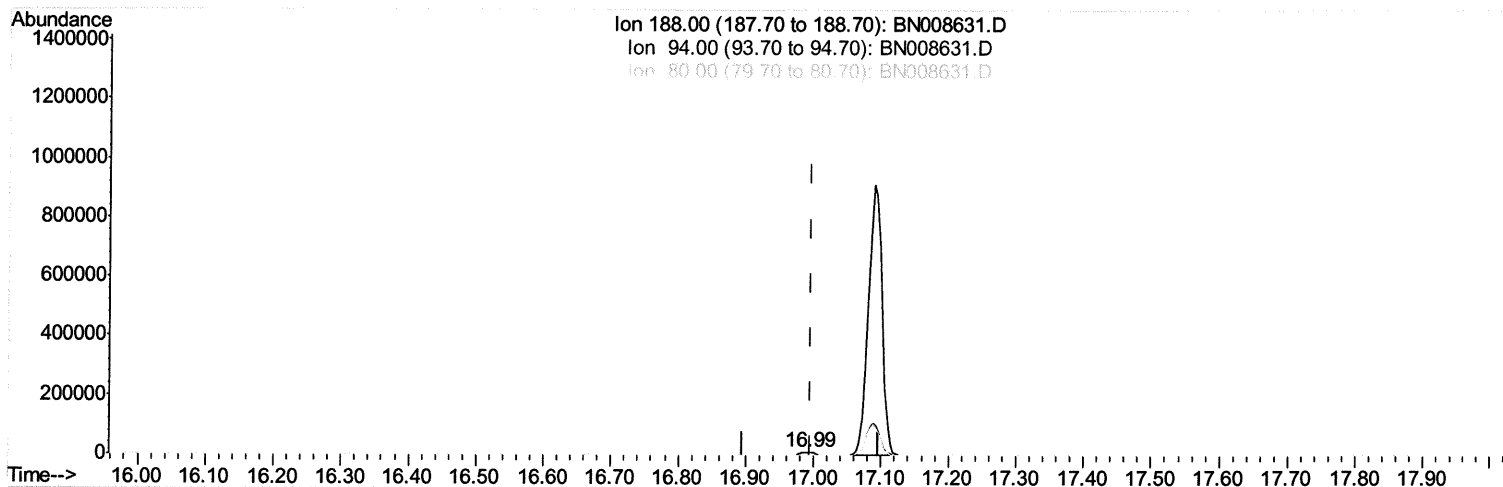

TIC: BN008631.D

(10) Phenanthrene-d10 (I)

16.992min (-0.004) 0.40ng/ul m

response 14260

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	10.94
80.00	11.80	12.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111919\
 Data File : BN008631.D
 Acq On : 19 Nov 2019 15:37
 Operator : JU
 Sample : PB124657BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK57

Manual Integrations
 APPROVED

mohammad
 11/21/2019 9:04:51 AM

Quant Time: Nov 19 16:20:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 19 01:47:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3083	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	11759	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	6726	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	14260m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	11843	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	11827	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152	7105	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	16973	0.39	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed