

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)


Data File : BN008635.D
Acq On : 19 Nov 2019 18:02
Operator : JU
Sample : PB124735BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK35

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:06 AM

Quant Time: Nov 20 03:59:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

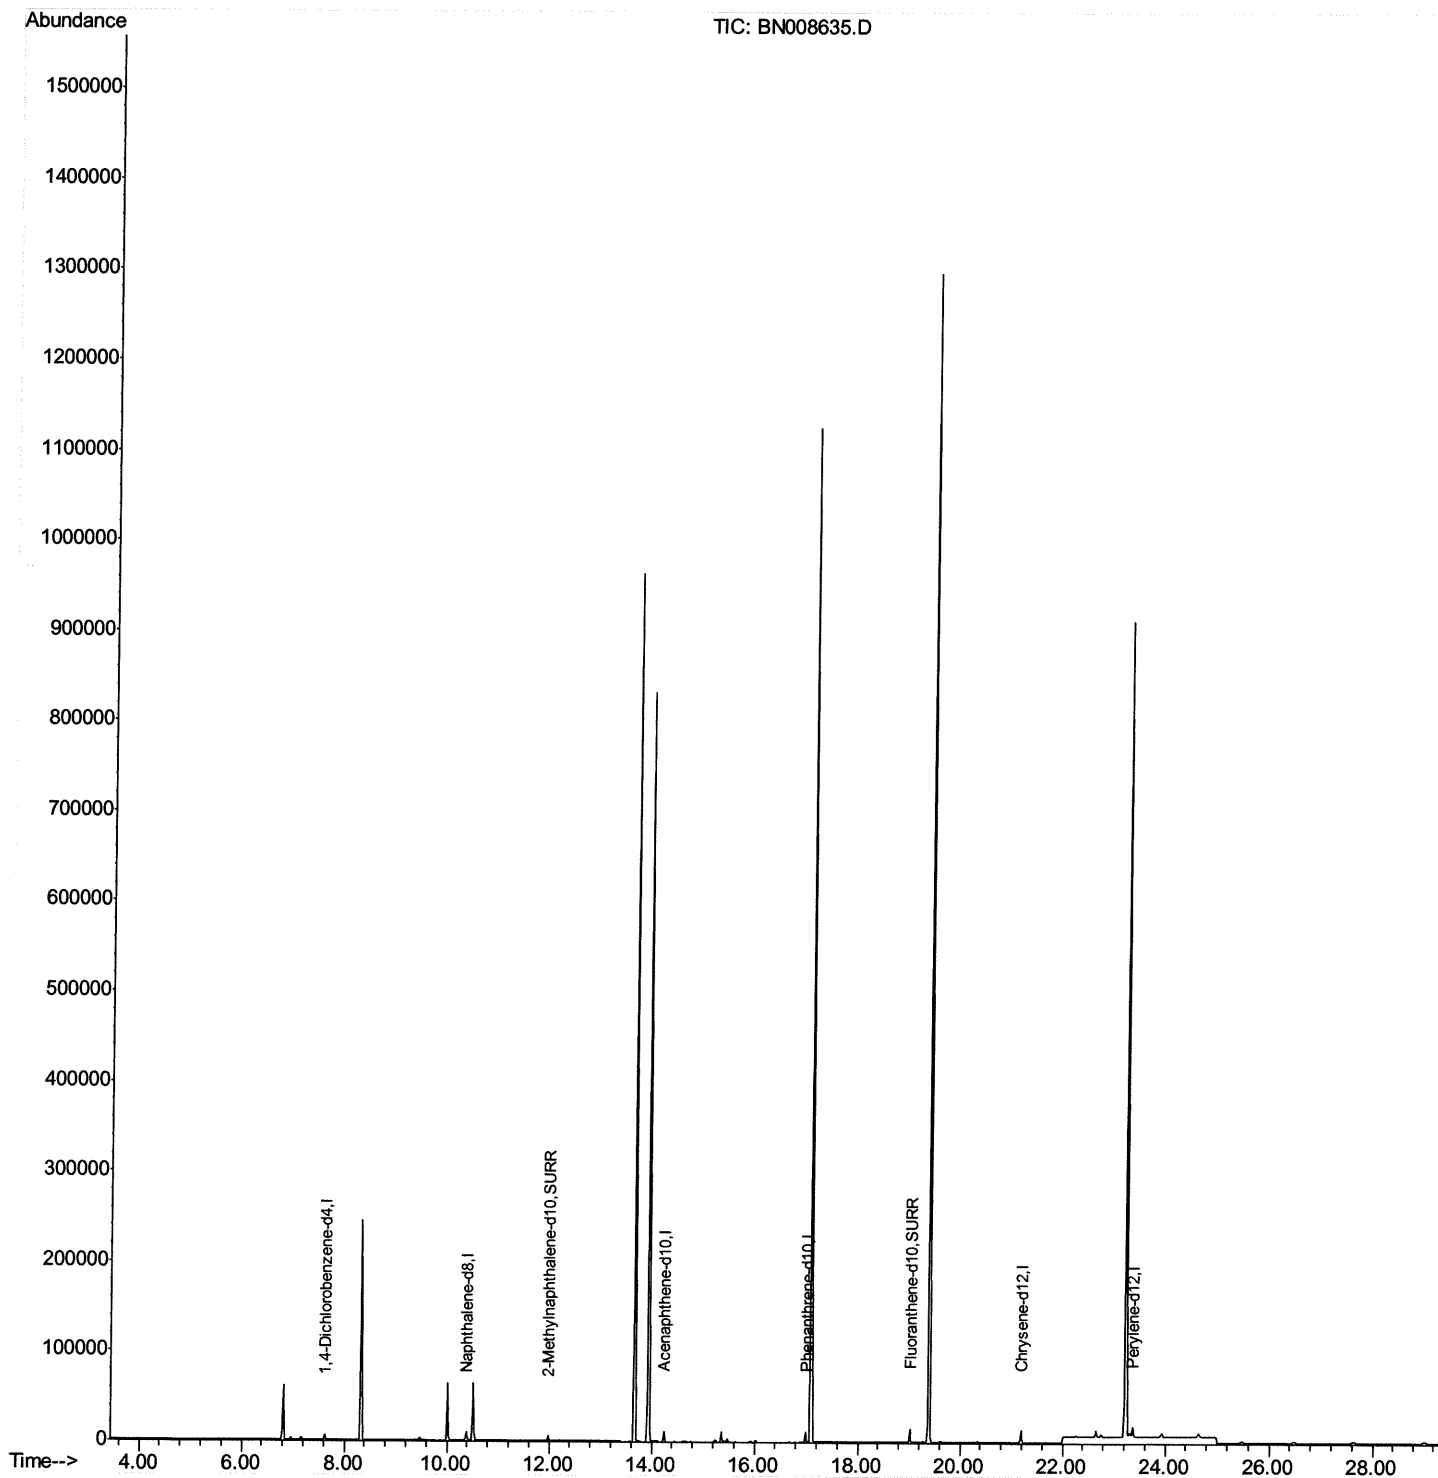

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008635.D
Acq On : 19 Nov 2019 18:02
Operator : JU
Sample : PB124735BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK35

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:06 AM

Quant Time: Nov 20 03:44:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

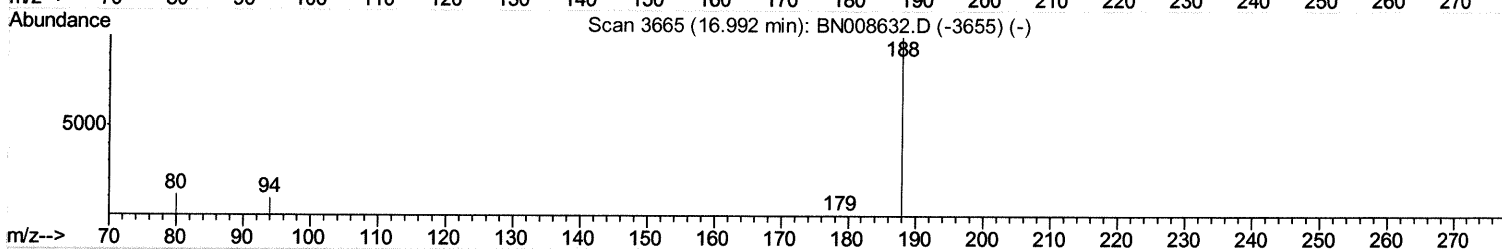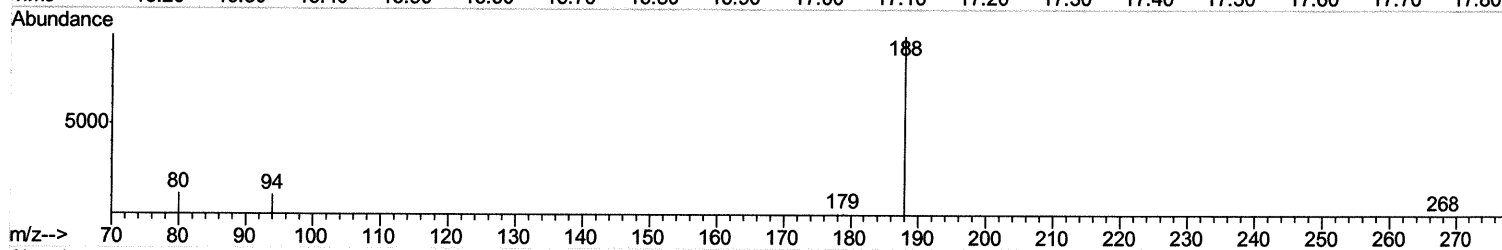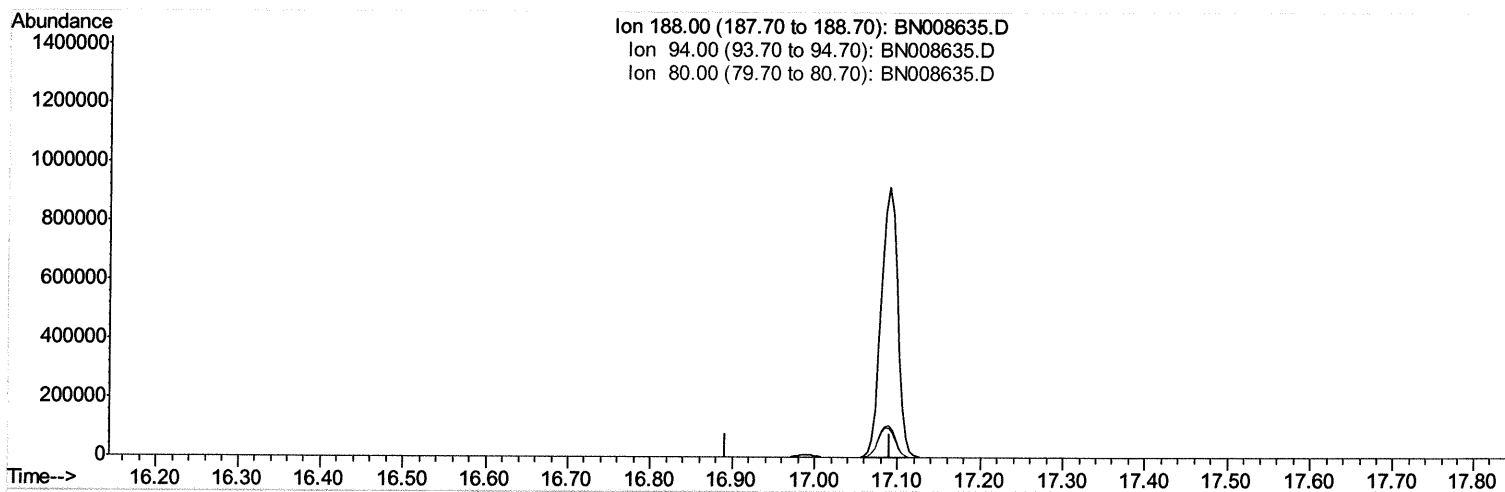

TIC: BN008635.D

(10) Phenanthrene-d10 (I)

16.992min (-16.992) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008635.D
Acq On : 19 Nov 2019 18:02
Operator : JU
Sample : PB124735BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK35

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:06 AM

Quant Time: Nov 20 03:44:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

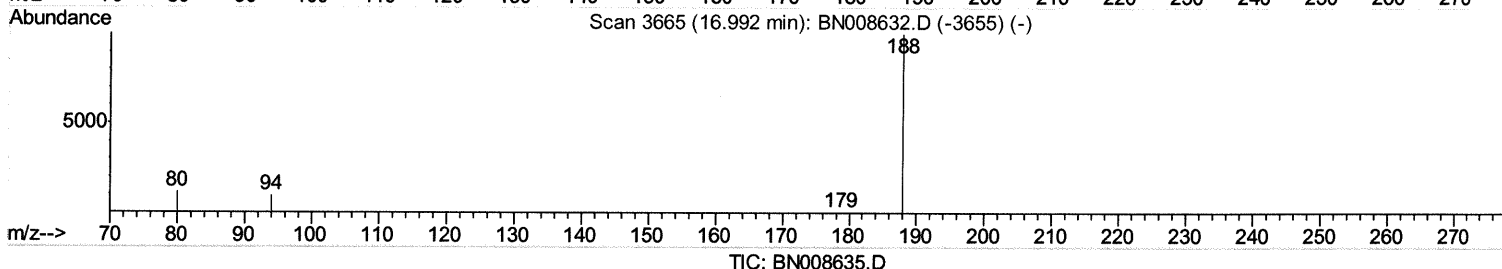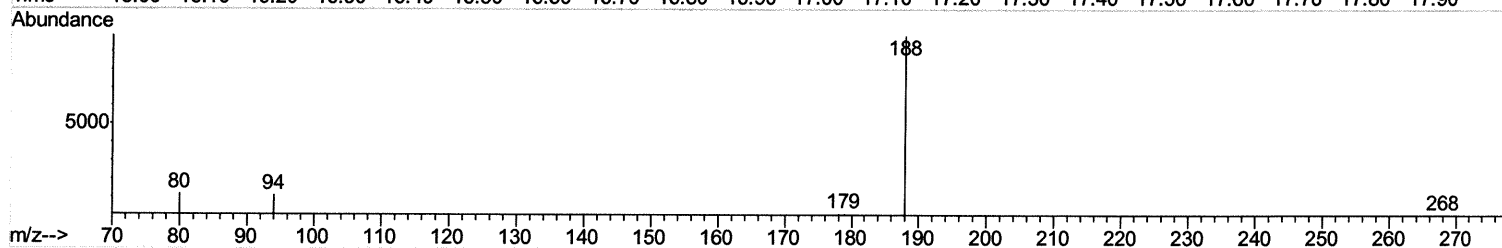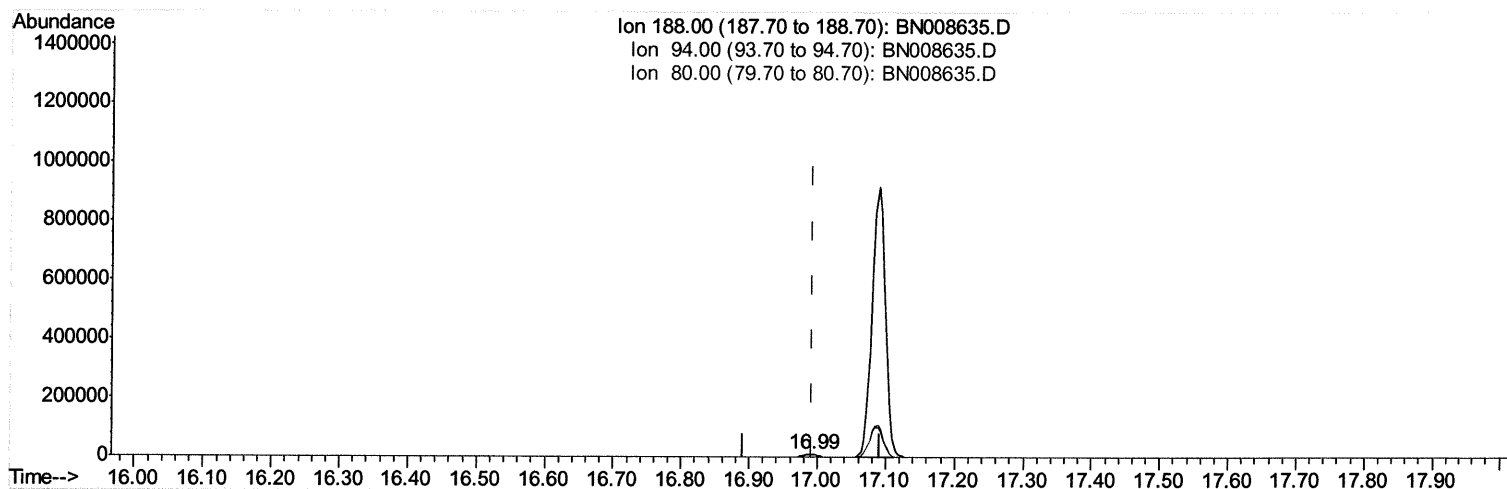

(10) Phenanthrene-d10 (I)

16.992min (-0.000) 0.40ng/ul m

response 13805

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	11.26
80.00	11.80	12.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008635.D
Acq On : 19 Nov 2019 18:02
Operator : JU
Sample : PB124735BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK35

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:06 AM

Quant Time: Nov 20 03:58:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

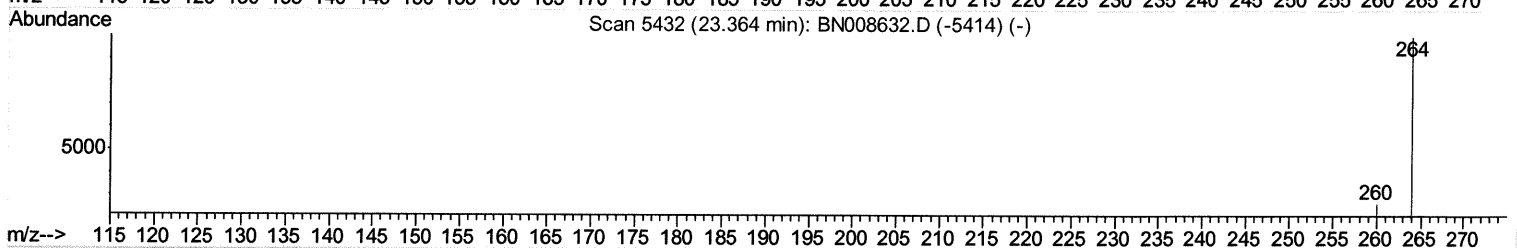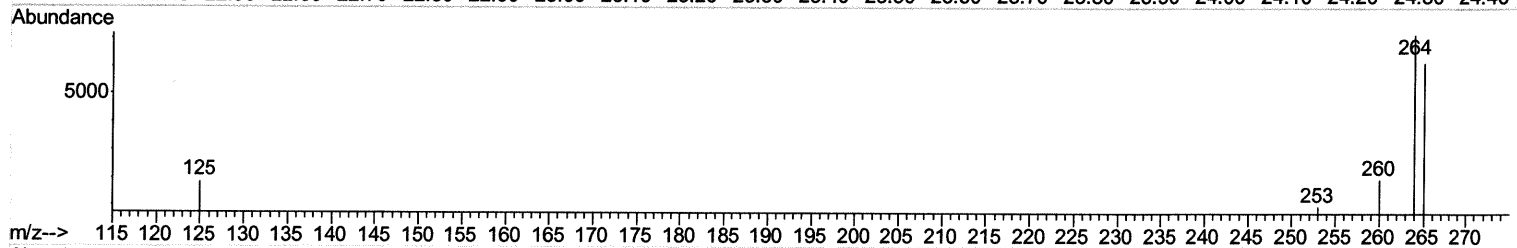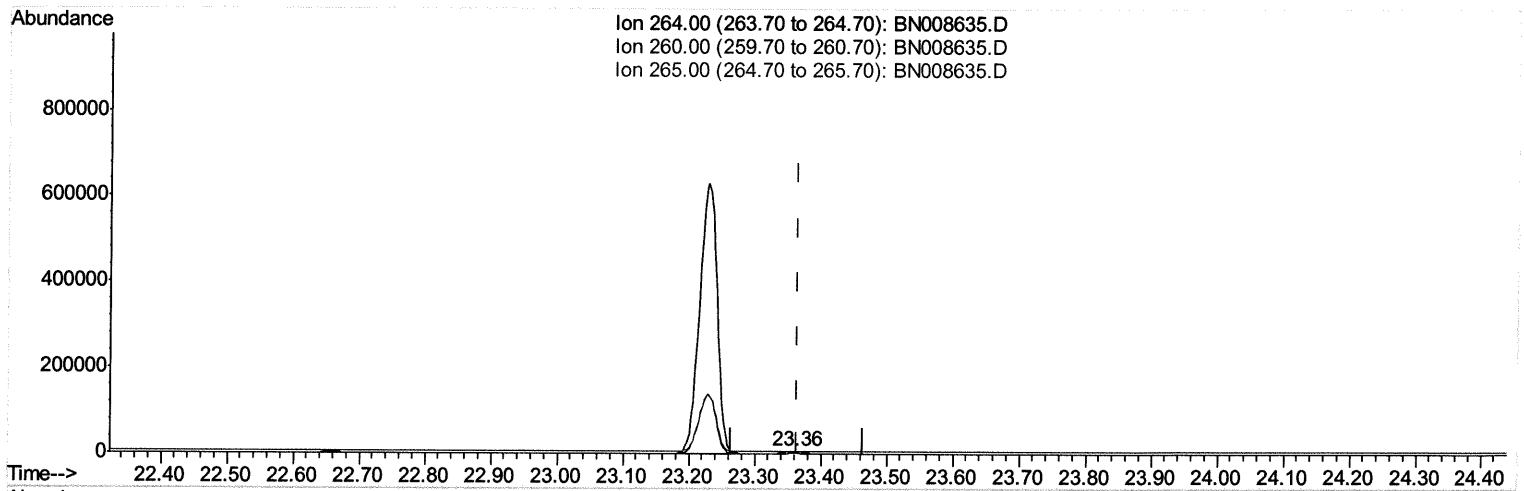

TIC: BN008635.D

(20) Perylene-d12 (I)

23.361min (-0.003) 0.40ng/ul

response 12665

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.48
265.00	69.30	86.19#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008635.D
Acq On : 19 Nov 2019 18:02
Operator : JU
Sample : PB124735BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK35

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:06 AM

Quant Time: Nov 20 03:58:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

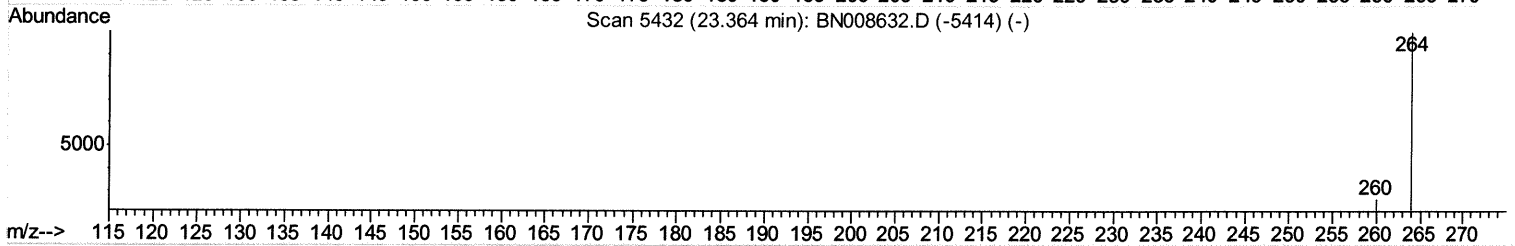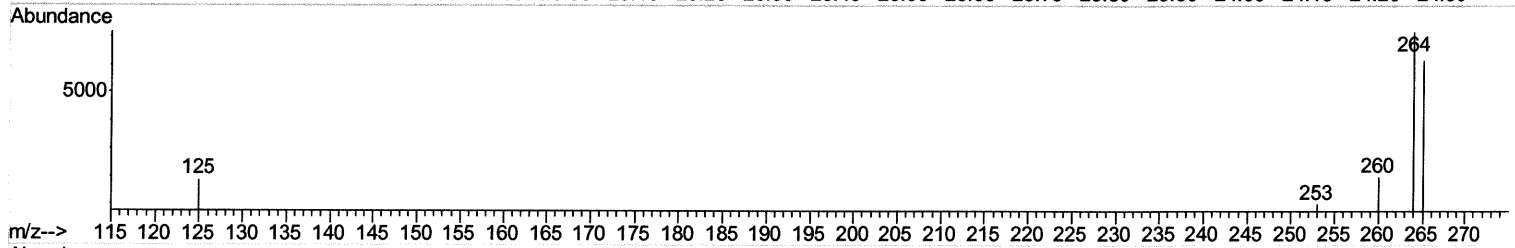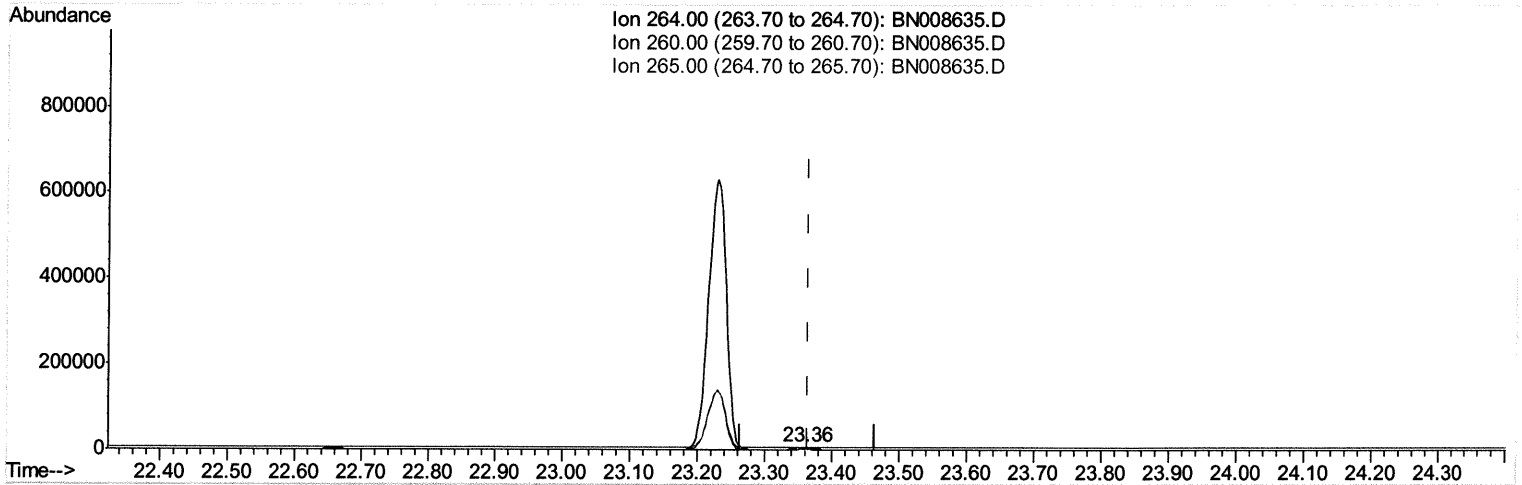

TIC: BN008635.D

(20) Perylene-d12 (I)

23.361min (-0.003) 0.40ng/ul m

response 11867

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.48
265.00	69.30	86.19#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)

Data File : BN008635.D
Acq On : 19 Nov 2019 18:02
Operator : JU
Sample : PB124735BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK35

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:06 AM

Quant Time: Nov 20 03:59:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3166	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	11575	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	6596	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	13805m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	12330	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	11867m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152	7041	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	16843	0.40	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Ju 11/21/19
Ju 11/21/19