

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)


Data File : BN008637.D
Acq On : 19 Nov 2019 19:14
Operator : JU
Sample : K5699-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J10

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:08 AM

Quant Time: Nov 20 04:15:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

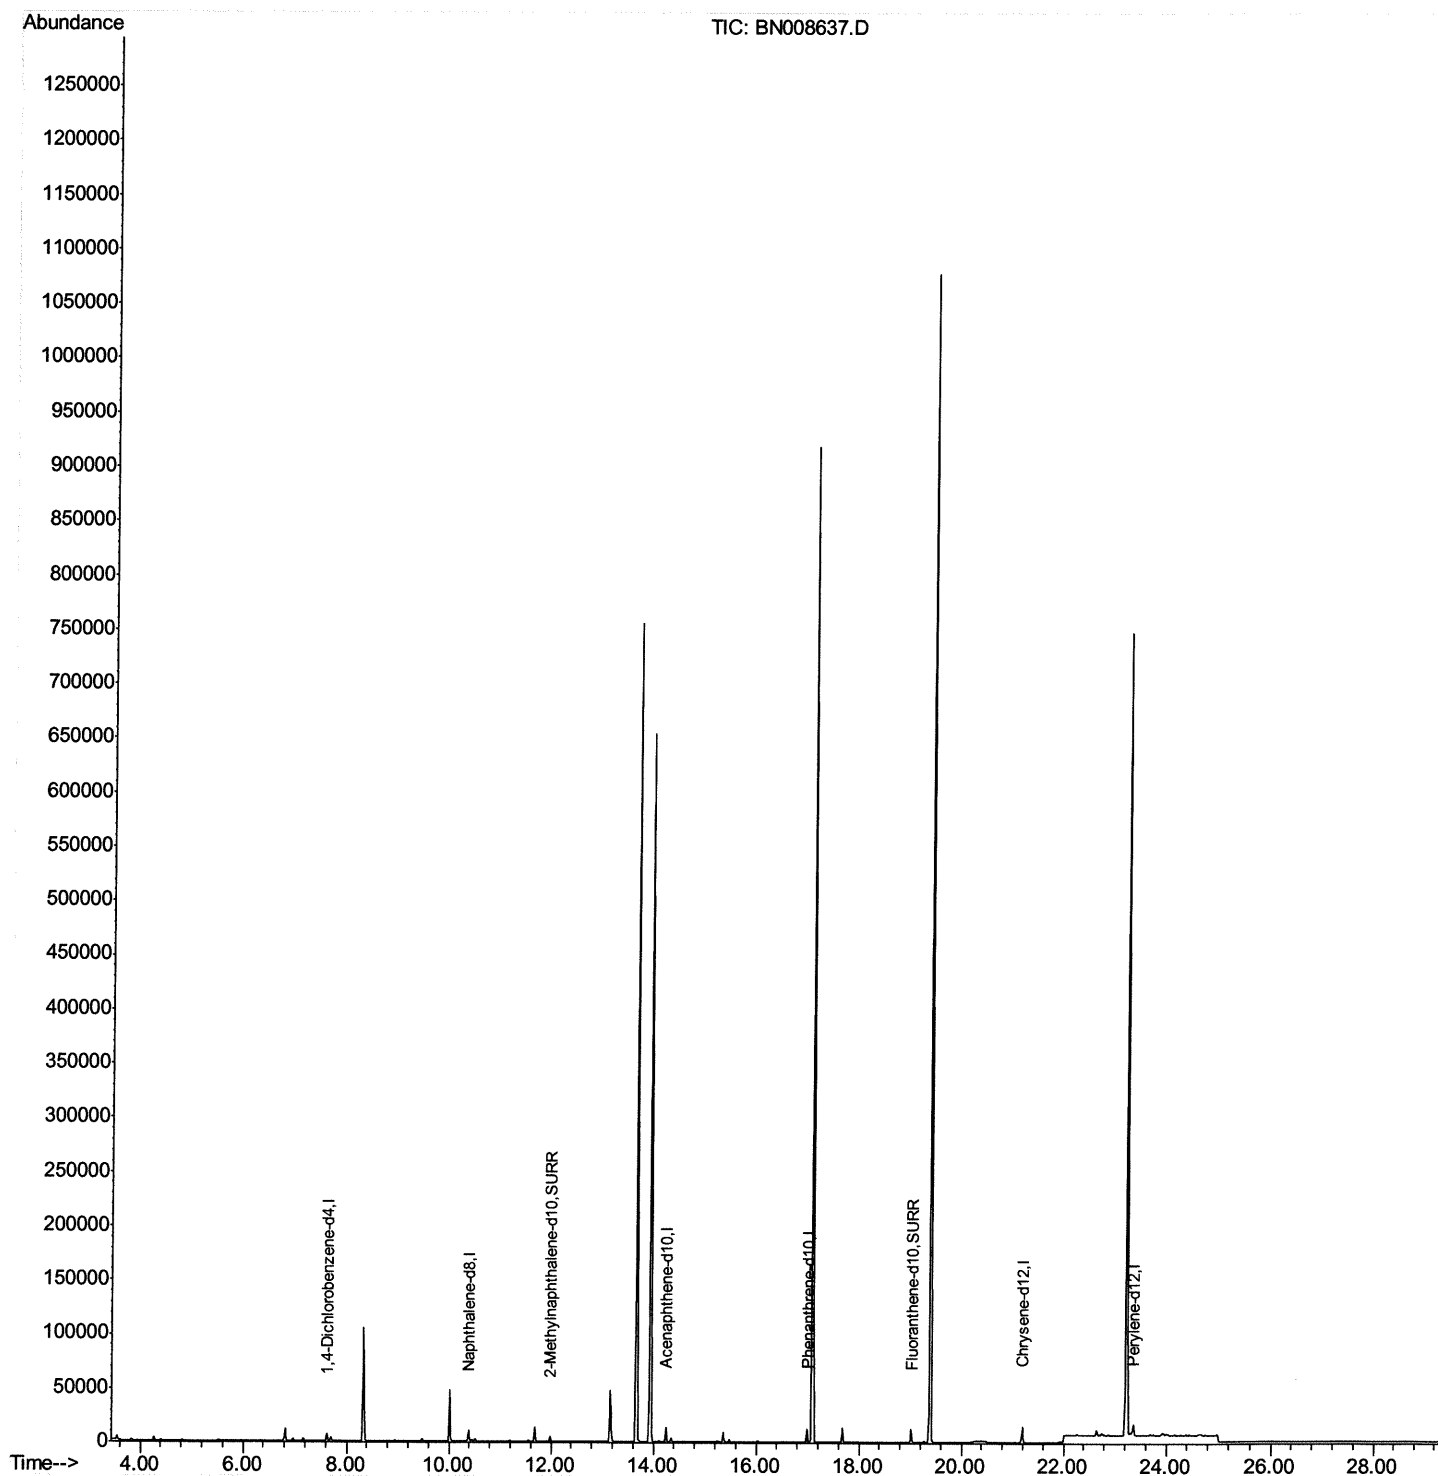

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008637.D
Acq On : 19 Nov 2019 19:14
Operator : JU
Sample : K5699-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J10

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:08 AM

Quant Time: Nov 20 03:44:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

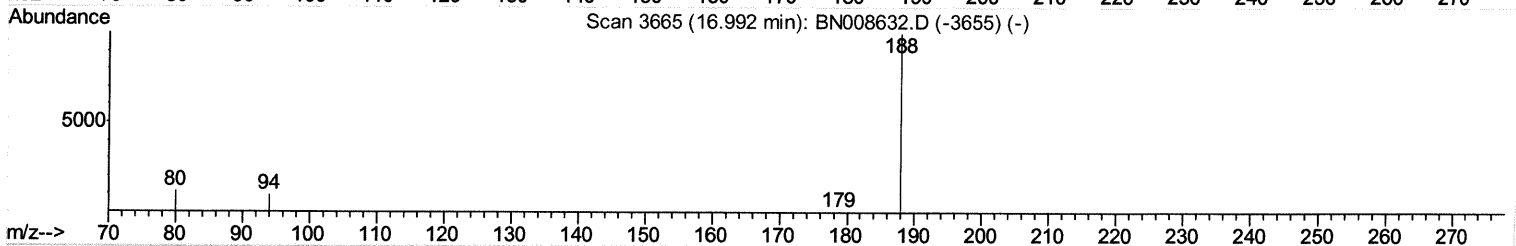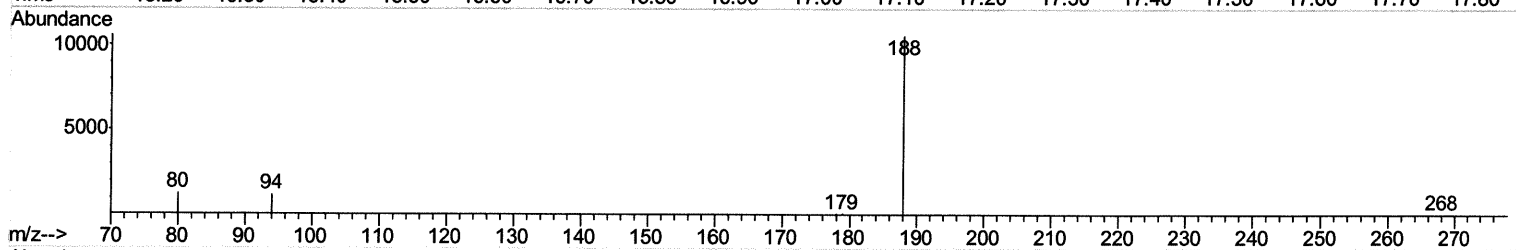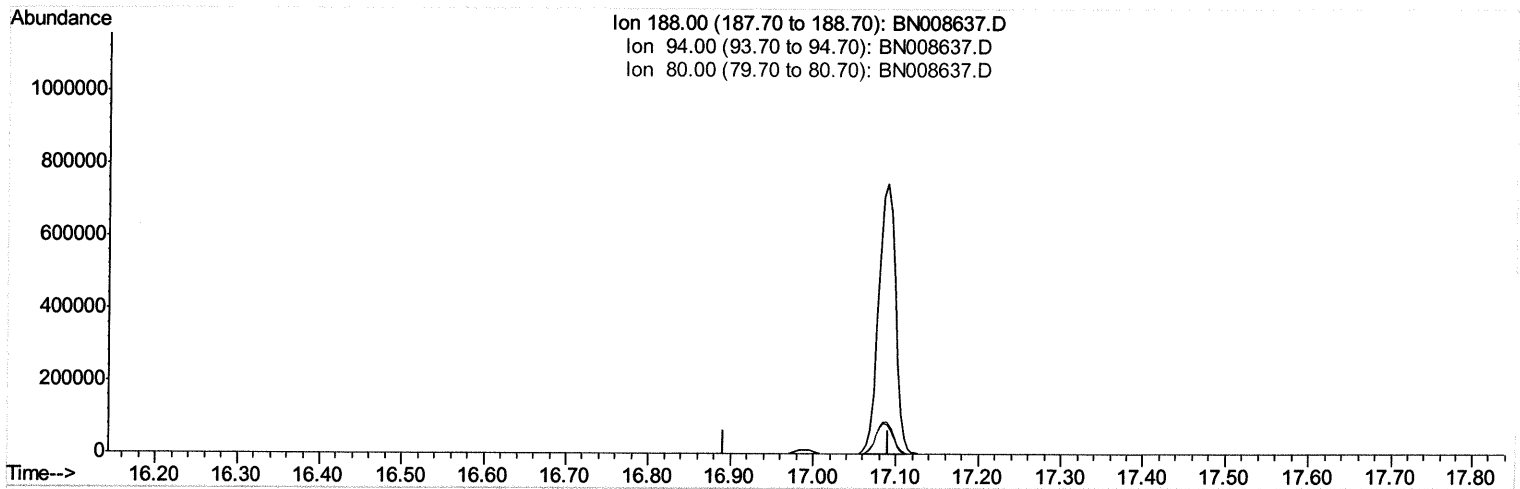

TIC: BN008637.D

(10) Phenanthrene-d10 (I)

16.992min (-16.992) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008637.D
Acq On : 19 Nov 2019 19:14
Operator : JU
Sample : K5699-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J10

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:08 AM

Quant Time: Nov 20 03:44:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

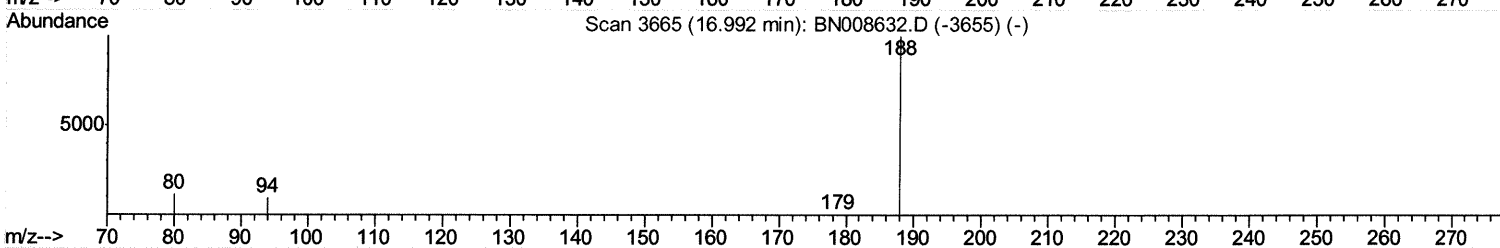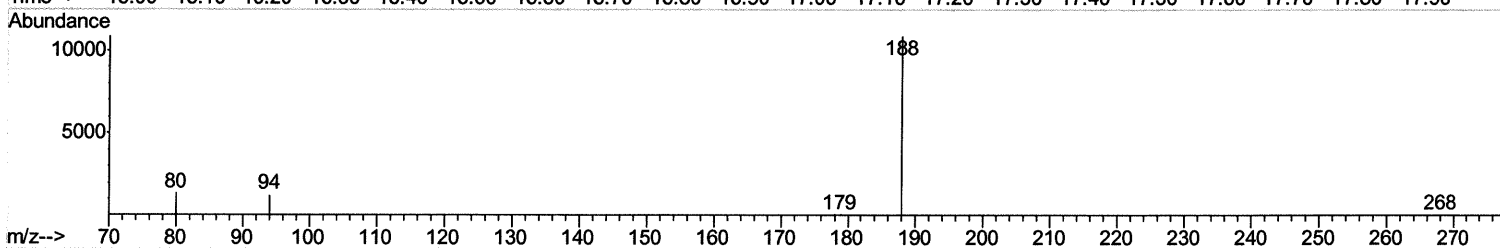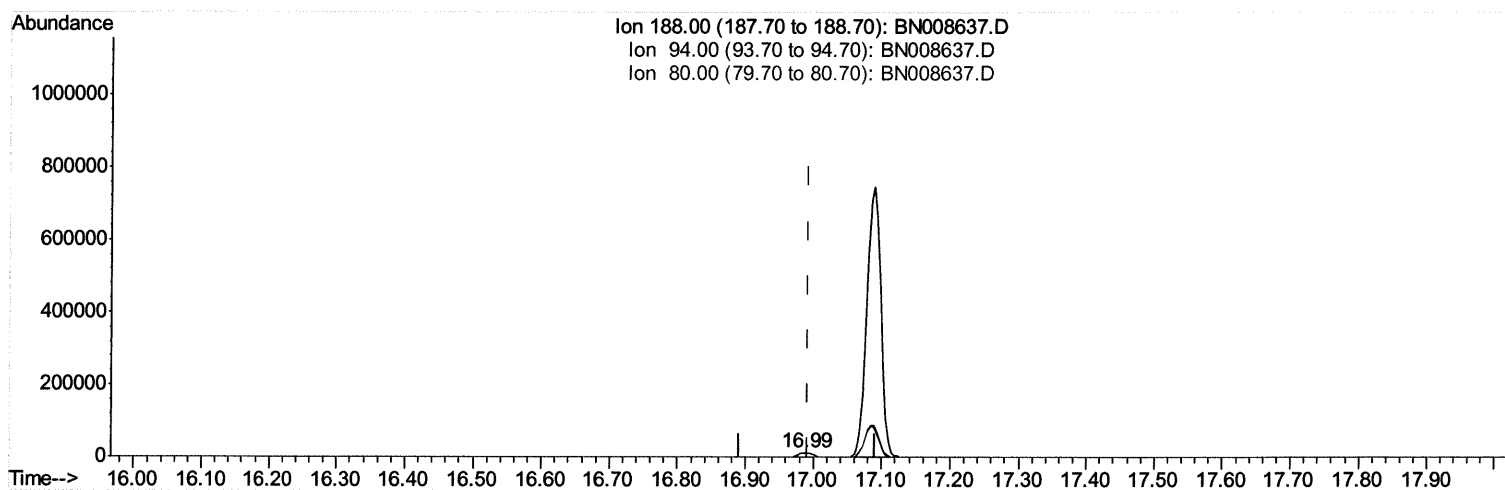

TIC: BN008637.D

(10) Phenanthrene-d10 (I)

16.988min (-0.004) 0.40ng/ul m

response 15363

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	11.63
80.00	11.80	12.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008637.D
Acq On : 19 Nov 2019 19:14
Operator : JU
Sample : K5699-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J10

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:08 AM

Quant Time: Nov 20 04:14:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

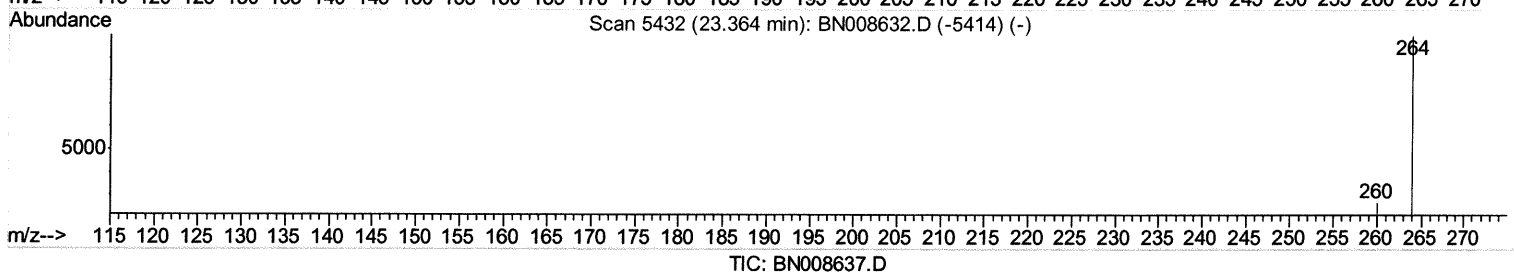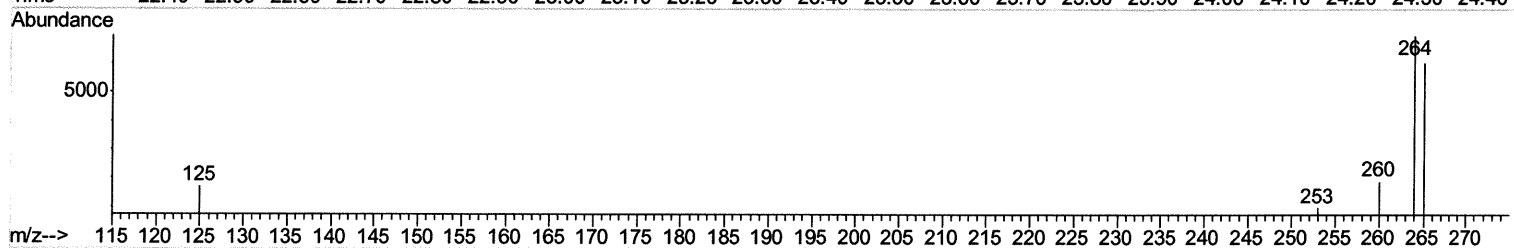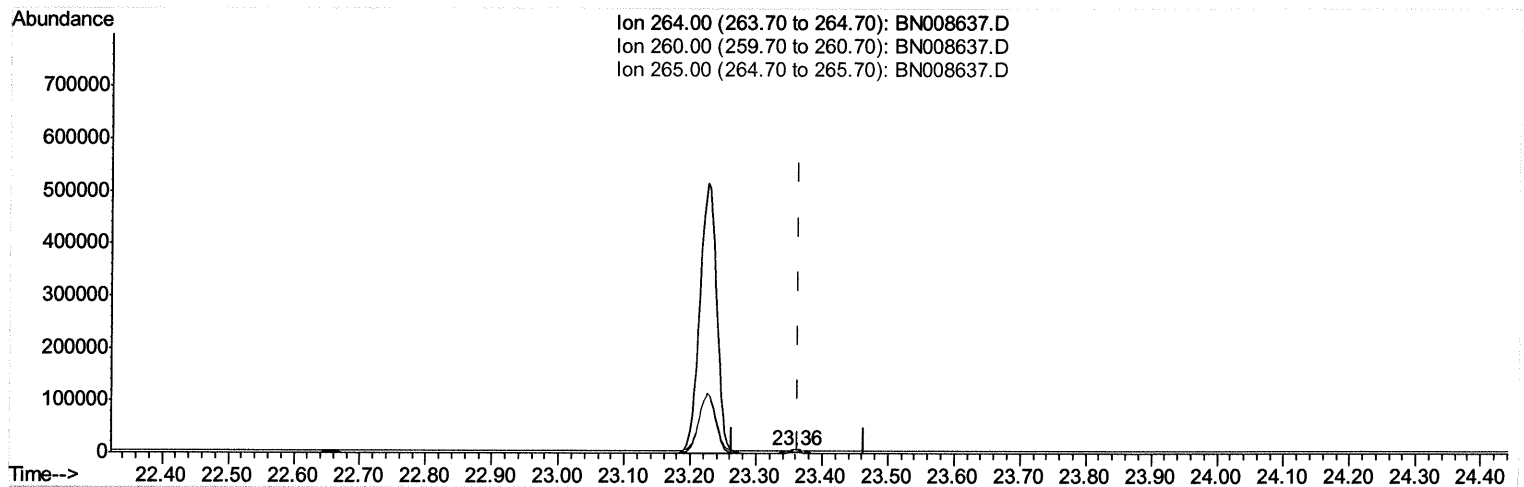

TIC: BN008637.D

(20) Perylene-d12 (I)

23.358min (-0.006) 0.40ng/ul

response 12877

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.19
265.00	69.30	86.54#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008637.D
Acq On : 19 Nov 2019 19:14
Operator : JU
Sample : K5699-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F2J10

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:08 AM

Quant Time: Nov 20 04:14:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

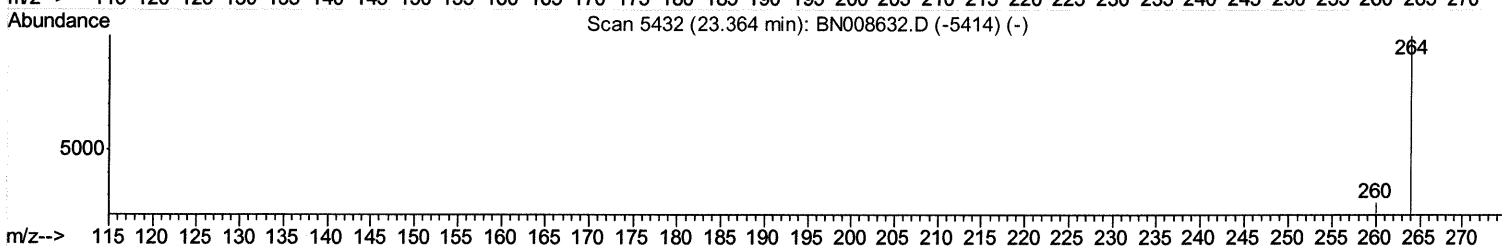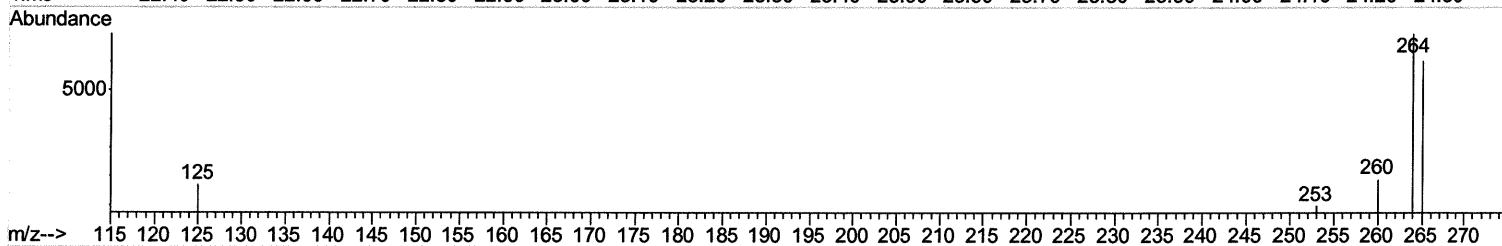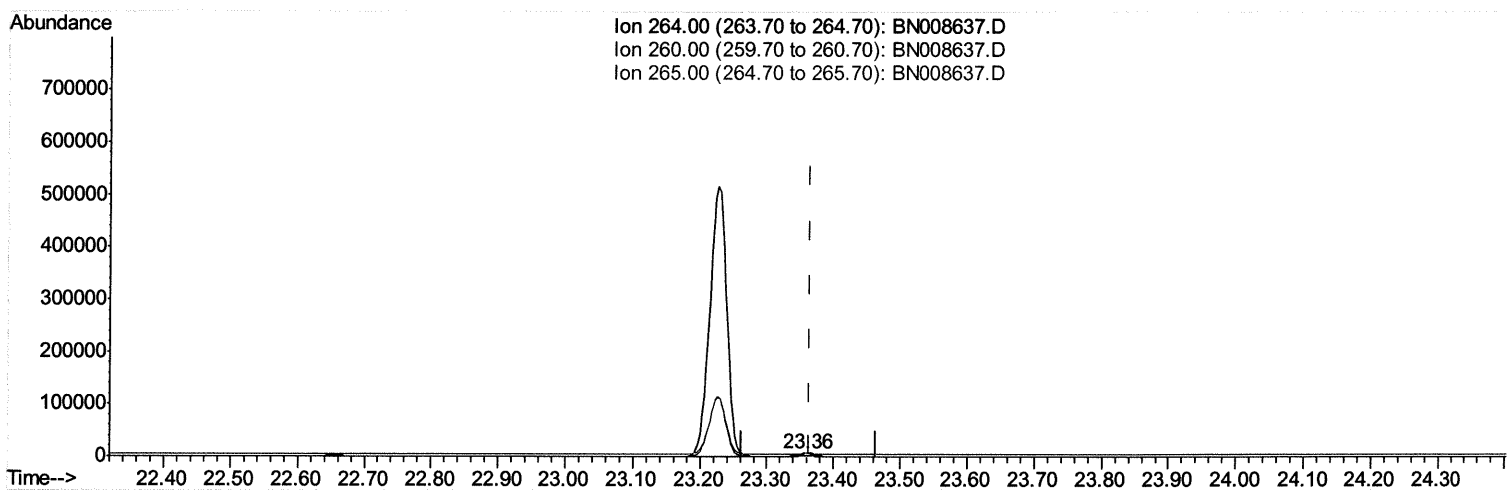

TIC: BN008637.D

(20) Perylene-d12 (I)

23.358min (-0.006) 0.40ng/ul m

response 12076

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.19
265.00	69.30	86.54#
0.00	0.00	0.00

ju 11/21/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)

Data File : BN008637.D
Acq On : 19 Nov 2019 19:14
Operator : JU
Sample : K5699-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J10

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:08 AM

Quant Time: Nov 20 04:15:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

Internal Standards	R.T.	Q	Ion	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.63	152		3401	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136		12753	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.25	164		7403	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188		15363m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240		12719	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264		12076m	0.40	ng/ul	0.00

J4 11/21/19
J4 11/21/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152		5317	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.02	212		13751	0.29	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed