

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)


Data File : BN008641.D
Acq On : 19 Nov 2019 21:39
Operator : JU
Sample : K5699-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J11

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:22 AM

Quant Time: Nov 20 04:25:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

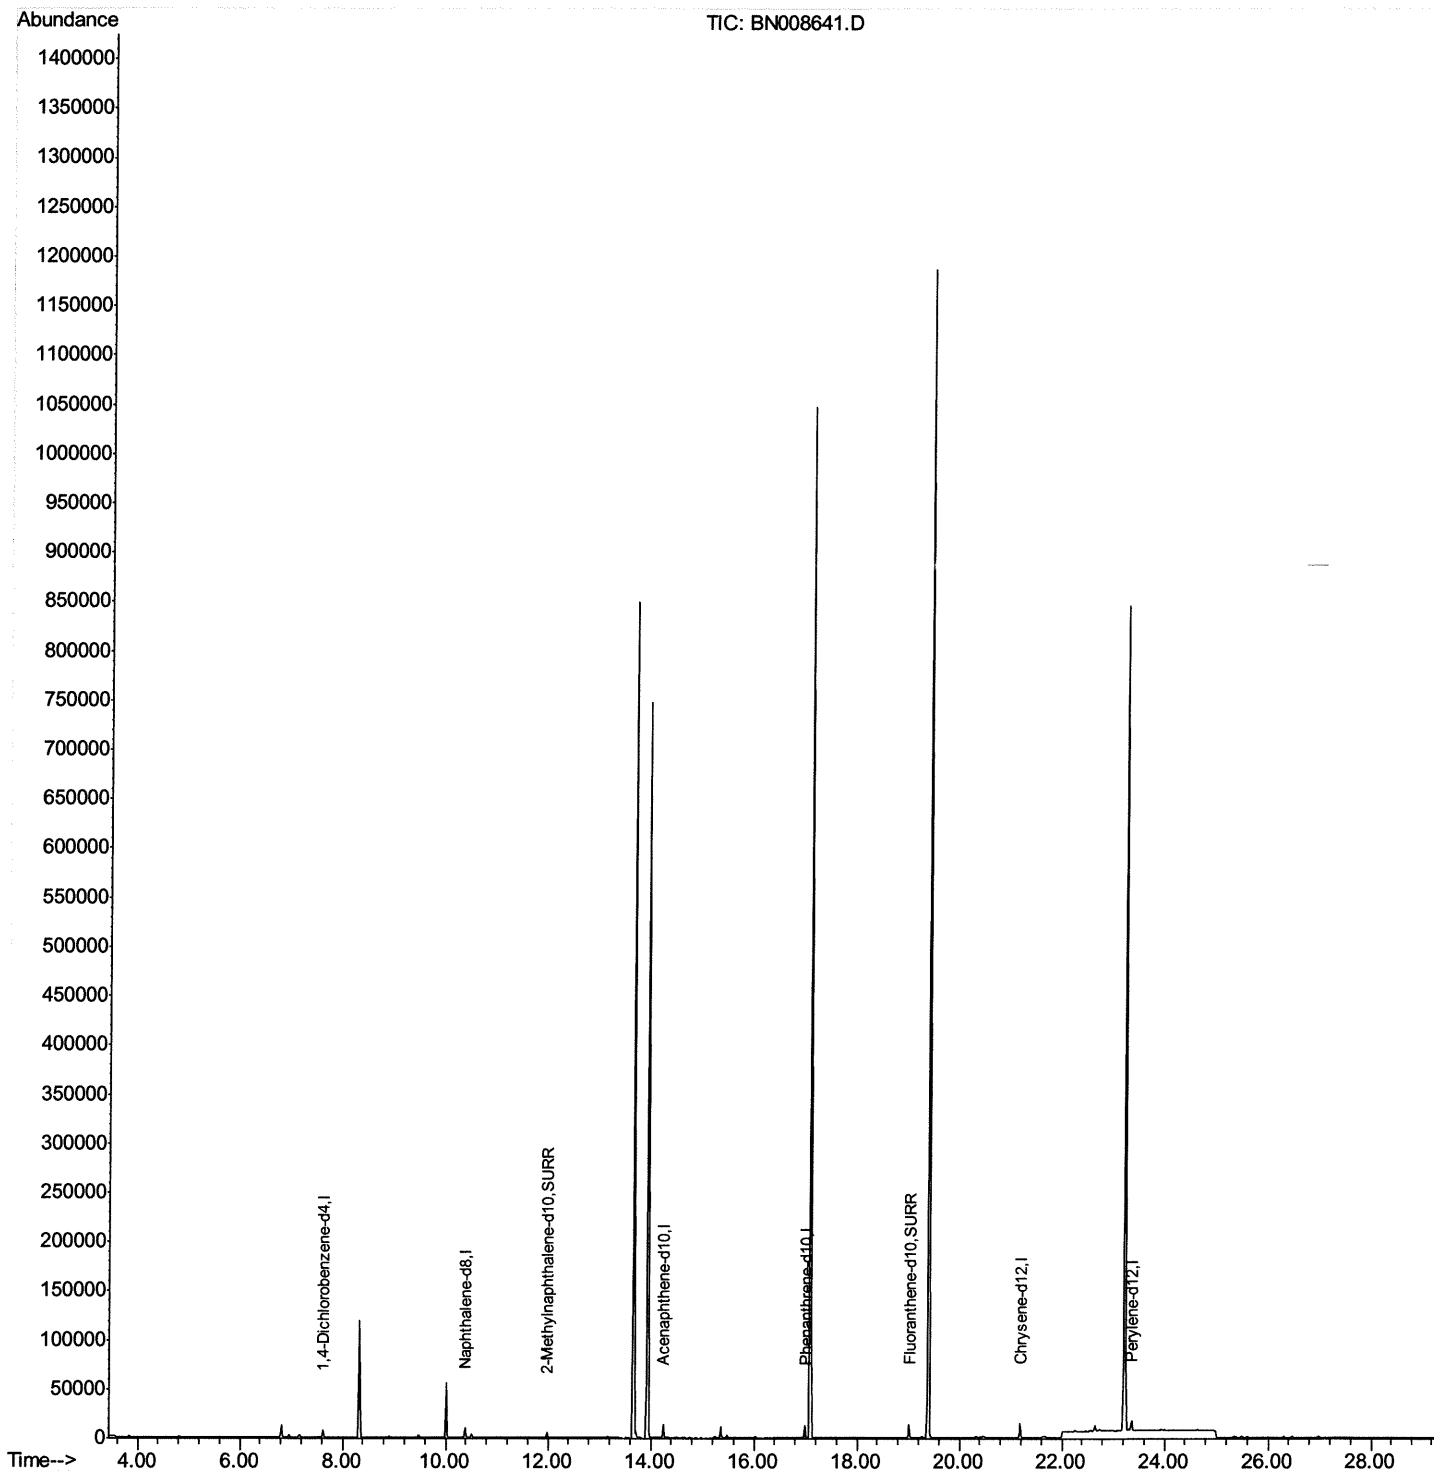

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008641.D
Acq On : 19 Nov 2019 21:39
Operator : JU
Sample : K5699-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J11

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:22 AM

Quant Time: Nov 20 03:44:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

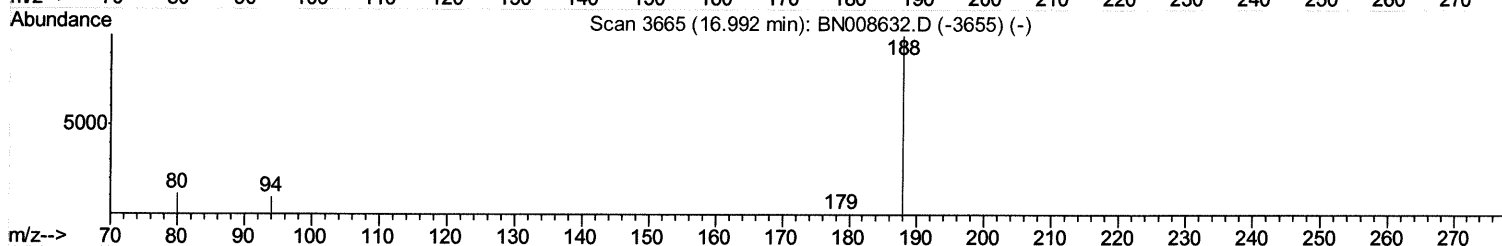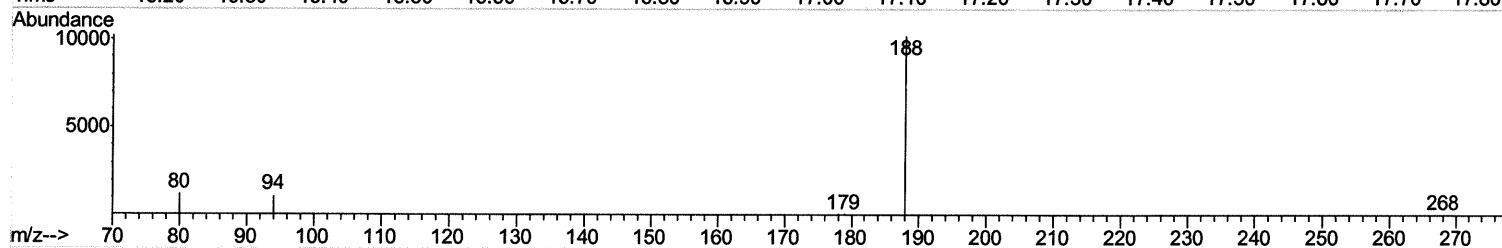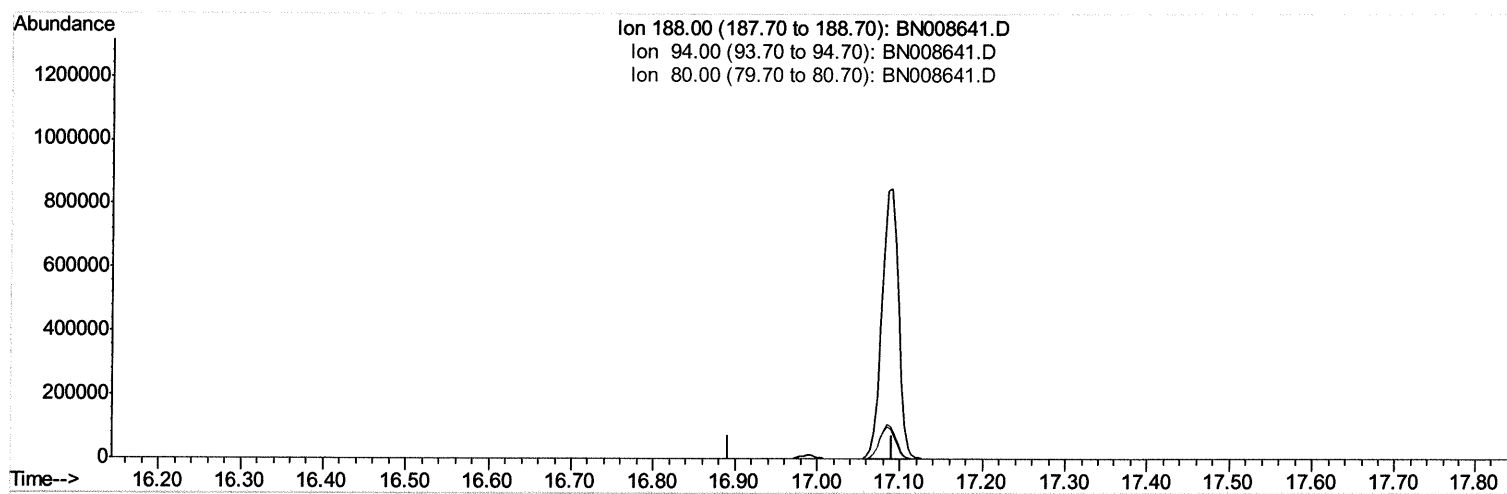

TIC: BN008641.D

(10) Phenanthrene-d10 (I)

16.992min (-16.992) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008641.D
Acq On : 19 Nov 2019 21:39
Operator : JU
Sample : K5699-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J11

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:22 AM

Quant Time: Nov 20 03:44:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

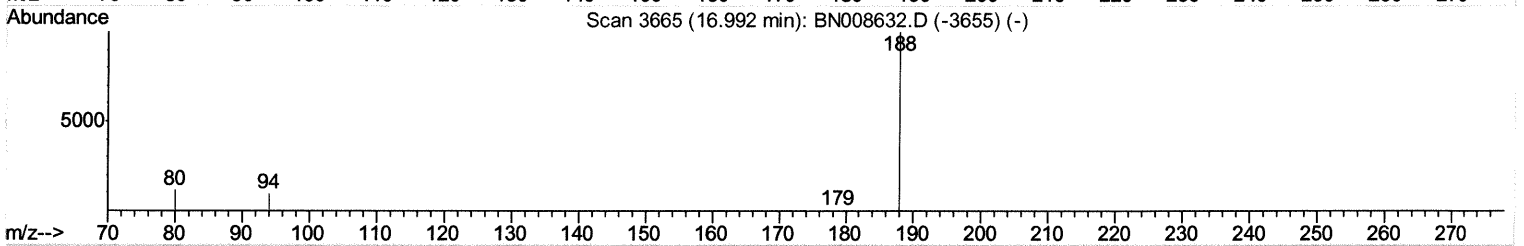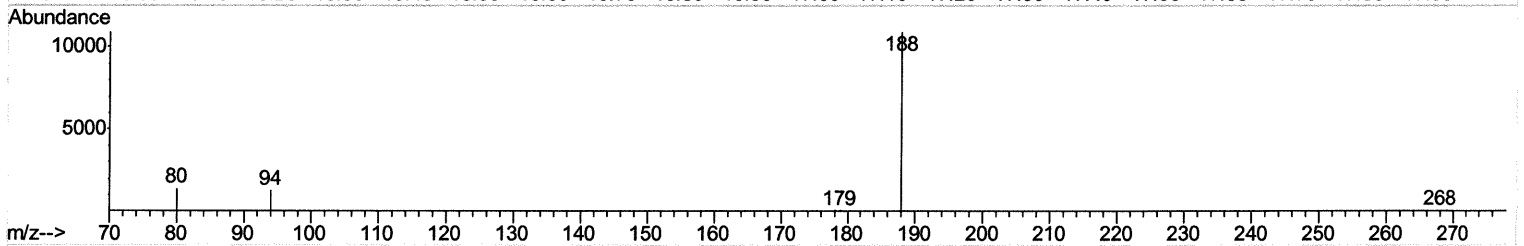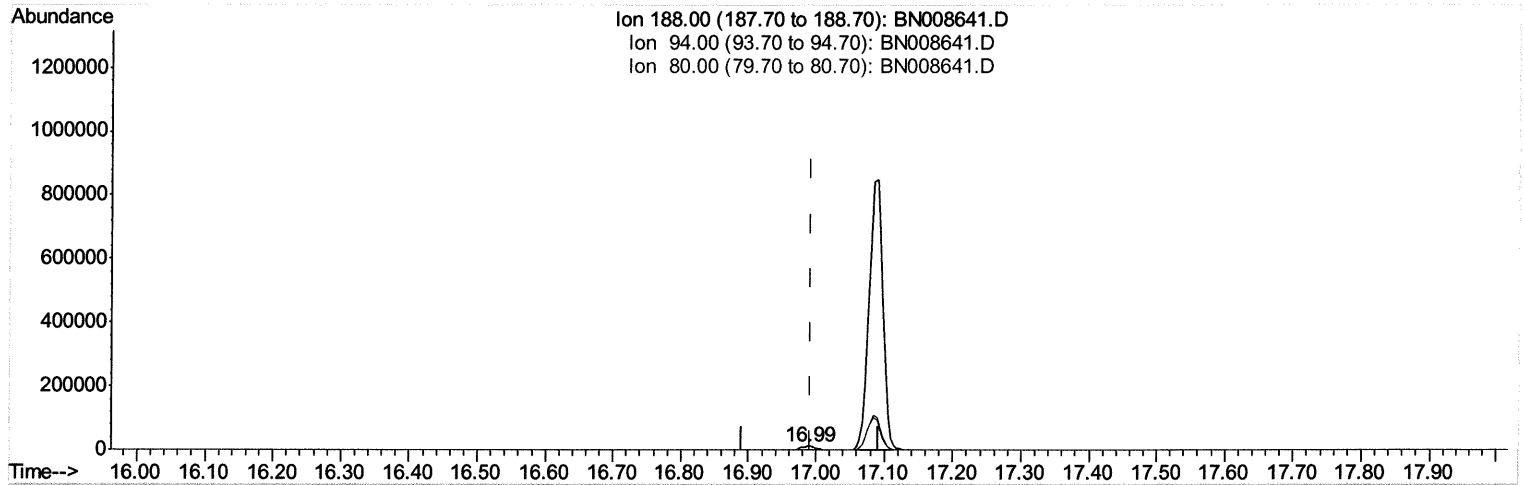

TIC: BN008641.D

(10) Phenanthrene-d10 (I)

16.988min (-0.004) 0.40ng/ul m

response 15003

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	11.78
80.00	11.80	12.85
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008641.D
Acq On : 19 Nov 2019 21:39
Operator : JU
Sample : K5699-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J11

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:22 AM

Quant Time: Nov 20 04:23:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

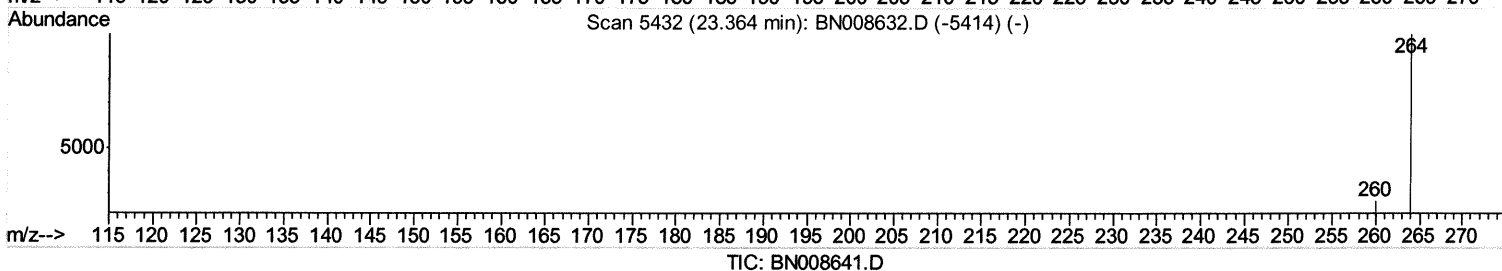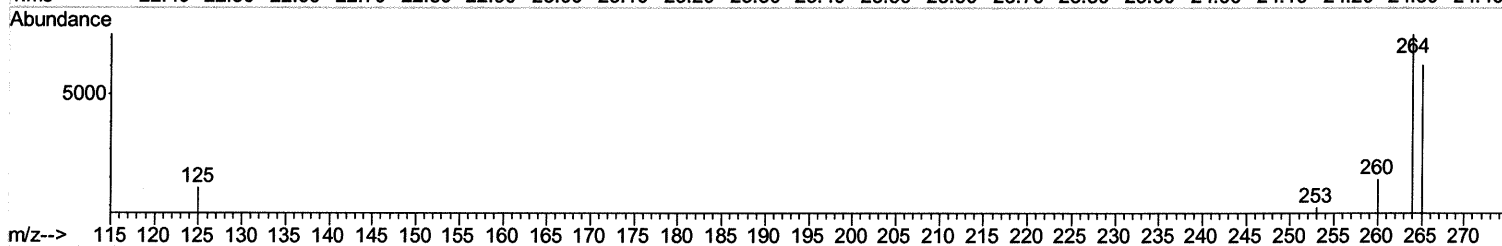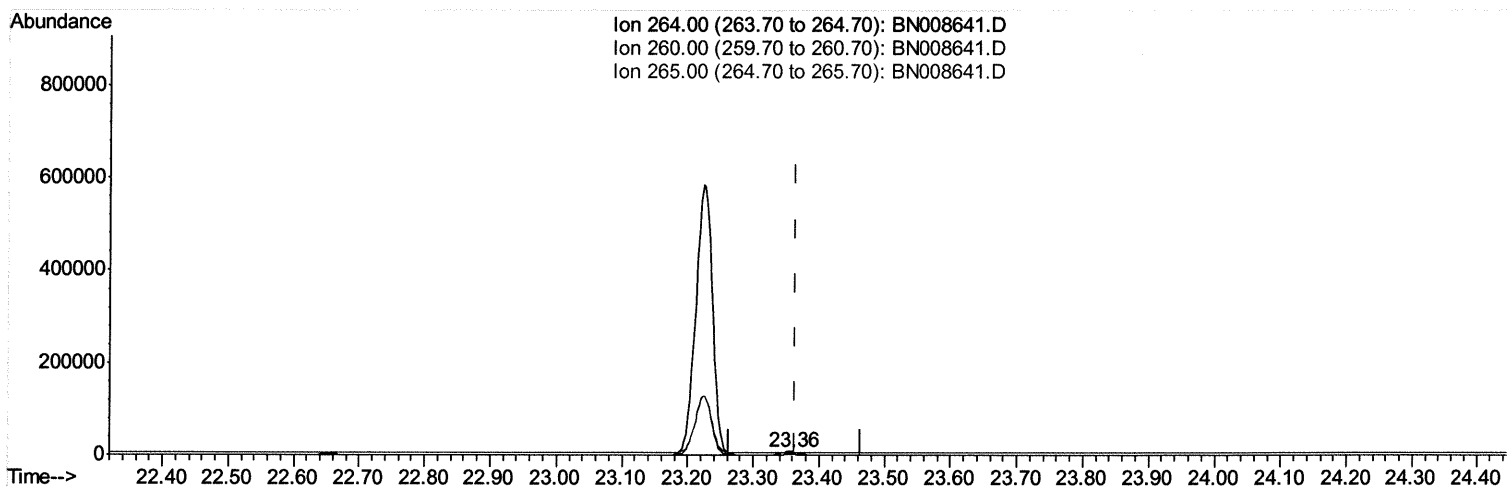

(20) Perylene-d12 (I)

23.358min (-0.006) 0.40ng/ul

response 13071

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.18
265.00	69.30	84.80#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008641.D
Acq On : 19 Nov 2019 21:39
Operator : JU
Sample : K5699-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F2J11

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:22 AM

Quant Time: Nov 20 04:23:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

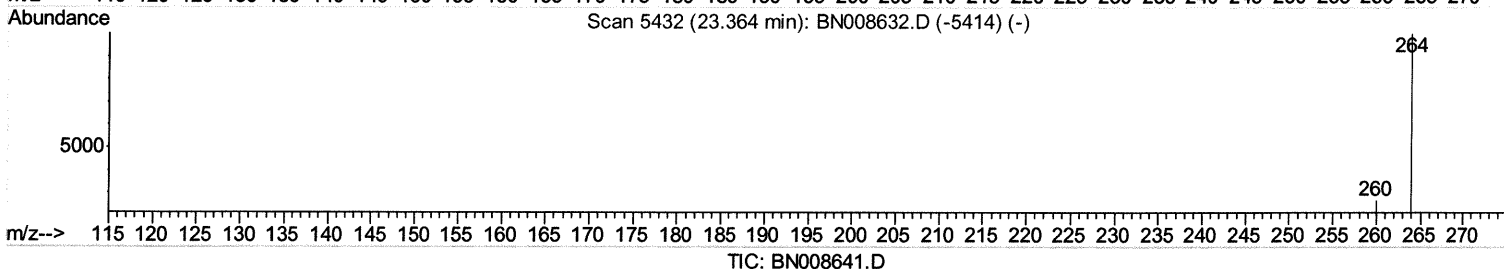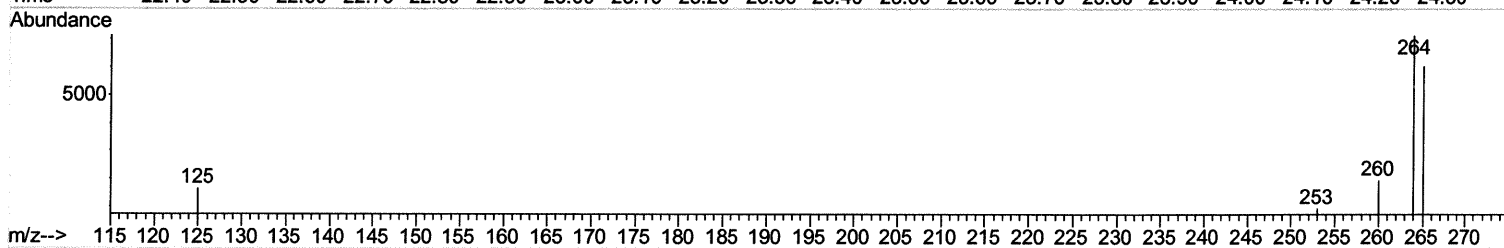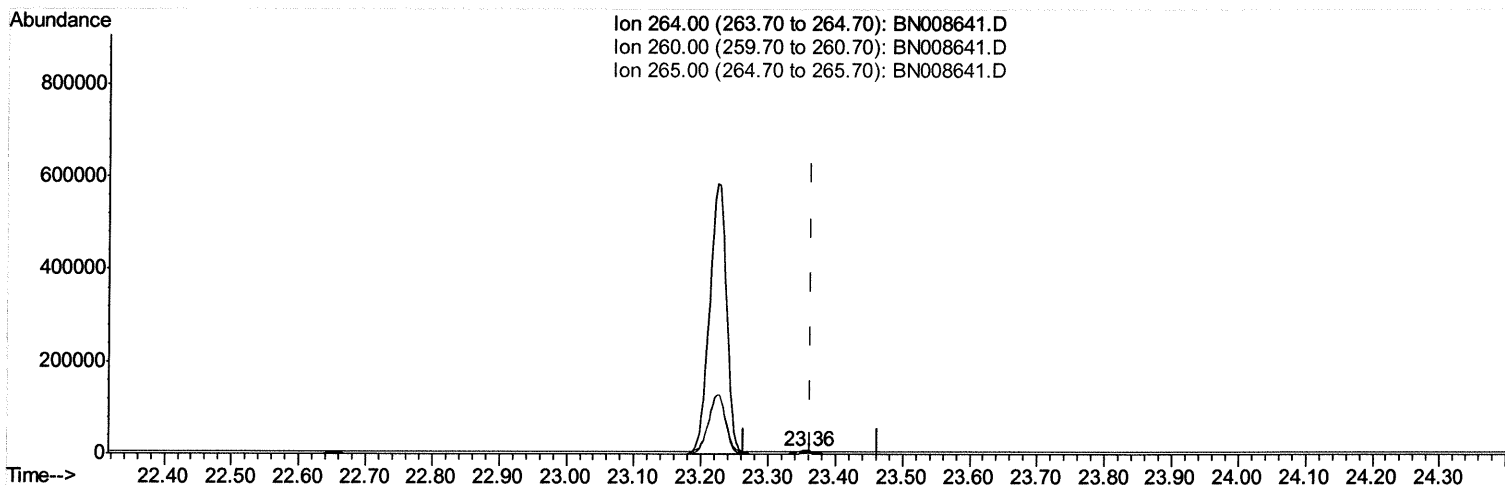

(20) Perylene-d12 (I)

23.358min (-0.006) 0.40ng/ul m

response 12578

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.18
265.00	69.30	84.80#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)

Data File : BN008641.D
Acq On : 19 Nov 2019 21:39
Operator : JU
Sample : K5699-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J11

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:22 AM

Quant Time: Nov 20 04:25:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 03:41:50 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	3418	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	12741	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	7129	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	15003m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	12765	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	12578m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152	6359	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	15464	0.34	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 11/21/19
JU 11/21/19