

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)


Data File : BN008650.D
Acq On : 20 Nov 2019 03:40
Operator : JU
Sample : K5699-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J21

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:45 AM

Quant Time: Nov 20 04:56:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

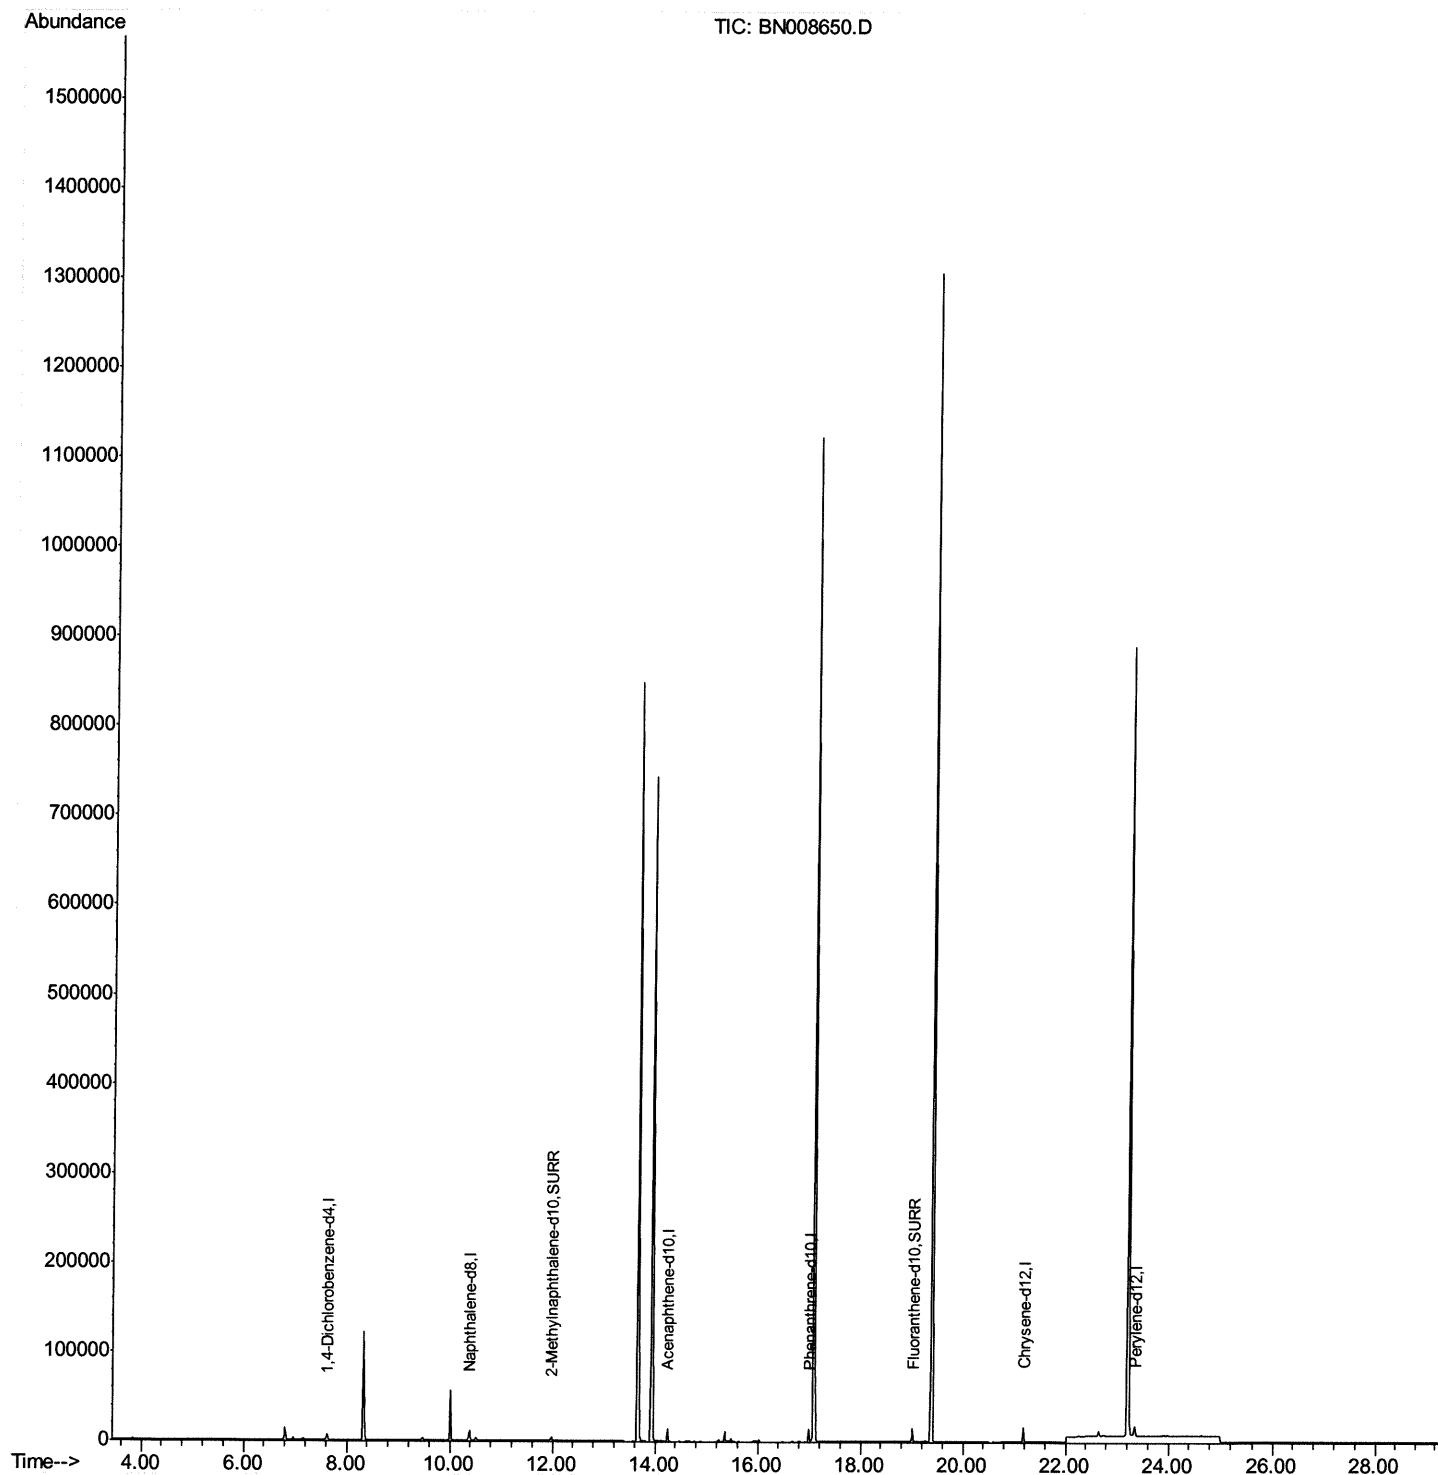

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008650.D
Acq On : 20 Nov 2019 03:40
Operator : JU
Sample : K5699-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J21

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:45 AM

Quant Time: Nov 20 04:49:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

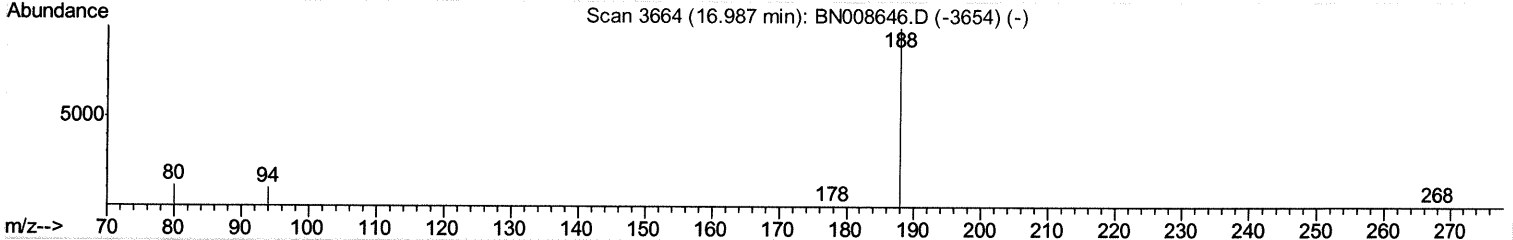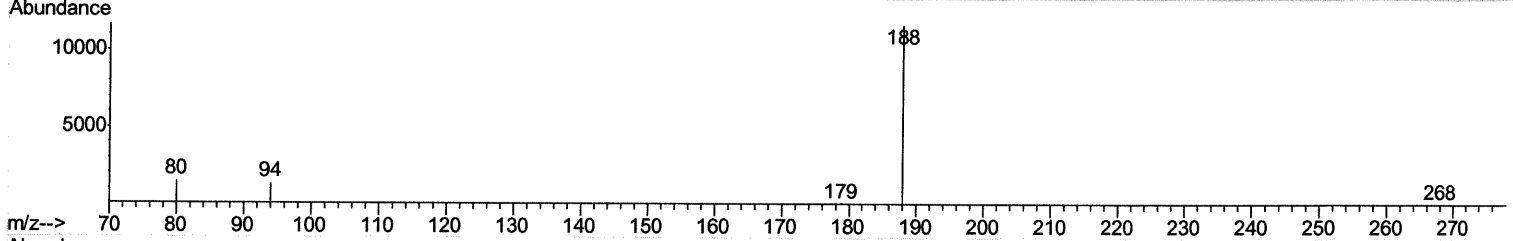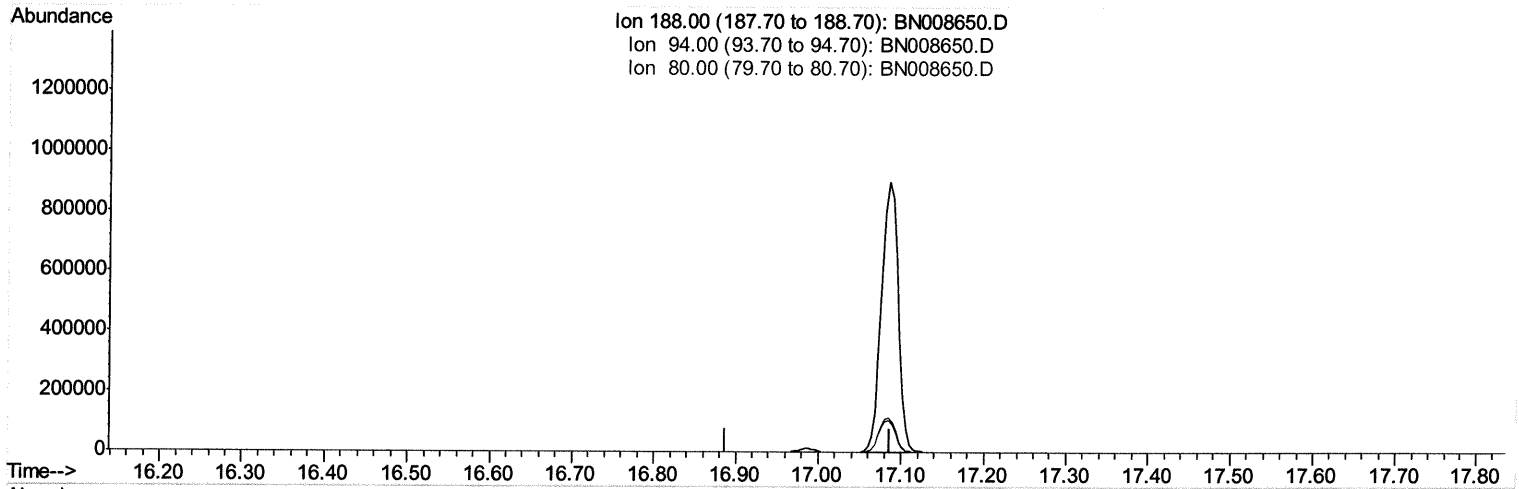

TIC: BN008650.D

(10) Phenanthrene-d10 (I)

16.987min (-16.987) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008650.D
Acq On : 20 Nov 2019 03:40
Operator : JU
Sample : K5699-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J21

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:45 AM

Quant Time: Nov 20 04:49:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

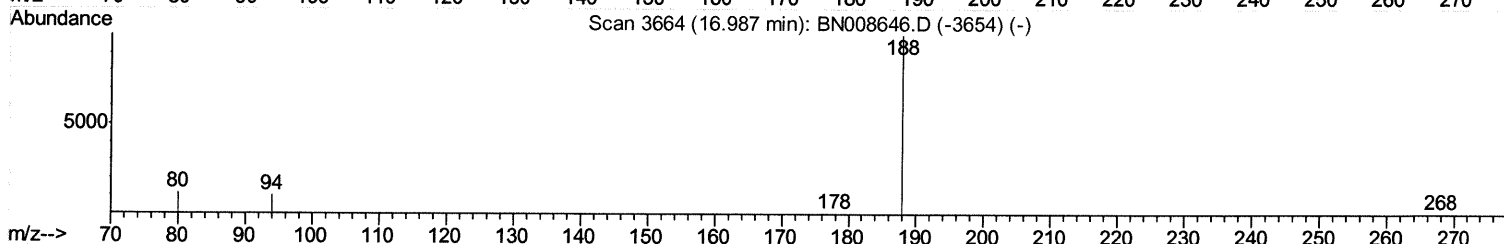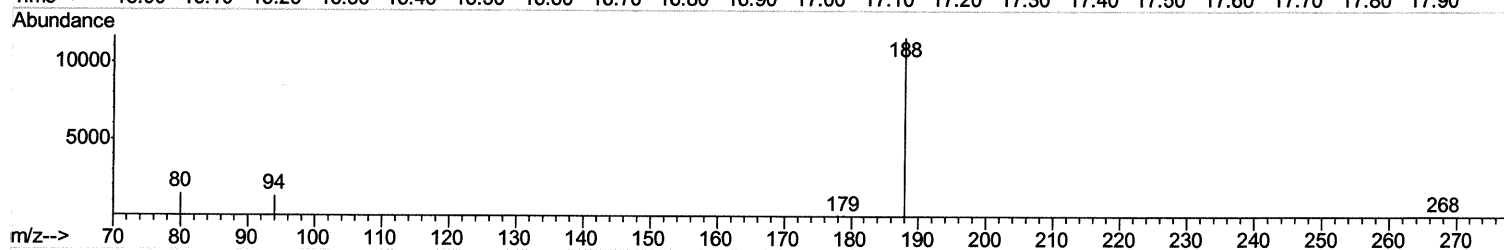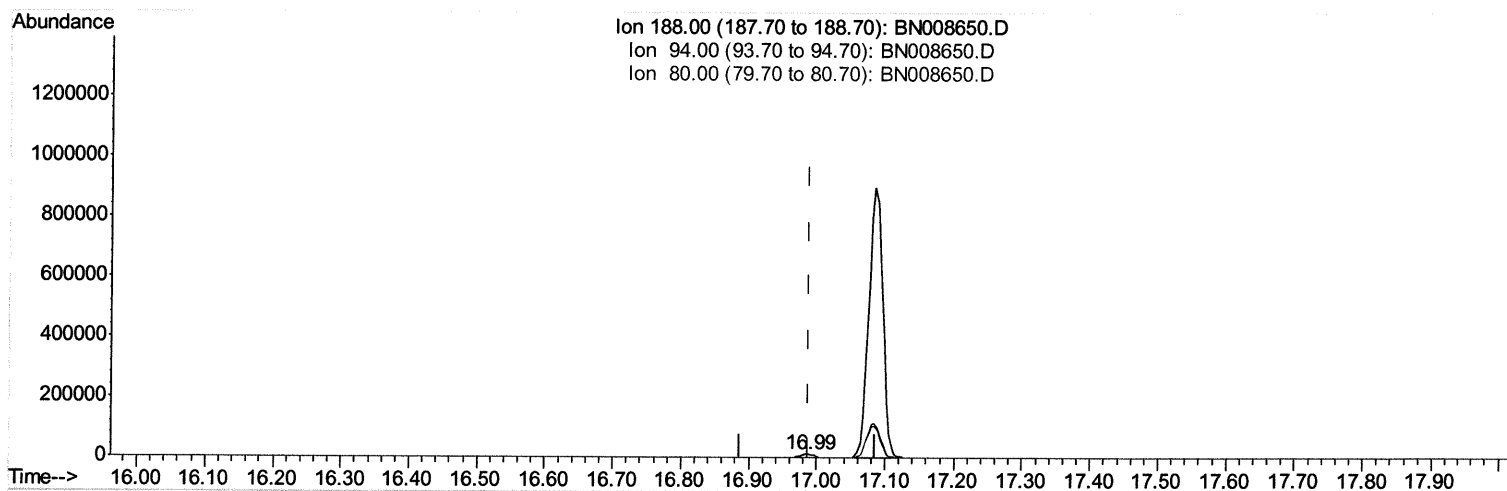

TIC: BN008650.D

(10) Phenanthrene-d10 (I)

16.988min (+0.000) 0.40ng/ul m

response 16542

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	11.46
80.00	11.80	12.96
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008650.D
Acq On : 20 Nov 2019 03:40
Operator : JU
Sample : K5699-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J21

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:45 AM

Quant Time: Nov 20 04:55:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

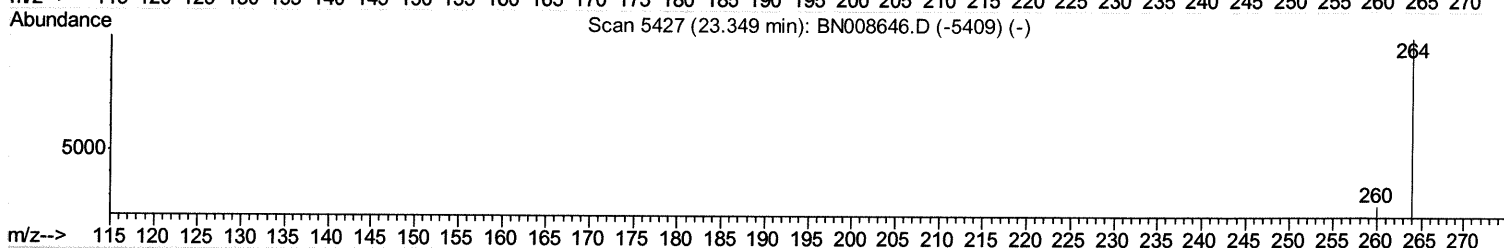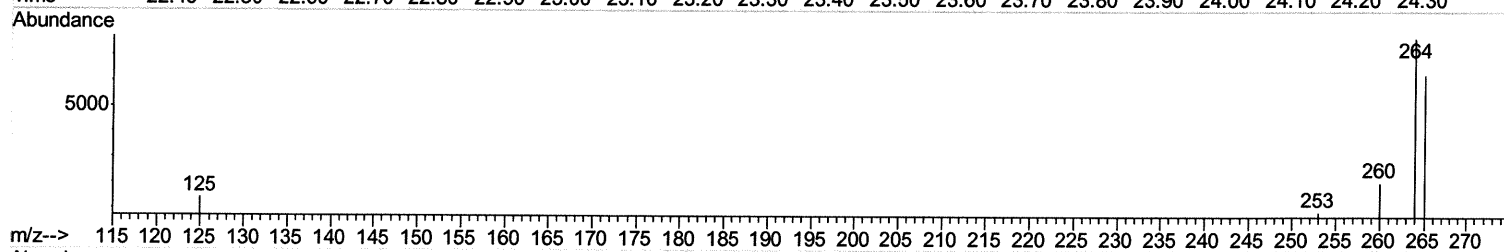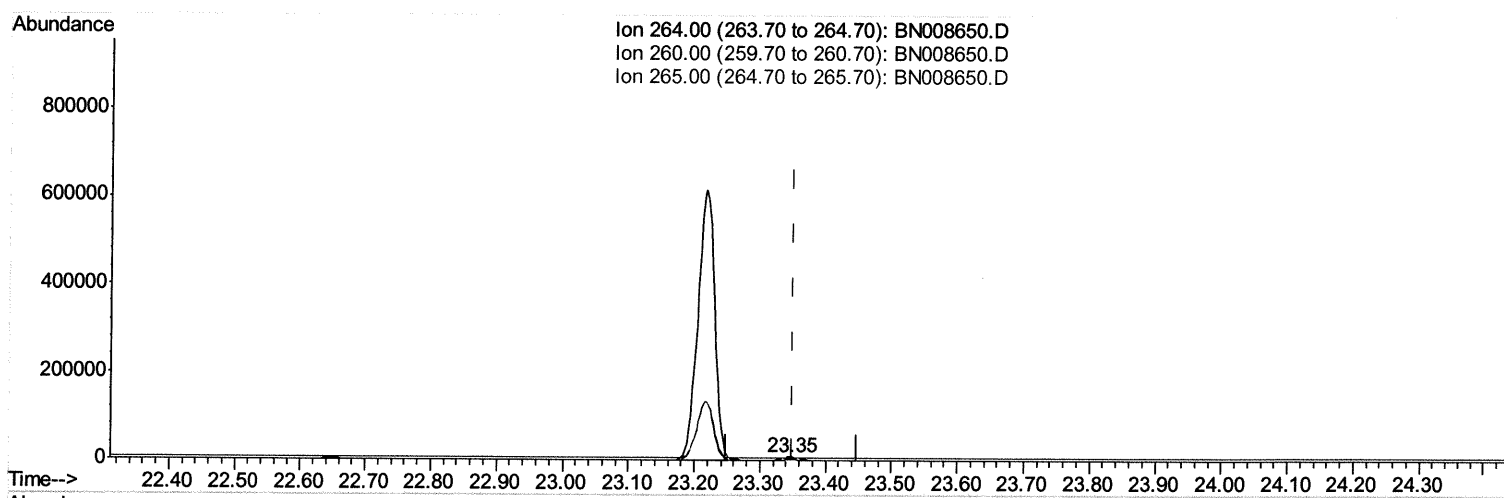

TIC: BN008650.D

(20) Perylene-d12 (I)

23.346min (-0.003) 0.40ng/ul

response 14031

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	26.65
265.00	69.30	80.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (Qedit)




Data File : BN008650.D
Acq On : 20 Nov 2019 03:40
Operator : JU
Sample : K5699-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J21

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:45 AM

Quant Time: Nov 20 04:55:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

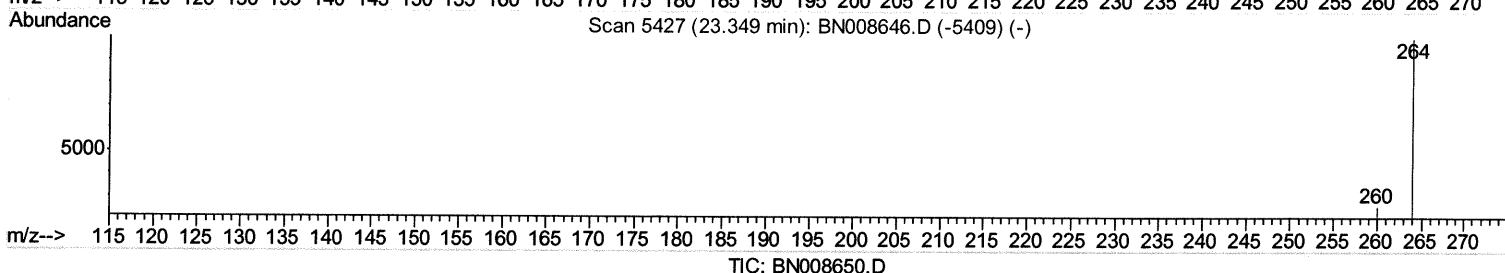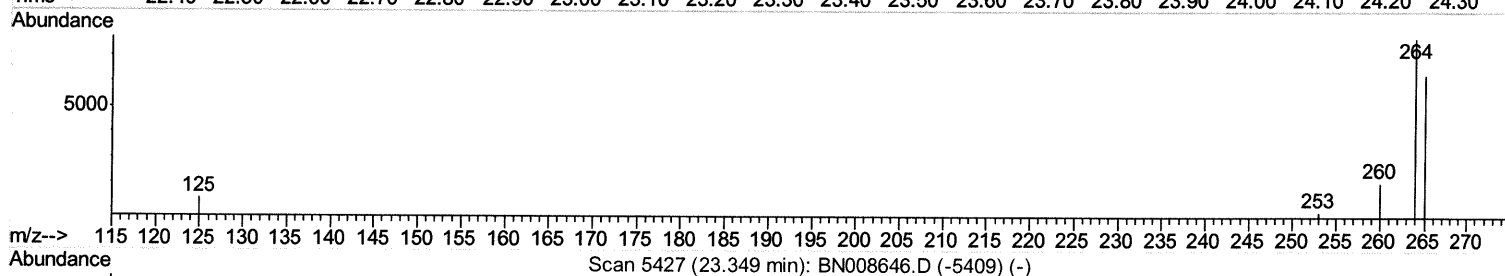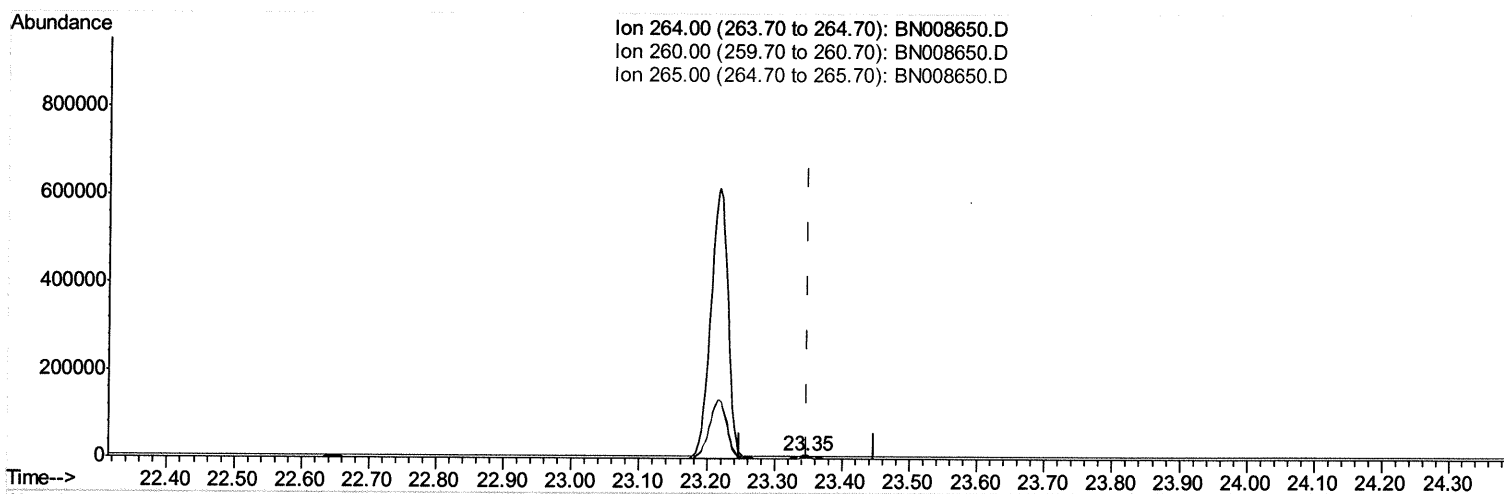

(20) Perylene-d12 (I)

23.346min (-0.003) 0.40ng/ul m

response 13032

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	26.65
265.00	69.30	80.99
0.00	0.00	0.00

JU 11/21/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111919\
Quantitation Report (QT Reviewed)

Data File : BN008650.D
Acq On : 20 Nov 2019 03:40
Operator : JU
Sample : K5699-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F2J21

Manual Integrations
APPROVED

mohammad
11/21/2019 9:05:45 AM

Quant Time: Nov 20 04:56:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 04:45:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	3900	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	14277	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	7977	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	16542m	0.40	ng/ul	0.00
16) Chrysene-d12	21.18	240	13766	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	13032m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.97	152	6418	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	16205	0.32	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 11/21/19
JU 11/21/19