
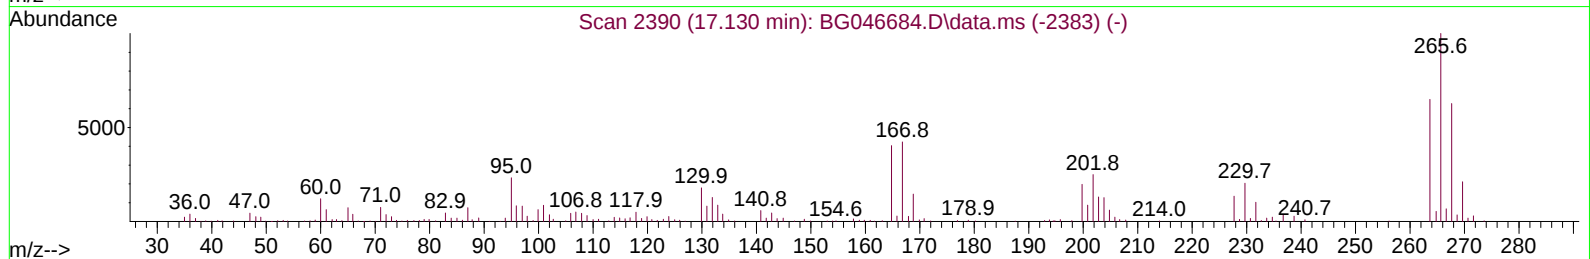
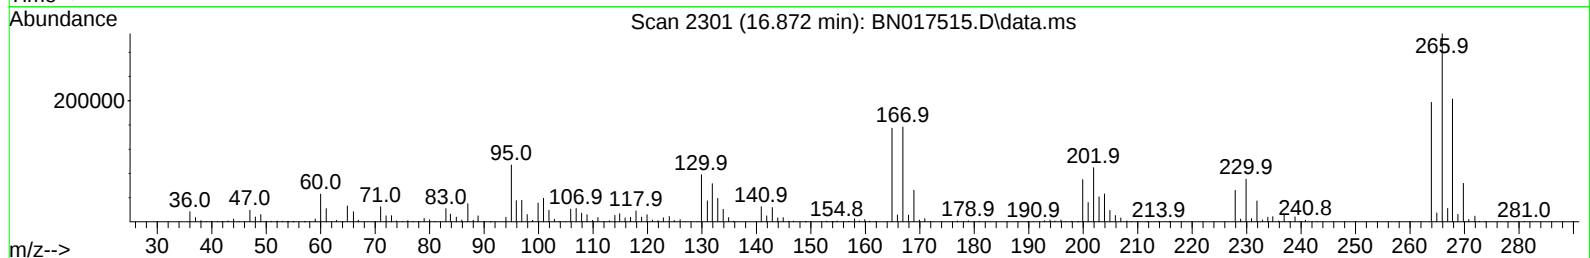


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111921\
 Data File : BN017515.D
 Acq On : 19 Nov 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 11:43:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 19 11:42:56 2021
 Response via : Initial Calibration

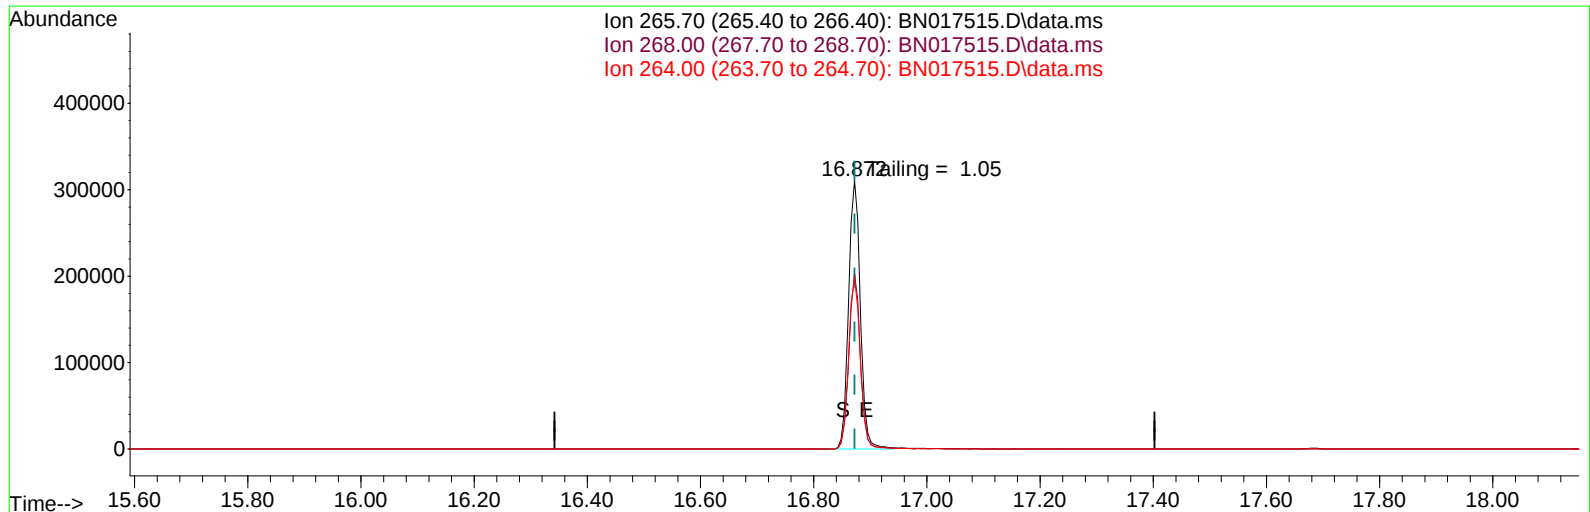

TIC: BN017515.D\data.ms

(70) Pentachlorophenol (C)




16.872min (0.000) 18448.12 ng

response 449530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.31
264.00	61.60	63.56
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111921\  
Data File : BN017515.D  
Acq On    : 19 Nov 2021  09:52  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 19 11:43:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

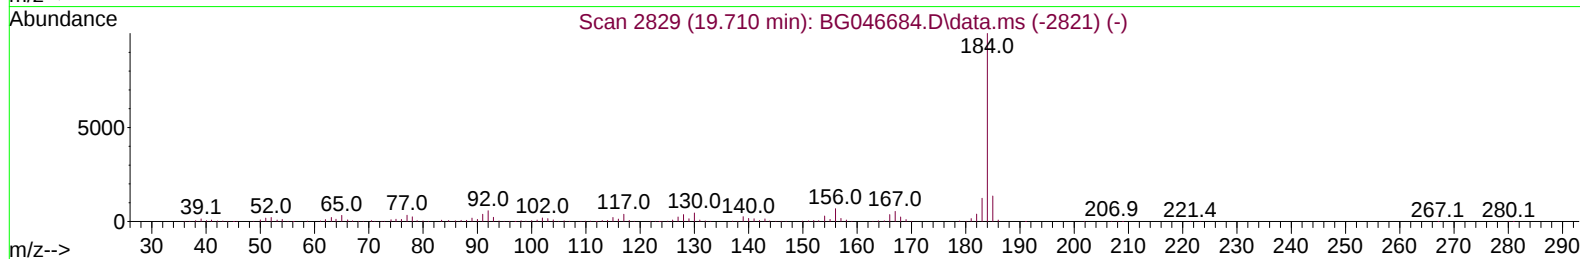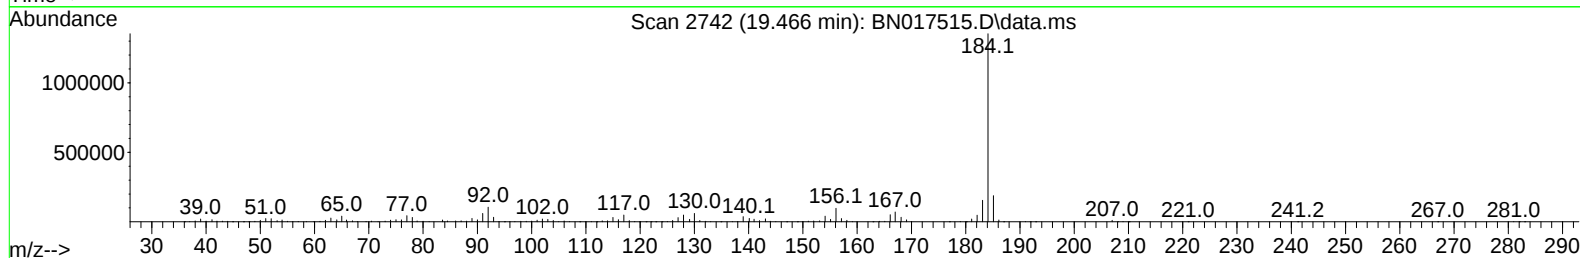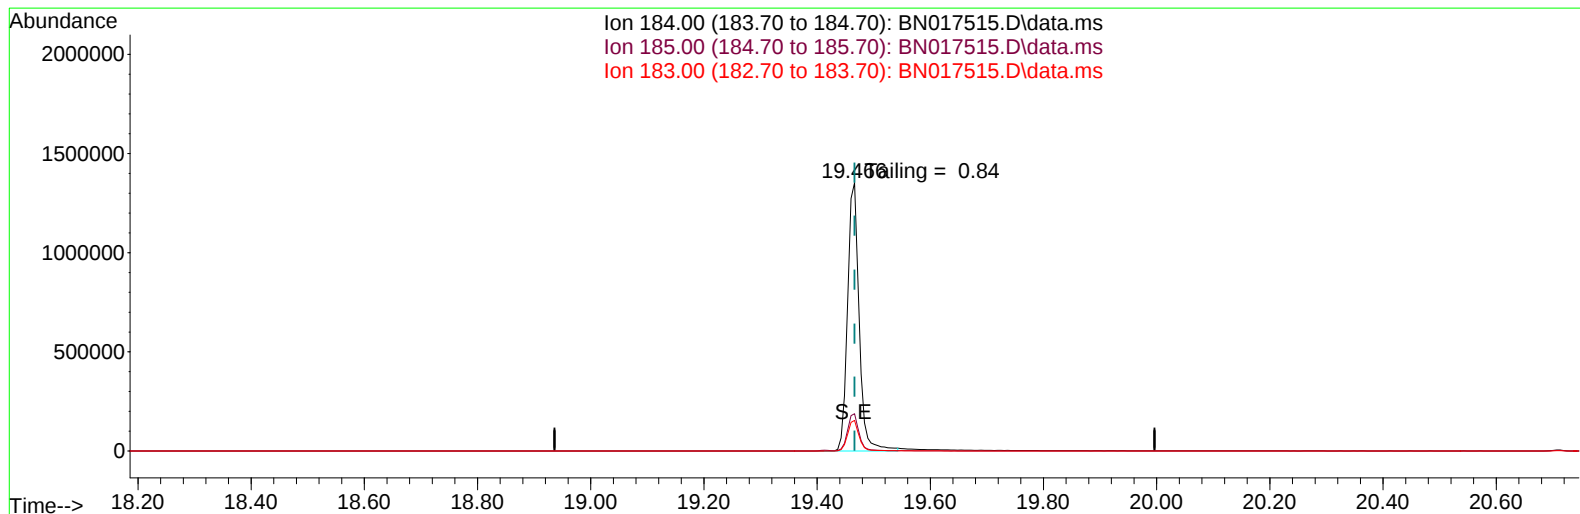

TIC: BN017515.D\data.ms

(77) Benzidine

19.466min (0.000) 0.00 ng

response **1985870**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	11.39
0.00	0.00	0.00