
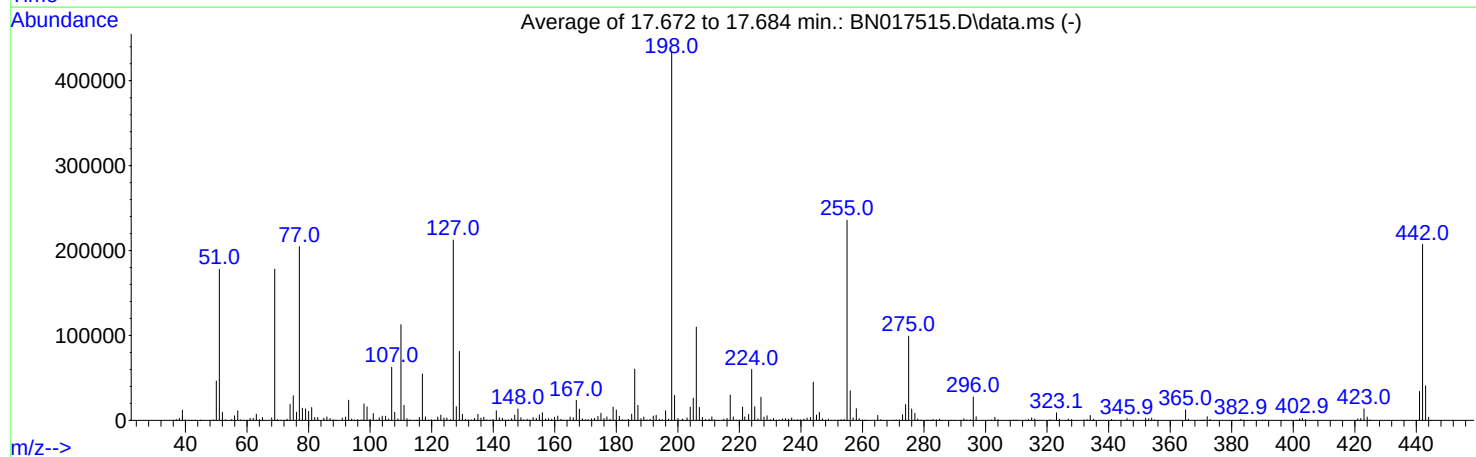


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111921\
 Data File : BN017515.D
 Acq On : 19 Nov 2021 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 19 14:57:14 2021

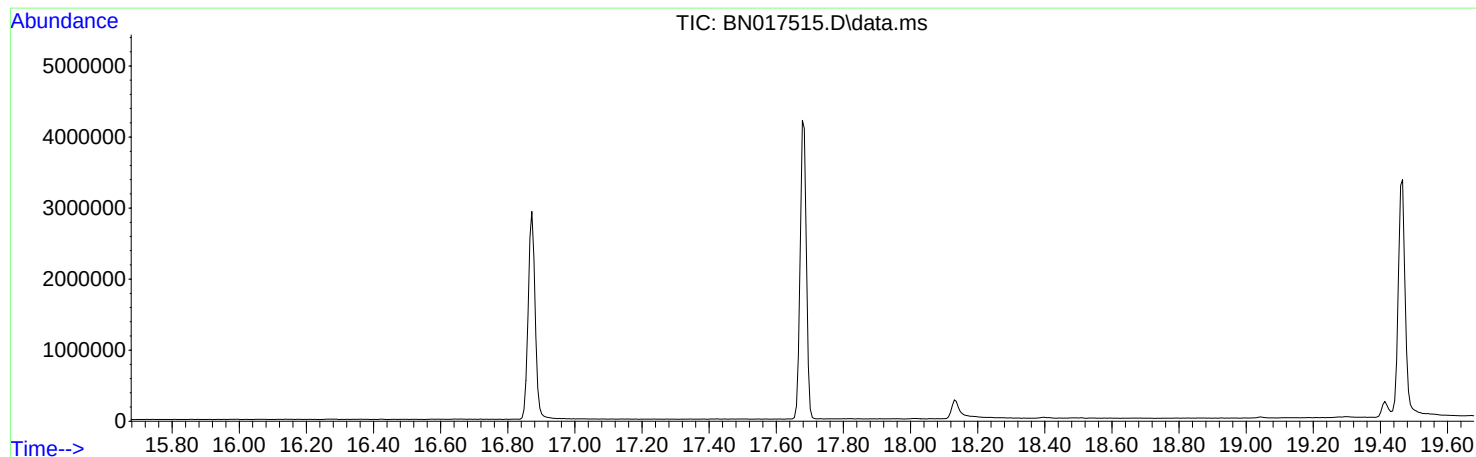




AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	177931	PASS
68	69	0.00	2	1.7	2976	PASS
69	198	0.00	100	41.1	178176	PASS
70	69	0.00	2	0.6	1035	PASS
127	198	10	80	49.0	212352	PASS
197	198	0.00	2	0.3	1456	PASS
198	198	100	100	100.0	433259	PASS
199	198	5	9	6.8	29365	PASS
275	198	10	60	22.9	99168	PASS
365	198	1	100	2.9	12411	PASS
441	198	0.01	100	7.9	34101	PASS
442	442	50	100	100.0	207269	PASS
443	442	15	24	19.6	40651	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111921\
Data File : BN017515.D
Acq On : 19 Nov 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:43:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

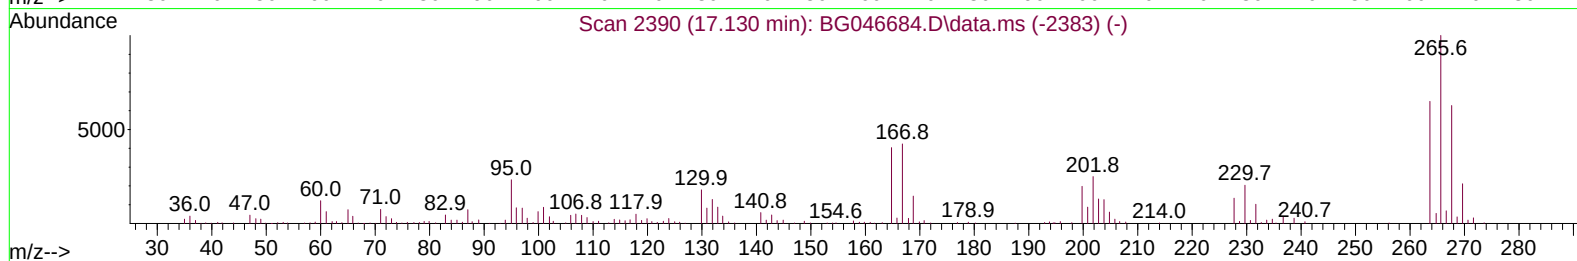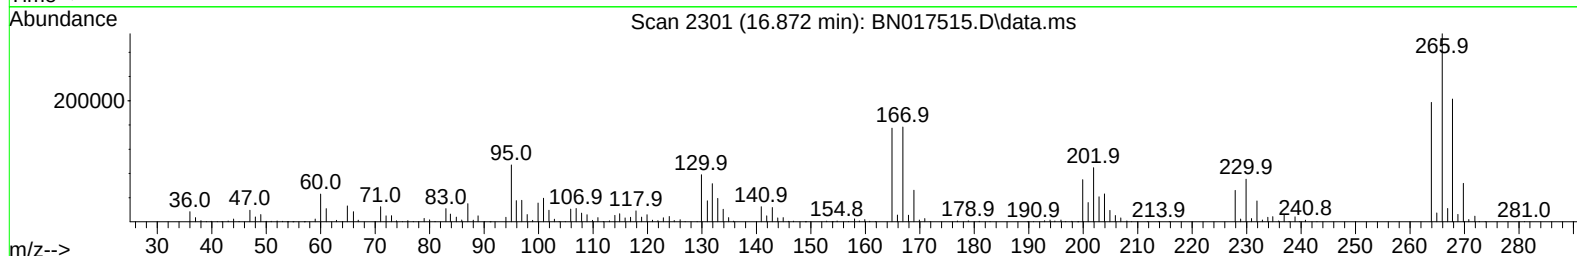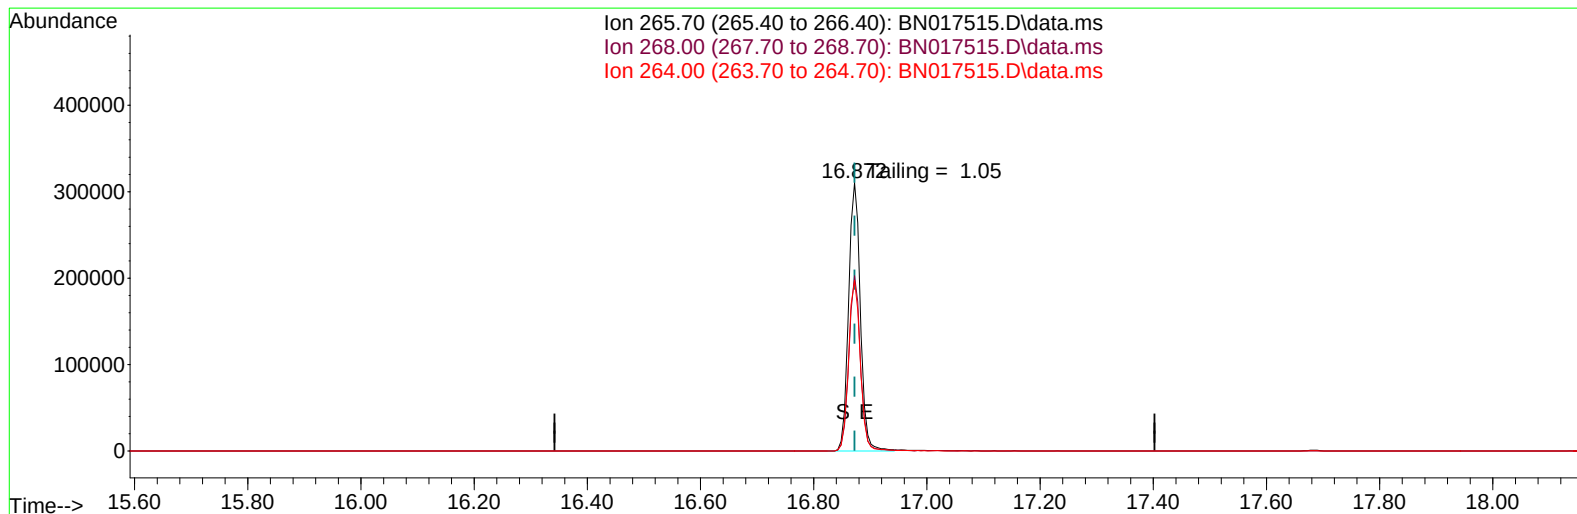

TIC: BN017515.D\data.ms

(70) Pentachlorophenol (C)

16.872min (0.000) 18448.12 ng




response 449530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.31
264.00	61.60	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111921\
Data File : BN017515.D
Acq On : 19 Nov 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:43:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

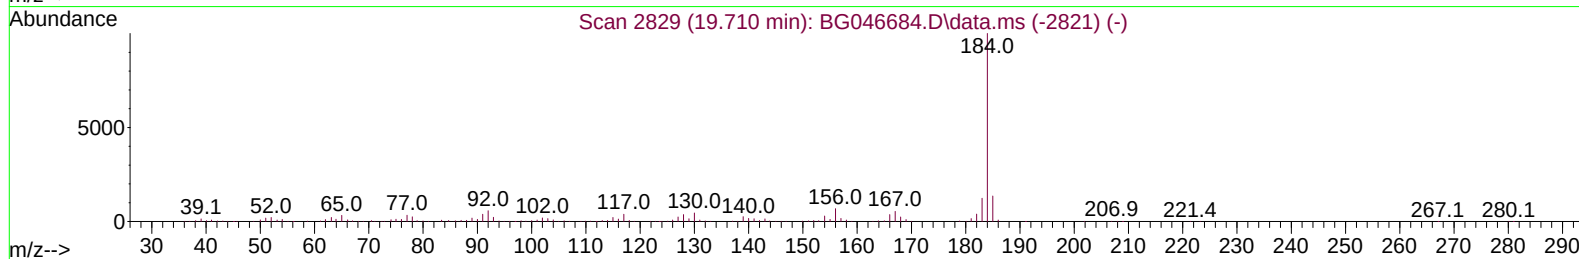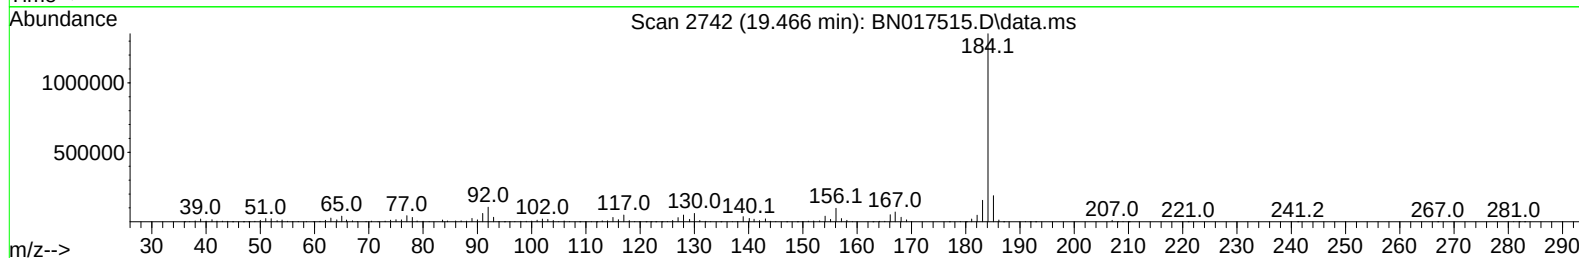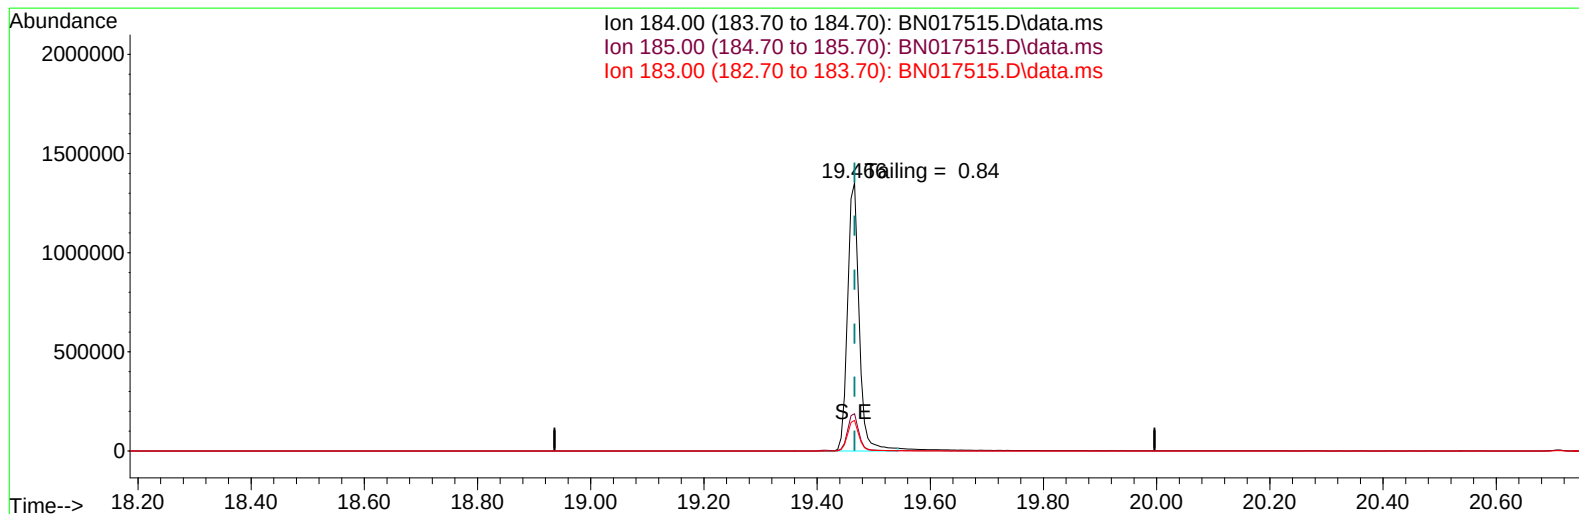

TIC: BN017515.D\data.ms

(77) Benzidine

19.466min (0.000) 0.00 ng

response 1985870

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/19/2021	BNA_N	<u>BN017515.D</u>
Compound Name	Response	Retention Time
DDT	1192518	20.7
DDD	15572	20.26
DDE	157	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15729	1208247	1.30

Instrument :
BNA_N
ClientSampleId :
DFTPP