

Data File : BN003635.D
Acq On : 20 Nov 2018 17:23
Operator : MJ/SJ
Sample : J6001-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40W6

Quant Time: Nov 21 00:12:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6753	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	28076	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	16487	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	2701240	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	33554	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	14541	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	4856	0.064	ng/ul#	12
23) Benzo(a)pyrene	23.56	252	10092	0.084	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003635.D
Acq On : 20 Nov 2018 17:23
Operator : MJ/SJ
Sample : J6001-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40W6

Quant Time: Nov 21 00:12:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration




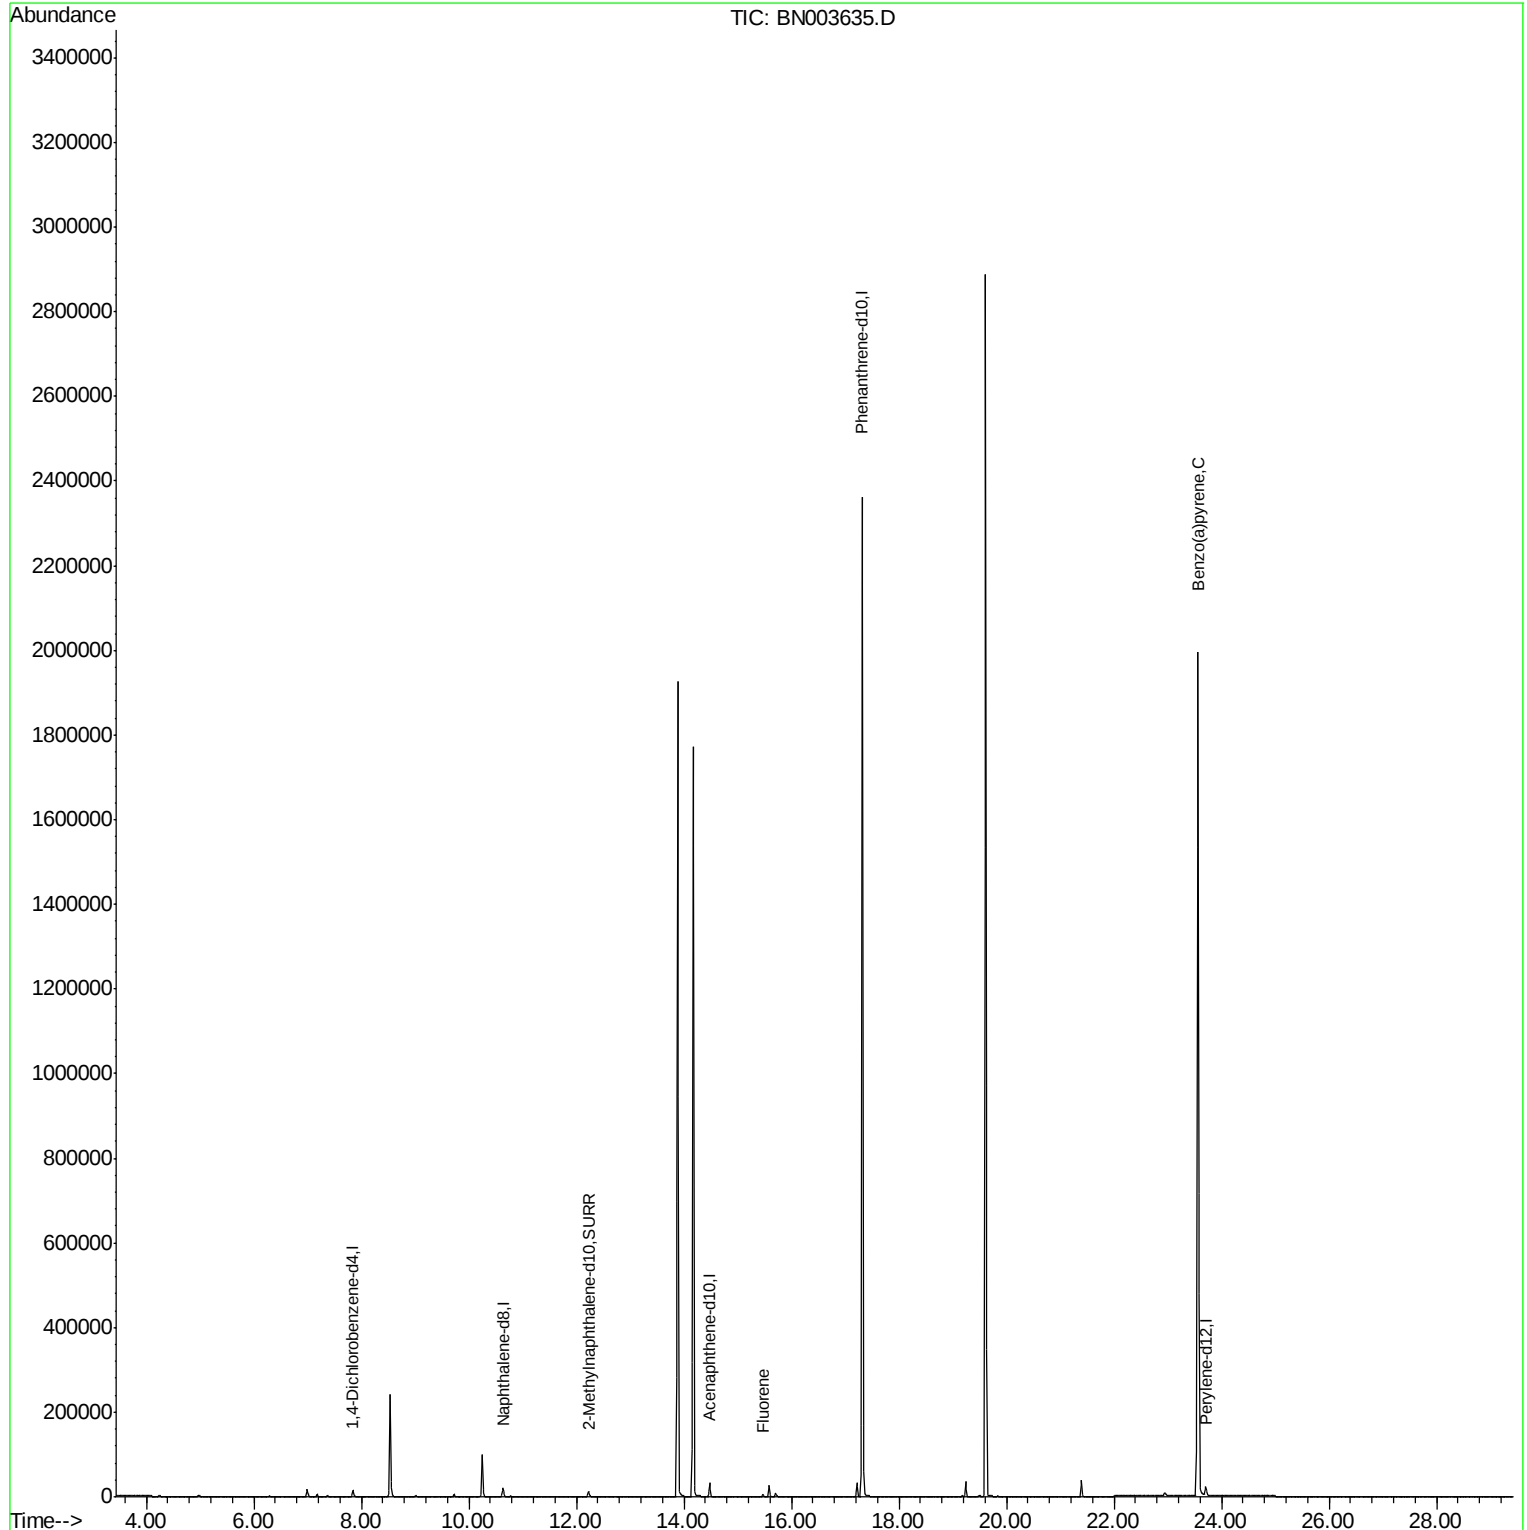


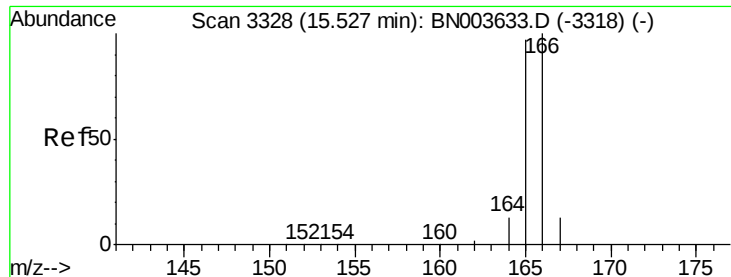

#9
Fluorene
 Concen: 0.064 ng/ul
 RT: 15.47 min Scan# 3316
 Delta R.T. -0.06 min
 Lab File: BN003635.D
 Acq: 20 Nov 2018 17:23

Instrument :
 BNA_N
 ClientSampleId :
 A40W6

Tgt Ion:166 Resp: 4856
 Ion Ratio Lower Upper
 166 100
 165 5.4 78.3 117.5#
 167 35.1 11.3 16.9#

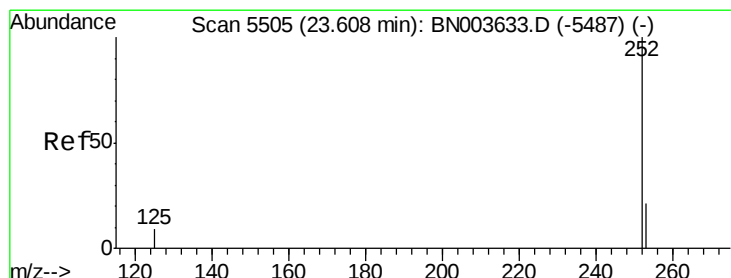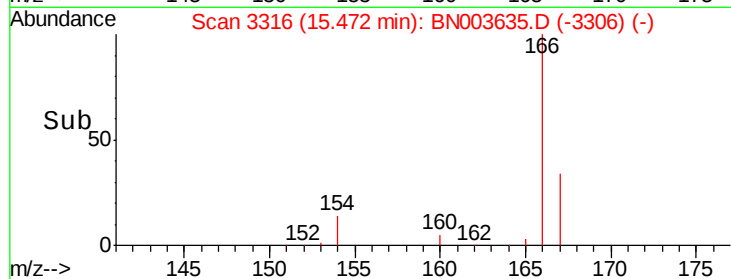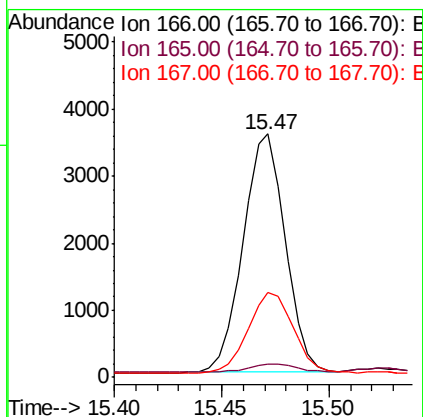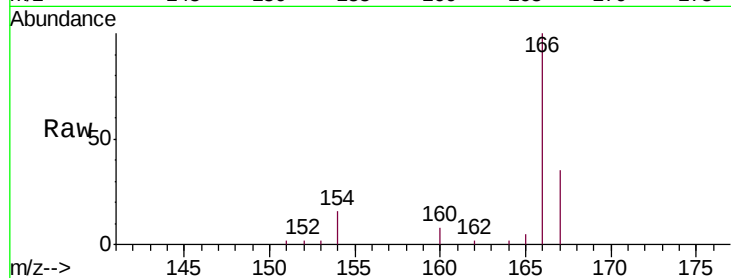

#23
Benzo(a)pyrene
 Concen: 0.084 ng/ul
 RT: 23.56 min Scan# 5490
 Delta R.T. -0.04 min
 Lab File: BN003635.D
 Acq: 20 Nov 2018 17:23

Tgt Ion:252 Resp: 10092
 Ion Ratio Lower Upper
 252 100
 253 34.3 19.0 28.4#
 125 27.5 10.2 15.4#

