

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Not Reviewed)

Data File : BN003638.D
Acq On : 20 Nov 2018 19:08
Operator : MJ/SJ
Sample : J6001-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40X0

Quant Time: Nov 21 00:13:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5917	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	24788	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	14193	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	1986073	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	32588	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	10711	0.28	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.56	252	8121	0.070	ng/ul#	Qvalue 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003638.D
Acq On : 20 Nov 2018 19:08
Operator : MJ/SJ
Sample : J6001-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40X0

Quant Time: Nov 21 00:13:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

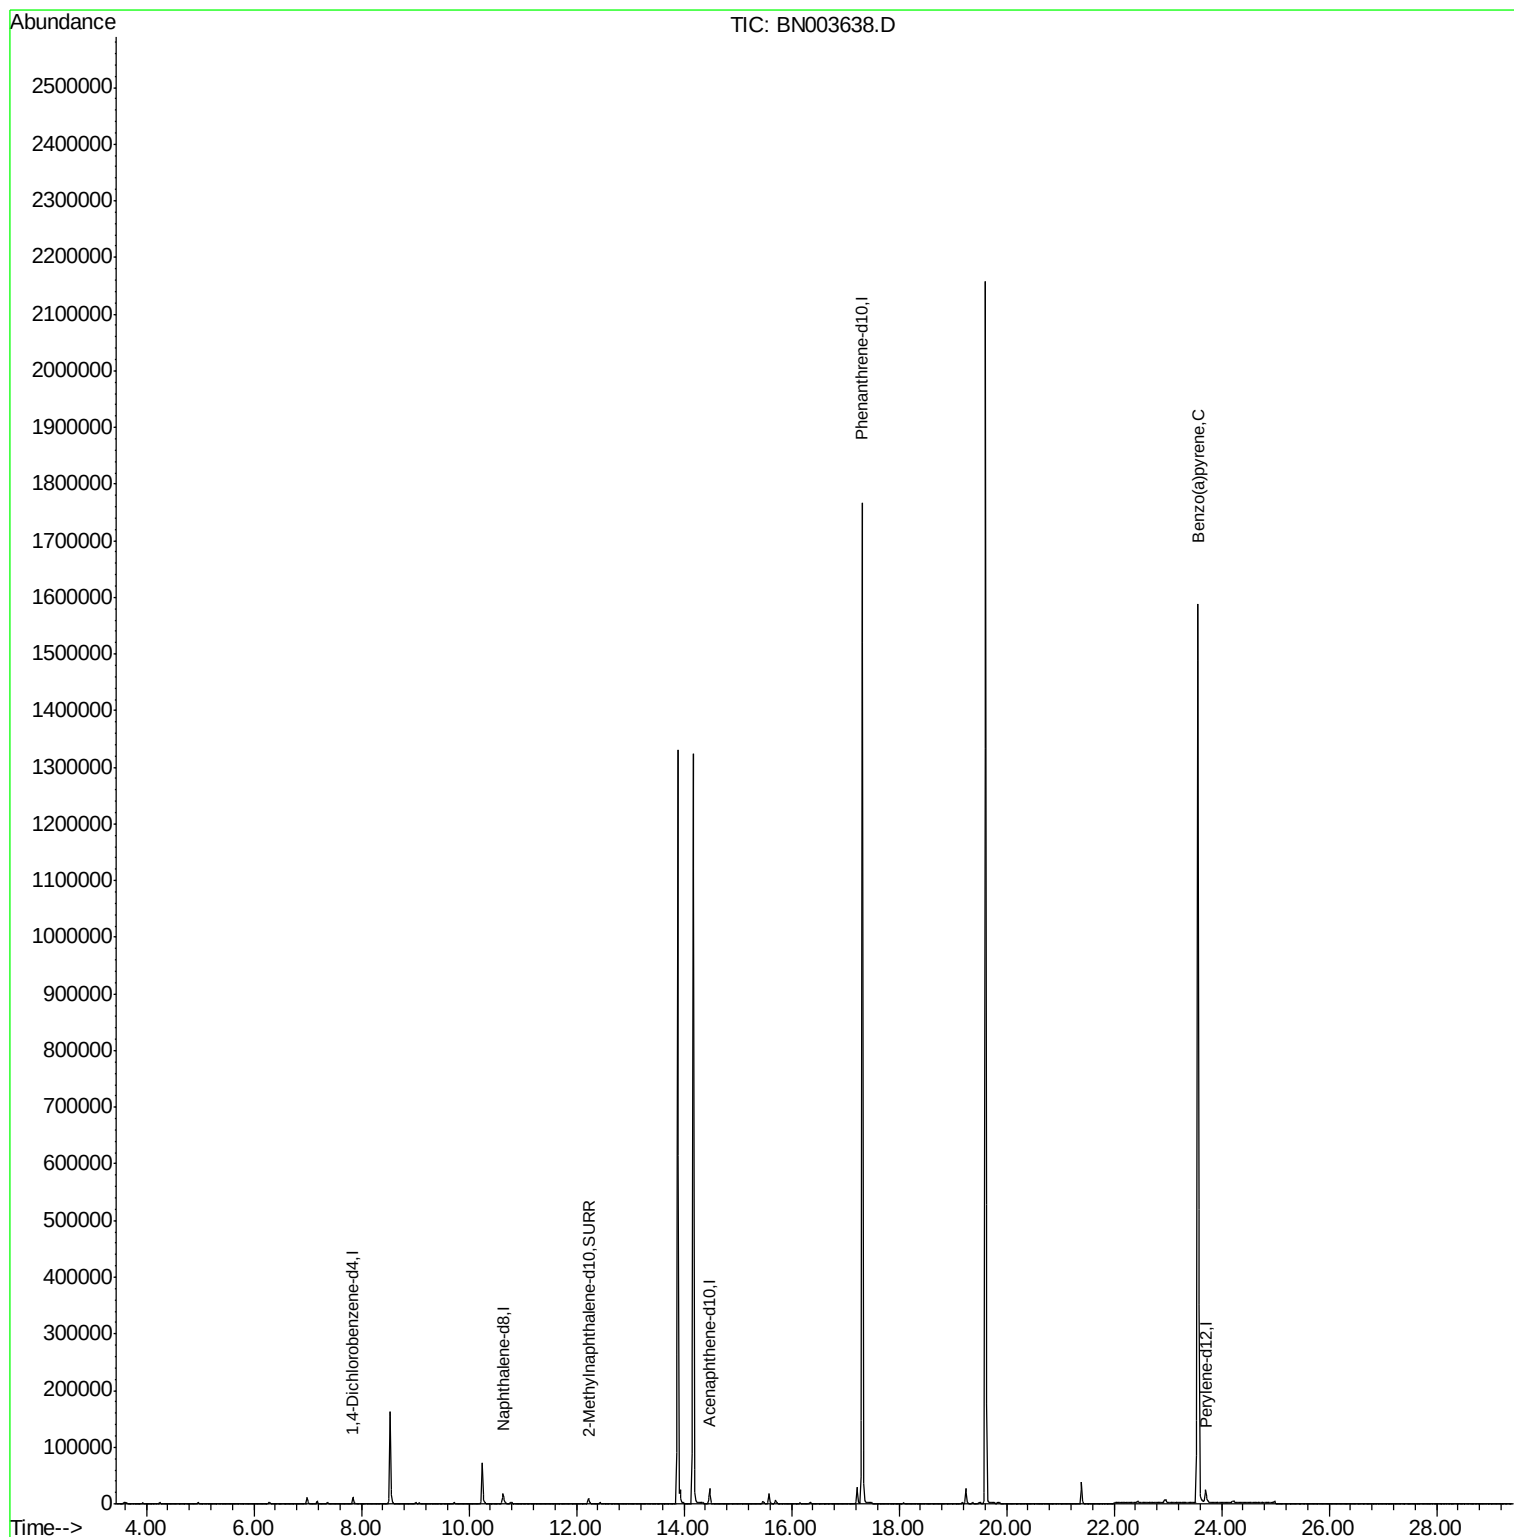

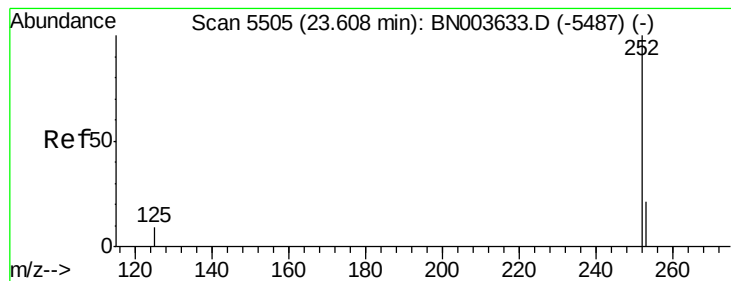

#23

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.56 min Scan# 5489

Delta R.T. -0.05 min

Lab File: BN003638.D


Acq: 20 Nov 2018 19:08

Instrument :

BNA_N

ClientSampleId :

A40X0

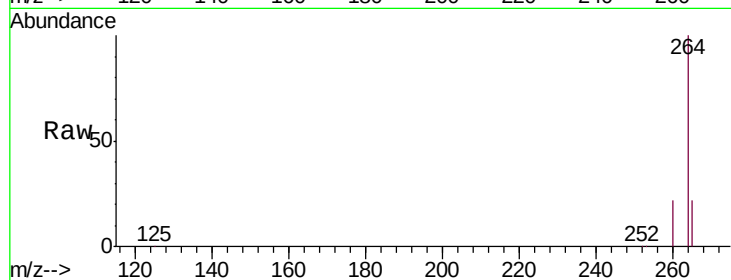

Tgt Ion: 252 Resp: 8121

Ion Ratio Lower Upper

252 100

253 37.1 19.0 28.4#

125 37.8 10.2 15.4#

