

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Not Reviewed)

Data File : BN003639.D
Acq On : 20 Nov 2018 19:43
Operator : MJ/SJ
Sample : J6001-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y2

Quant Time: Nov 21 00:13:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6173	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	26023	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	14478	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	33888	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	33599	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	32169	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	4895	0.12	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	12823	0.13	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.56	252	3920	0.034	ng/ul#	Qvalue 16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003639.D
Acq On : 20 Nov 2018 19:43
Operator : MJ/SJ
Sample : J6001-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y2

Quant Time: Nov 21 00:13:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

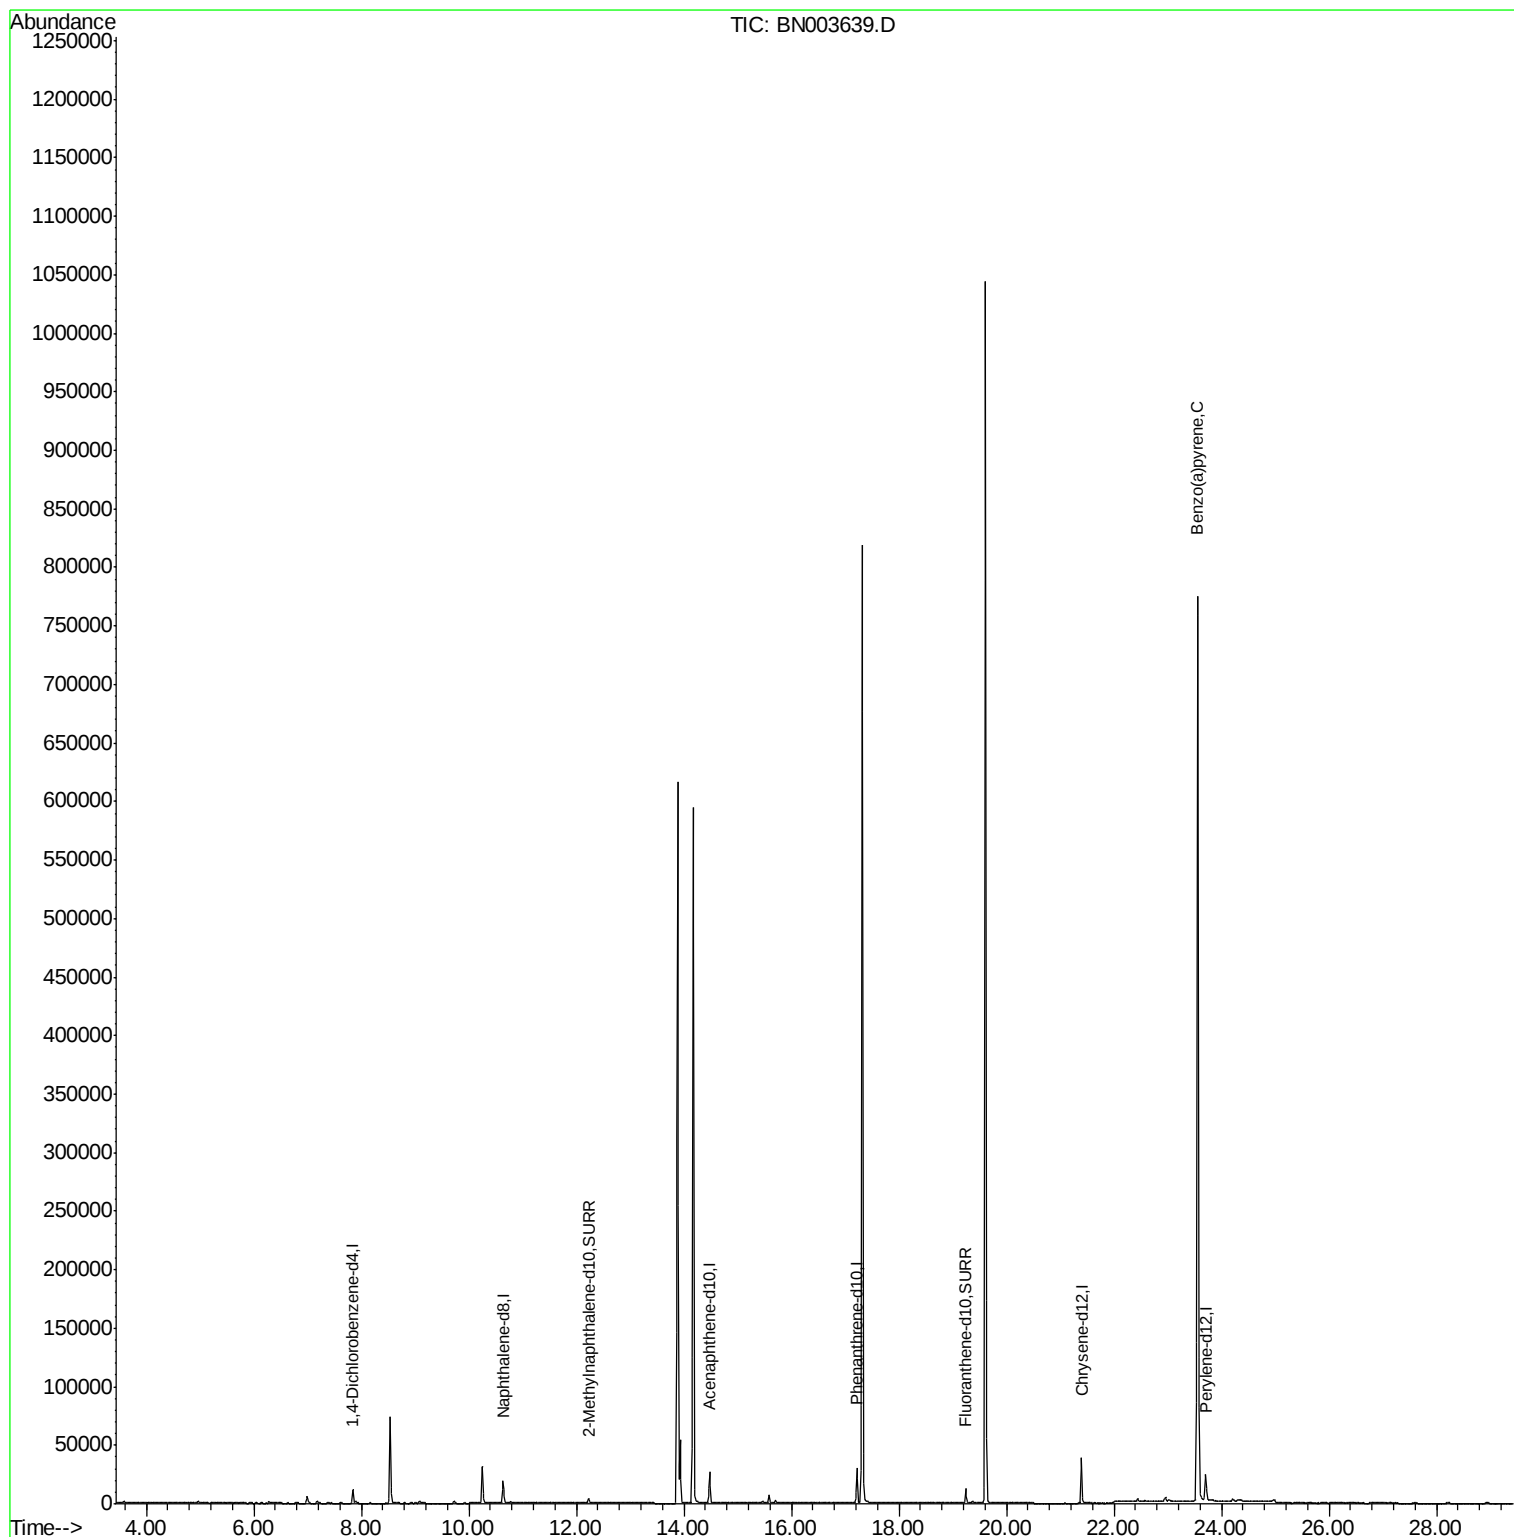

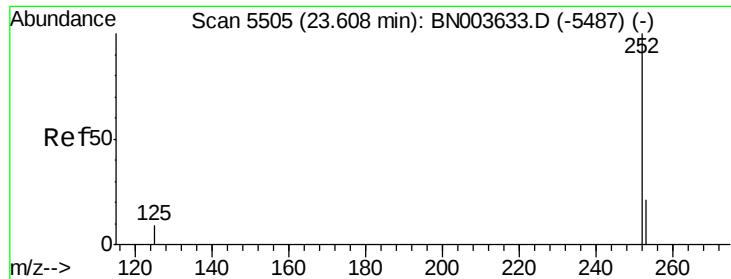

#23

Benzo(a)pyrene

Concen: 0.034 ng/ul

RT: 23.56 min Scan# 5487

Delta R.T. -0.05 min

Lab File: BN003639.D

Acq: 20 Nov 2018 19:43

Instrument :

BNA_N

ClientSampleId :

A40Y2

Tgt Ion: 252 Resp: 3920

Ion Ratio Lower Upper

252 100

253 50.2 19.0 28.4#

125 67.7 10.2 15.4#

