

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\

Quantitation Report (QT Reviewed)

Data File : BN003636.D

Acq On : 20 Nov 2018 17:58

Operator : MJ/SJ

Sample : J6001-07

Misc :

ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:24:21 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Nov 21 00:09:42 2018

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


A40T8

Manual Integrations

APPROVED

Sohil

11/21/2018 5:22:31 PM

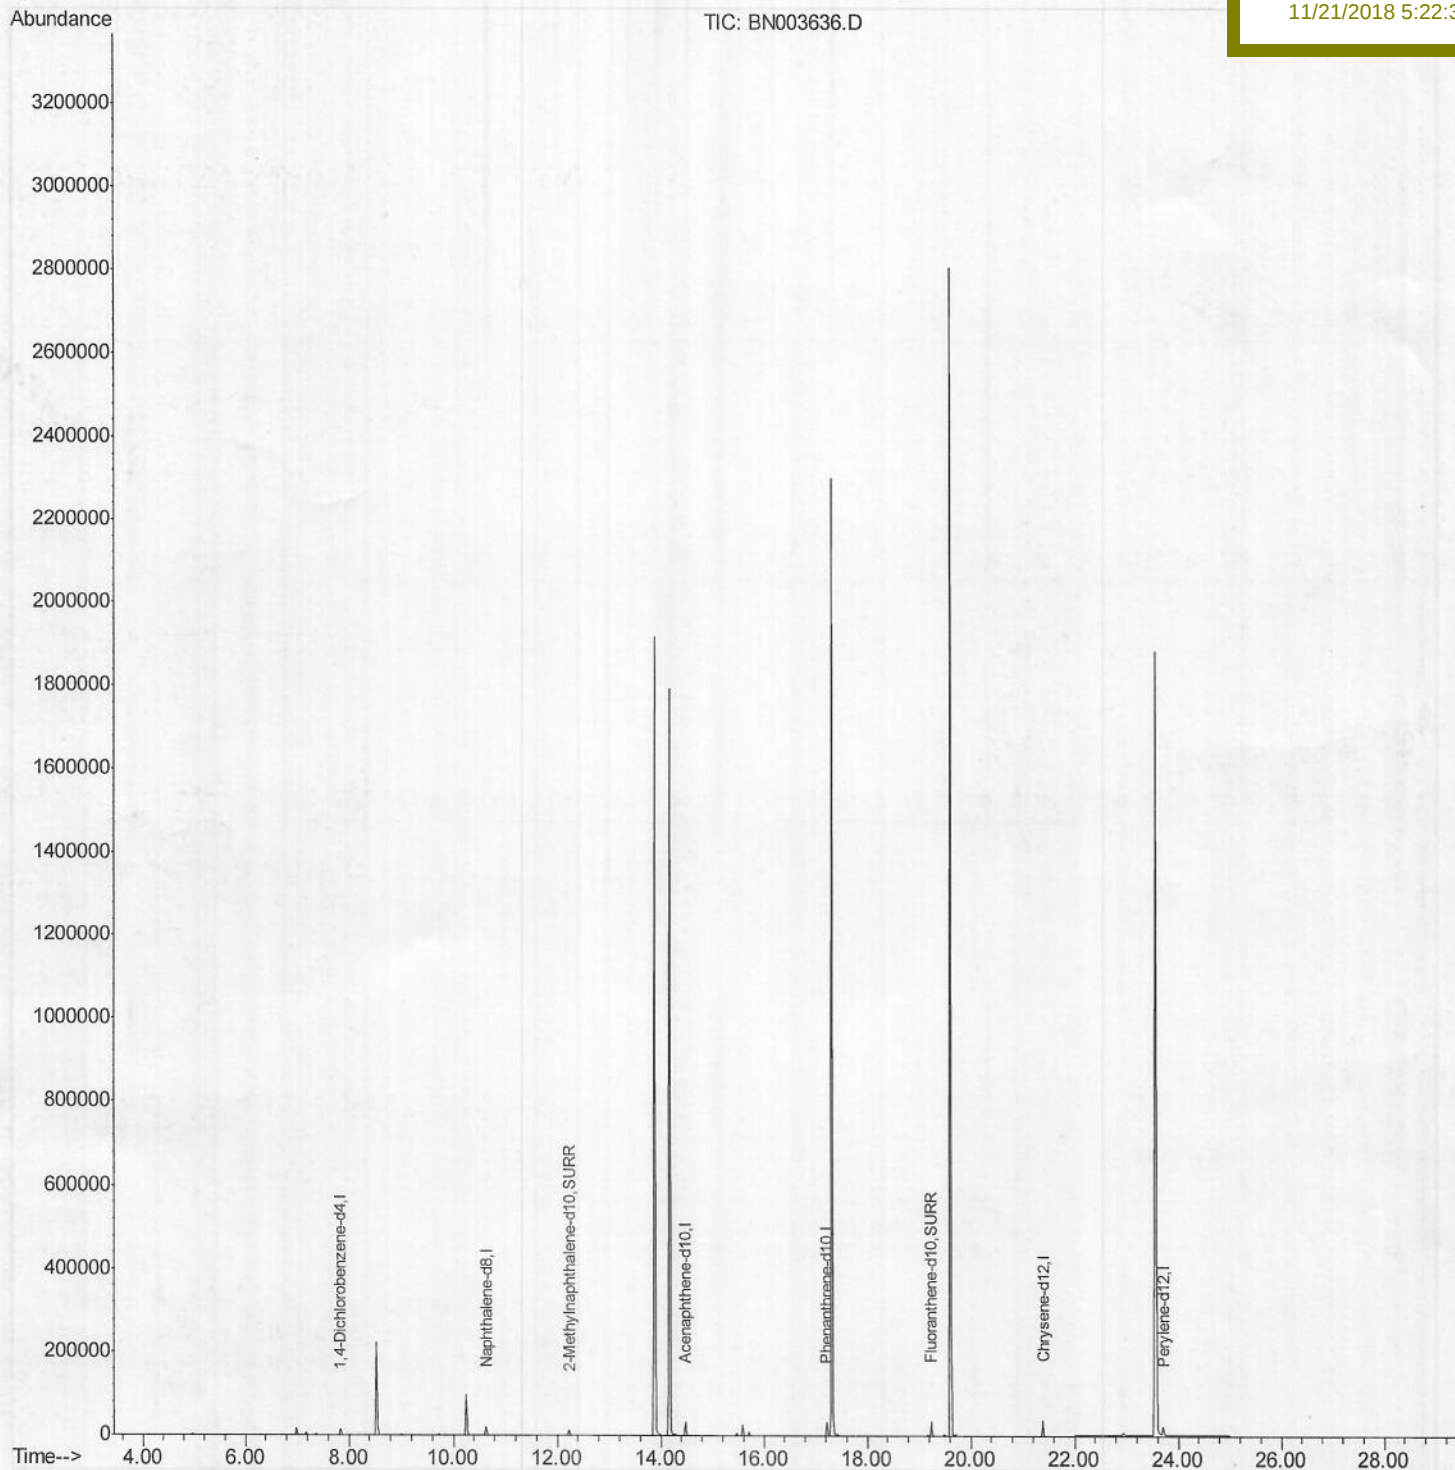

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:12:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

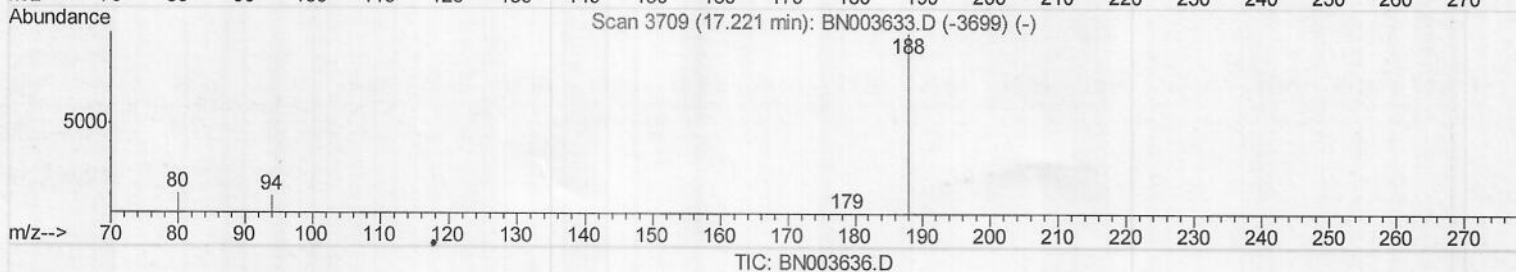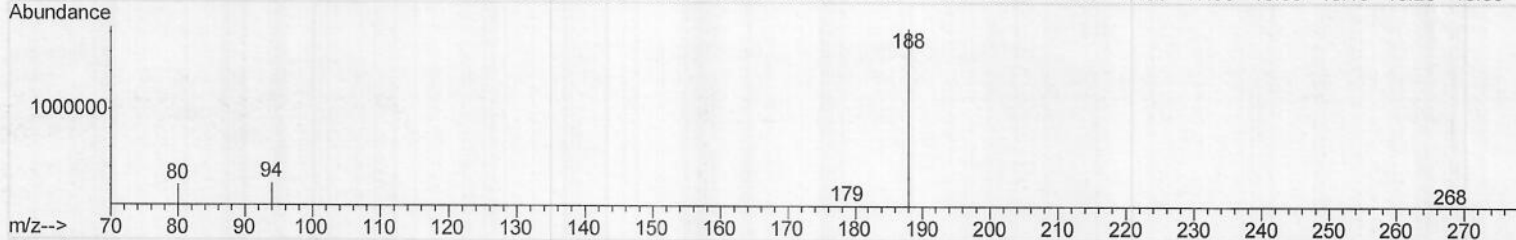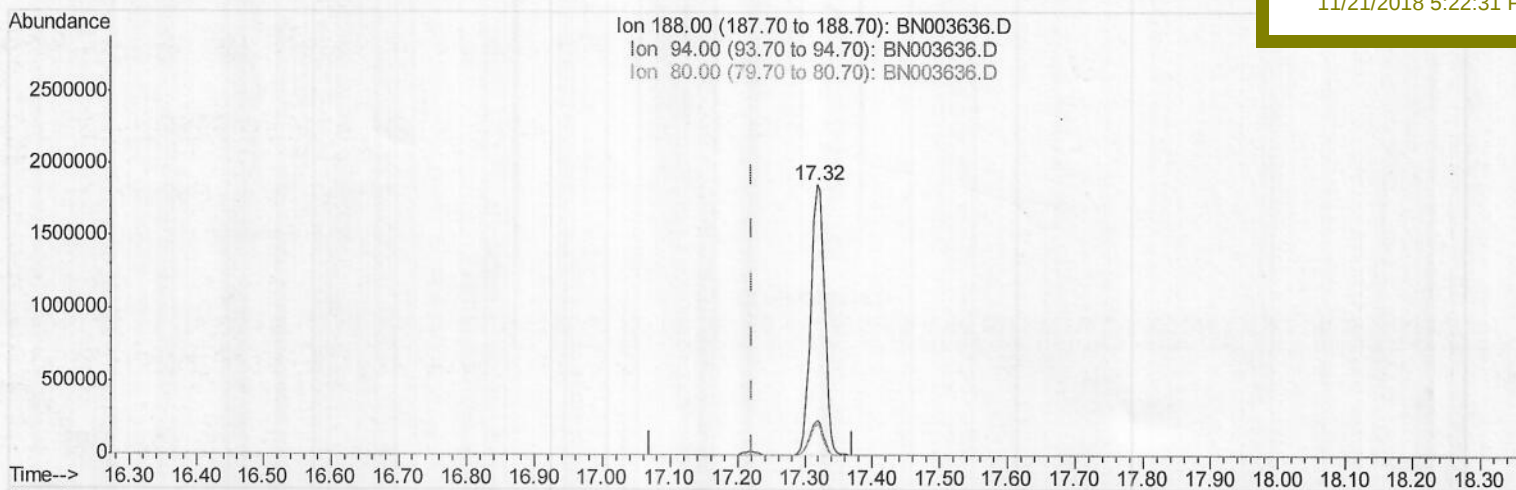

(10) Phenanthrene-d10 (I)
17.318min (+0.097) 0.40ng/ul
response 2633629

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.60#
80.00	11.60	11.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)


Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:12:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

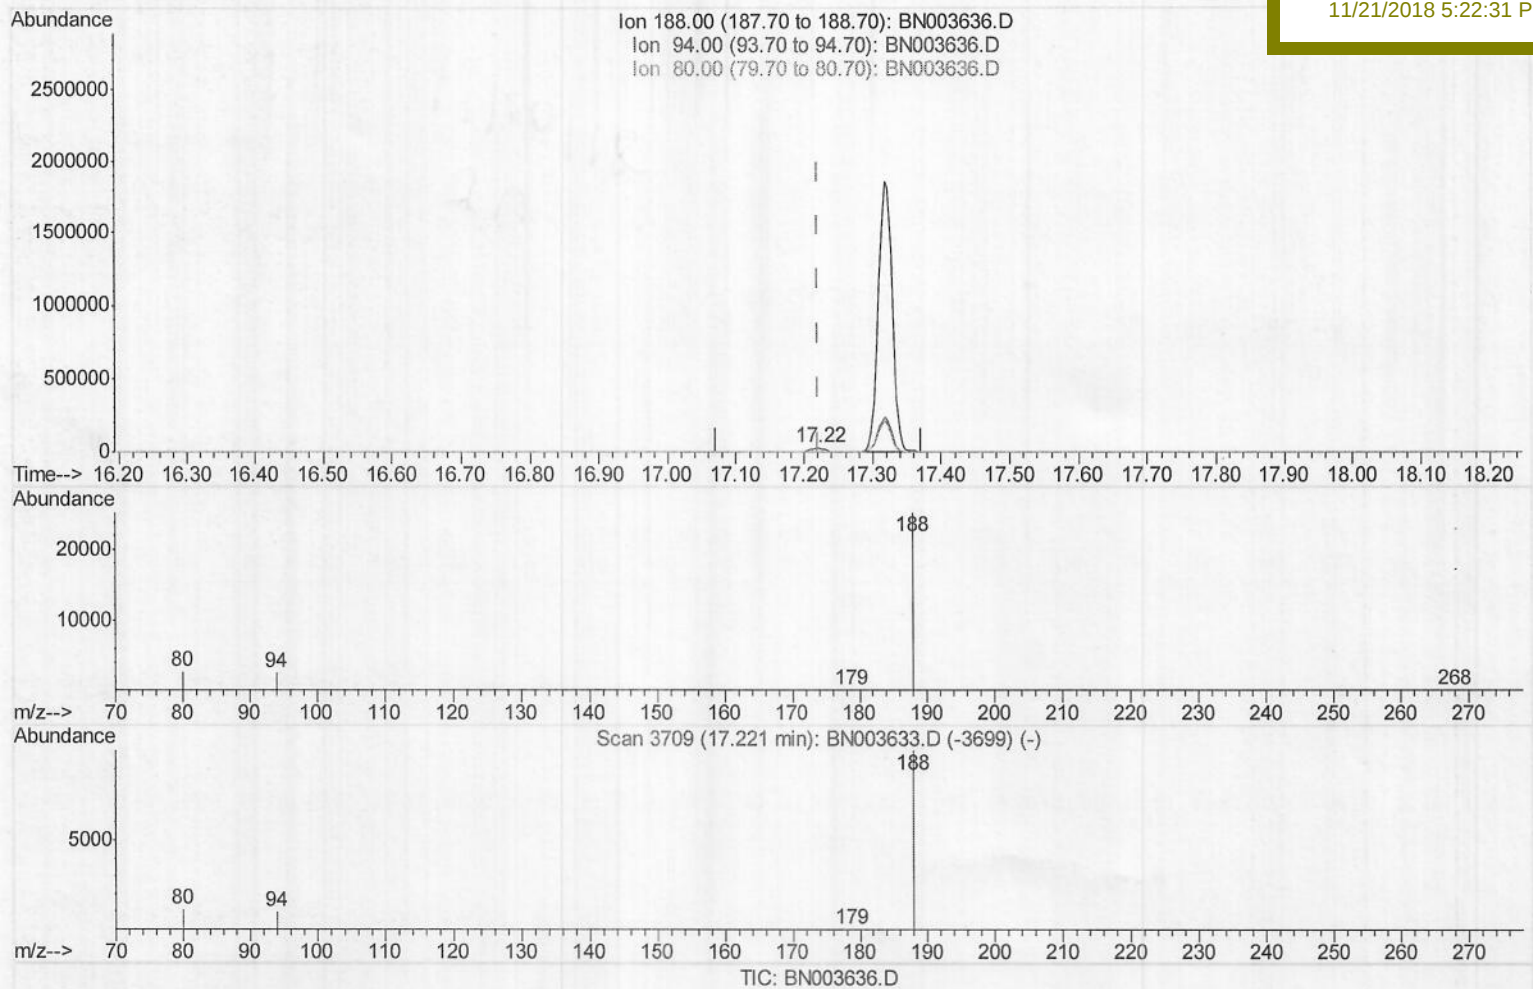

(10) Phenanthrene-d10 (I)

17.221min (+0.000) 0.40ng/ul m

response 35506

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.86
80.00	11.60	10.80
0.00	0.00	0.00

JU
11/20/18




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:22:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

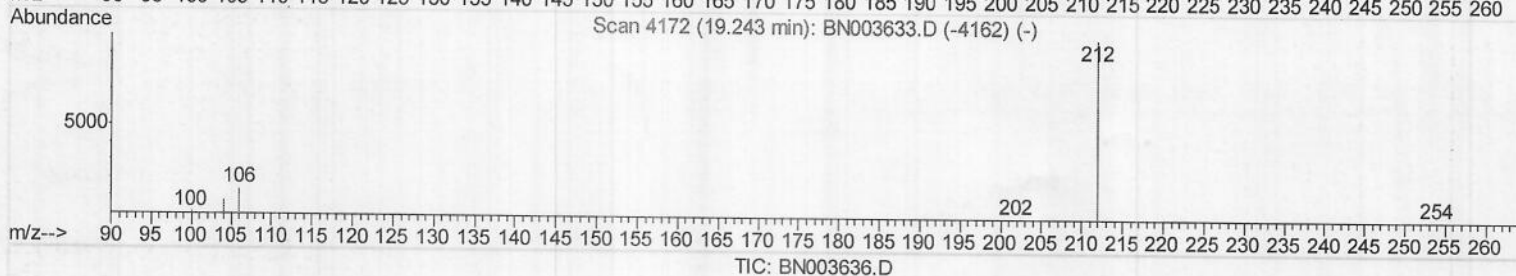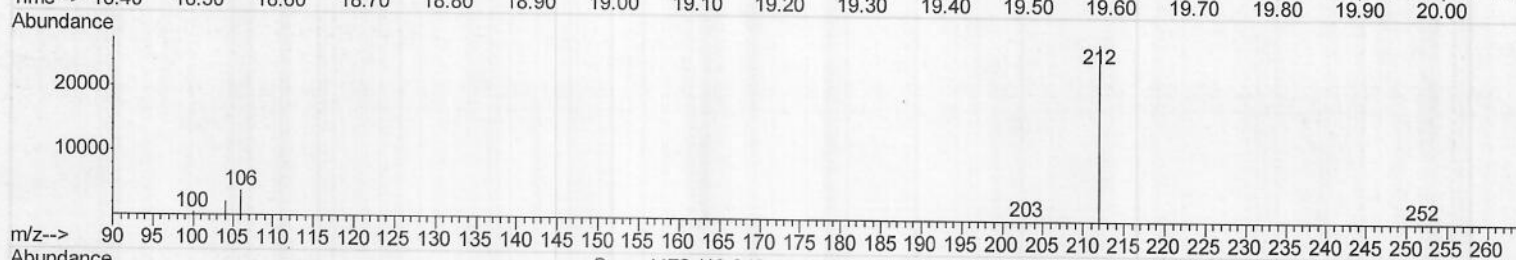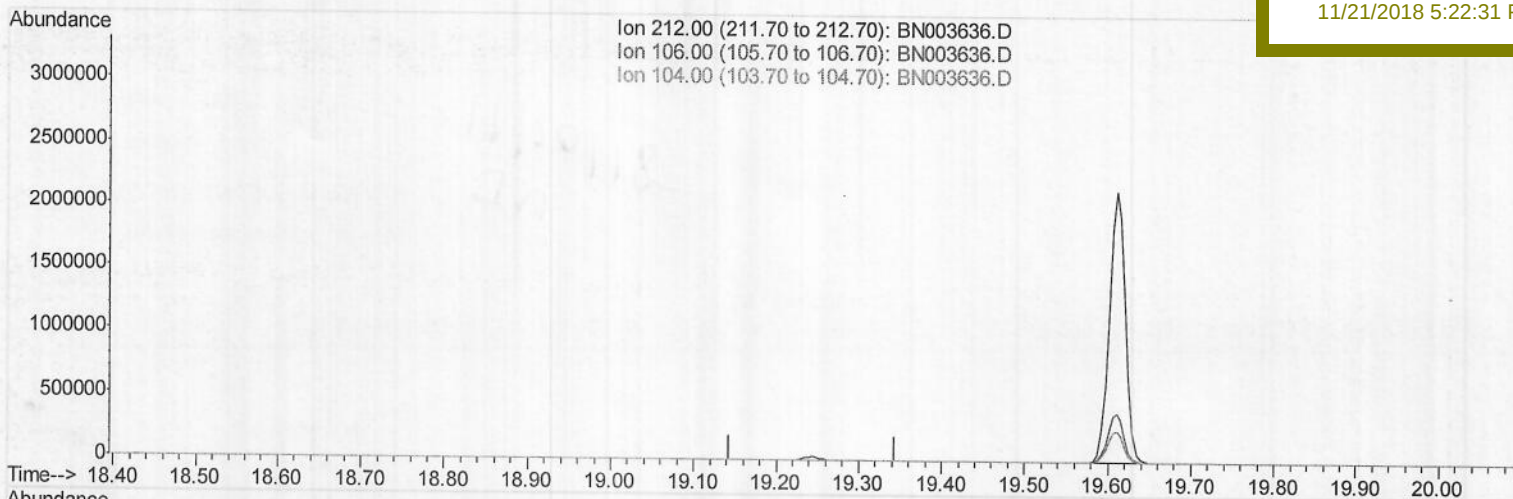

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:22:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

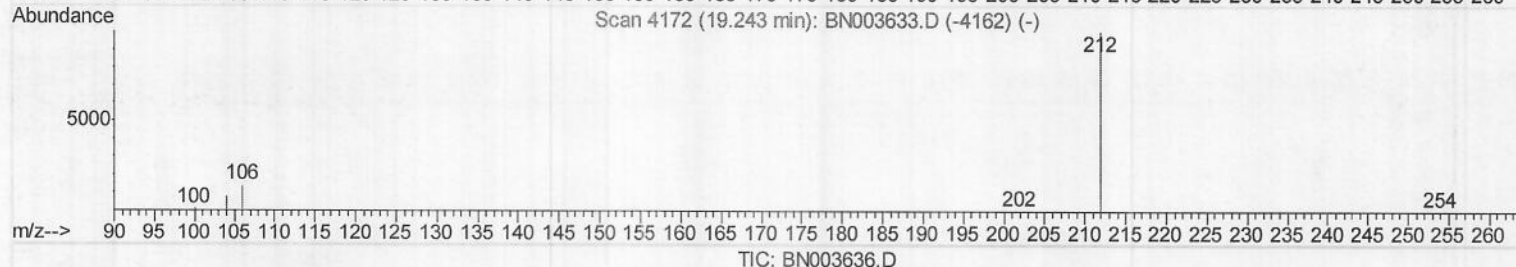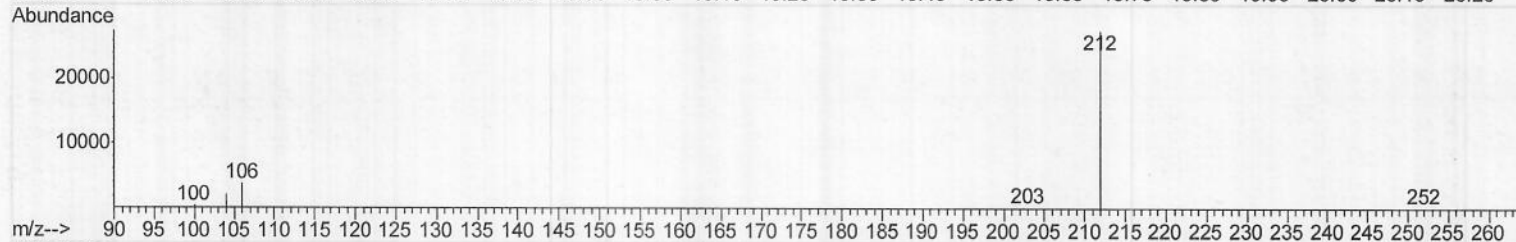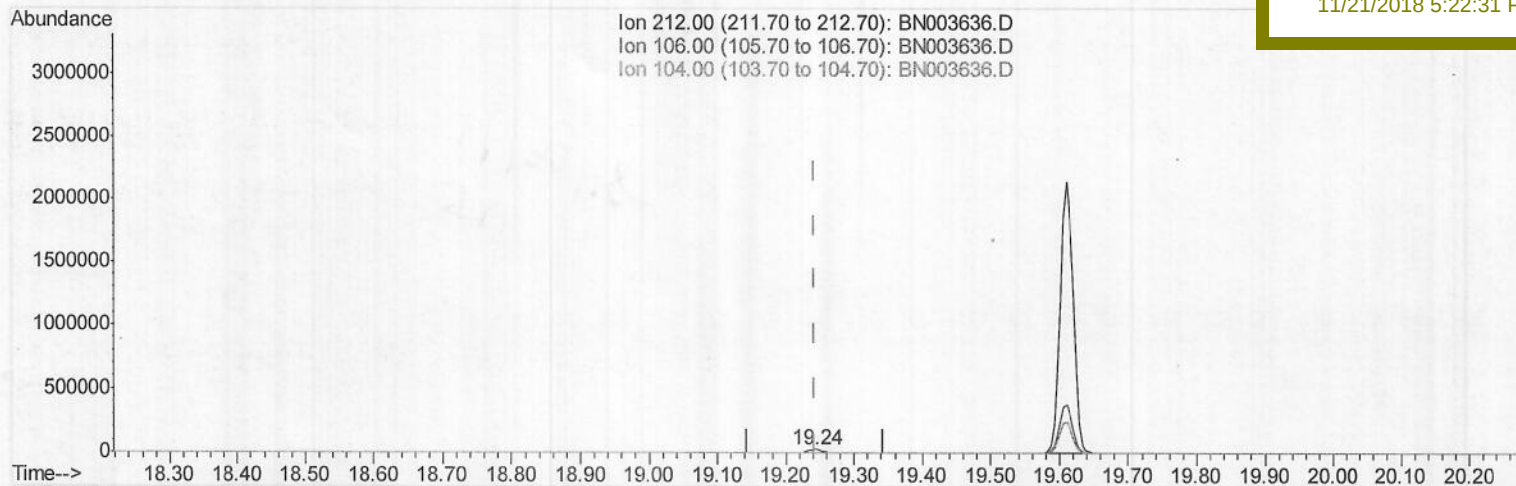

TIC: BN003636.D

(14) Fluoranthene-d10 (SURR)

19.244min (+0.000) 0.34ng/ul m

response 35431

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

JV
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:22:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

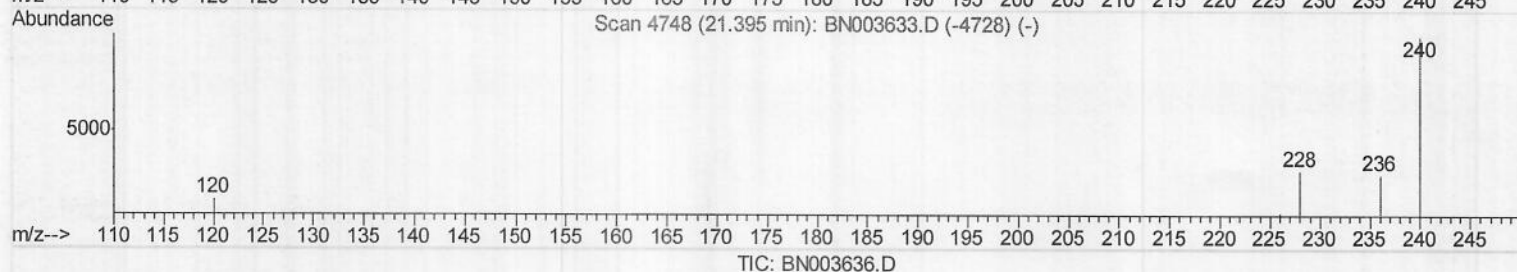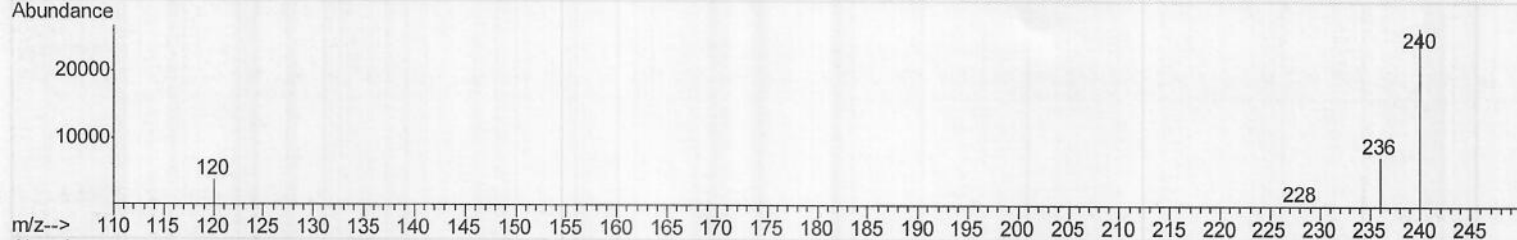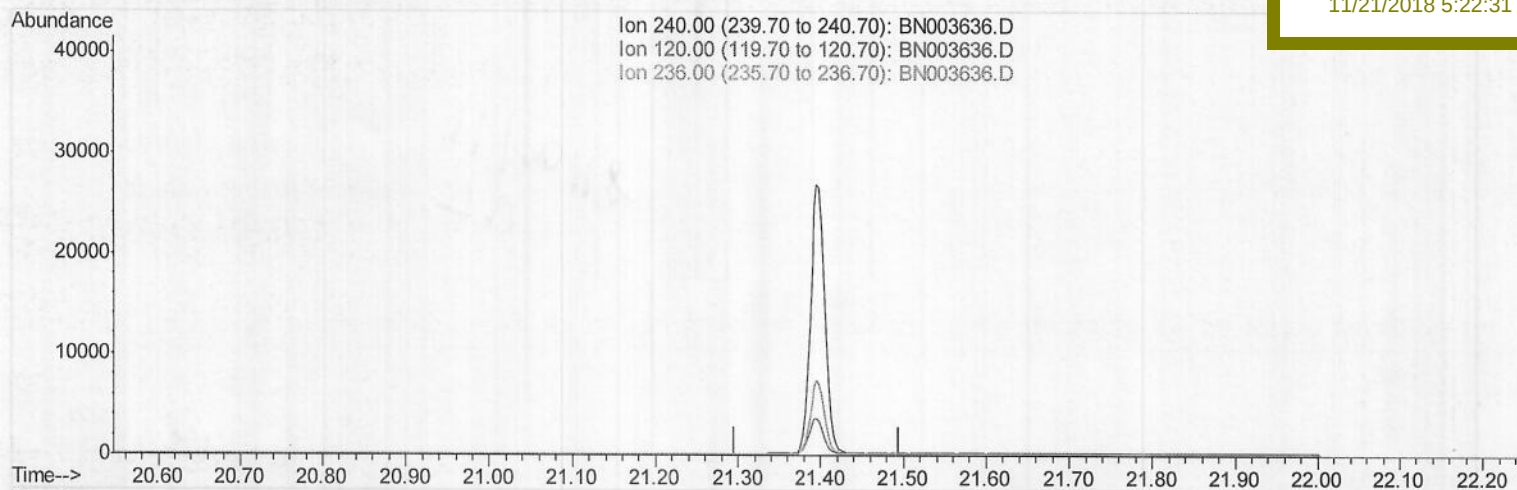

TIC: BN003636.D

(16) Chrysene-d12 (I)
21.395min (-21.395) 0.00ng/ul
response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40T8

Quant Time: Nov 21 00:22:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

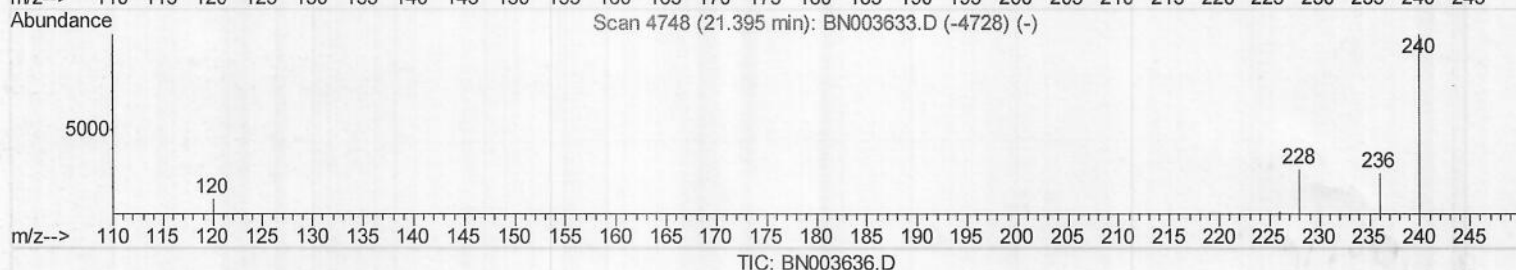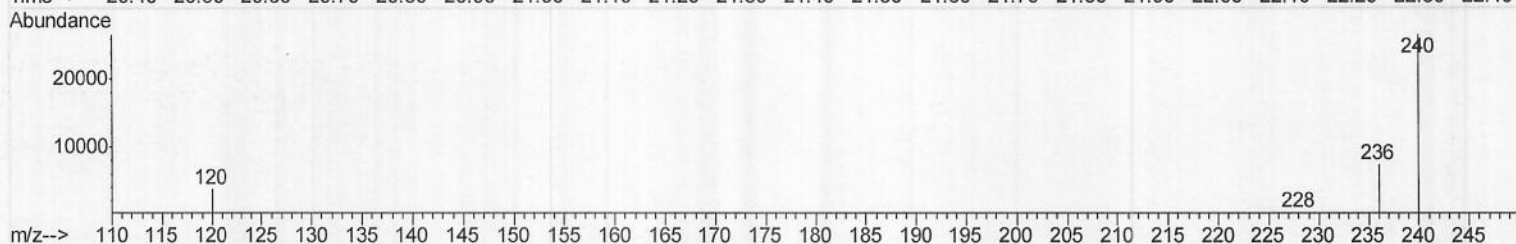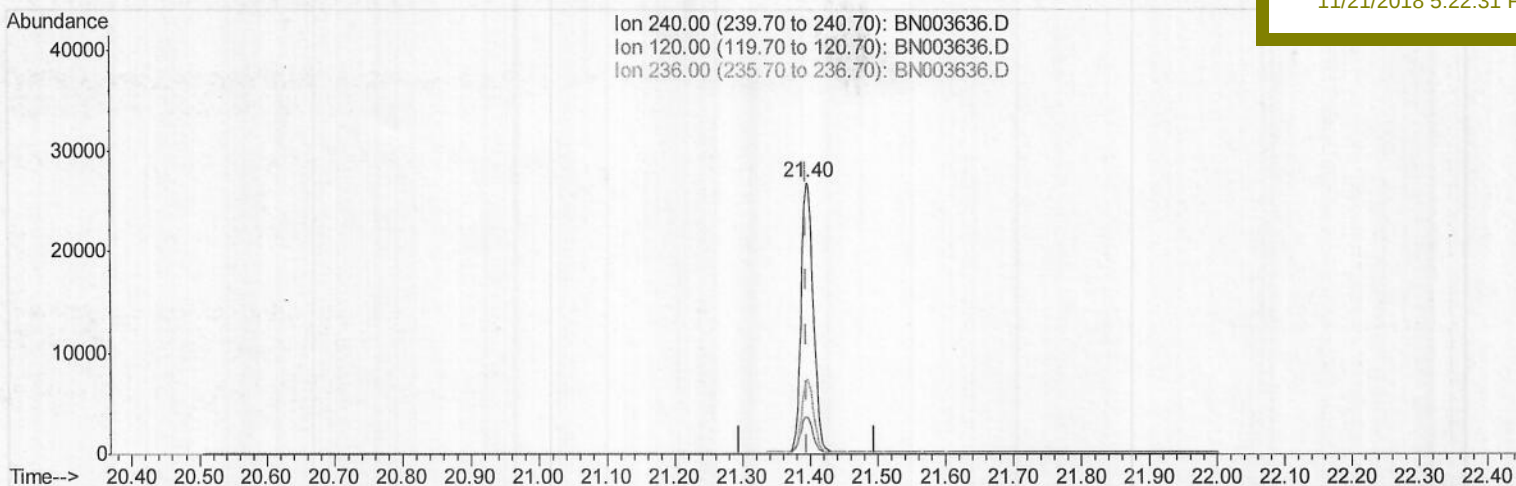

(16) Chrysene-d12 (I)

21.396min (+0.000) 0.40ng/ul m

response 33582

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	13.81
236.00	27.60	27.59
0.00	0.00	0.00

JU
11/20/18




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:23:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

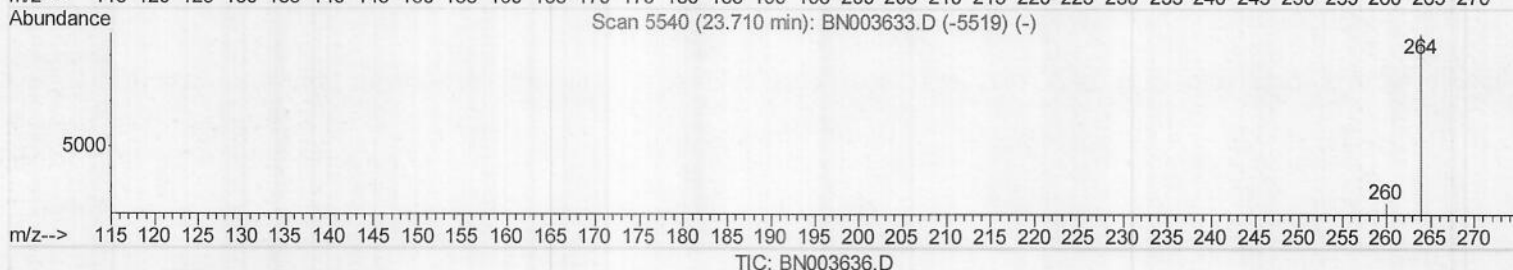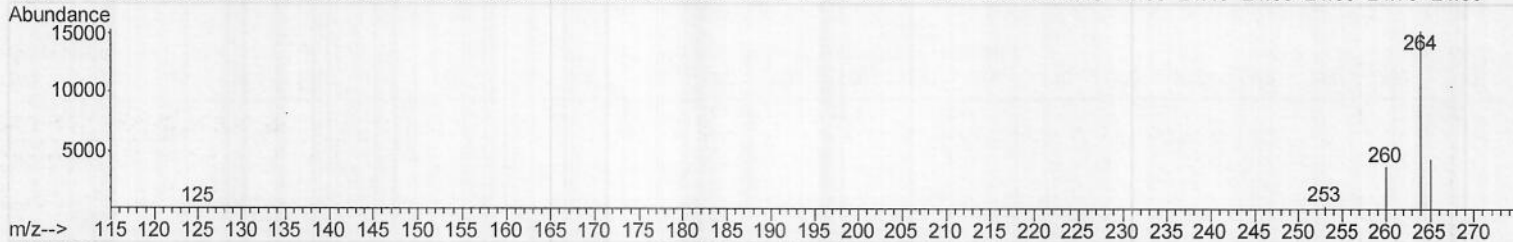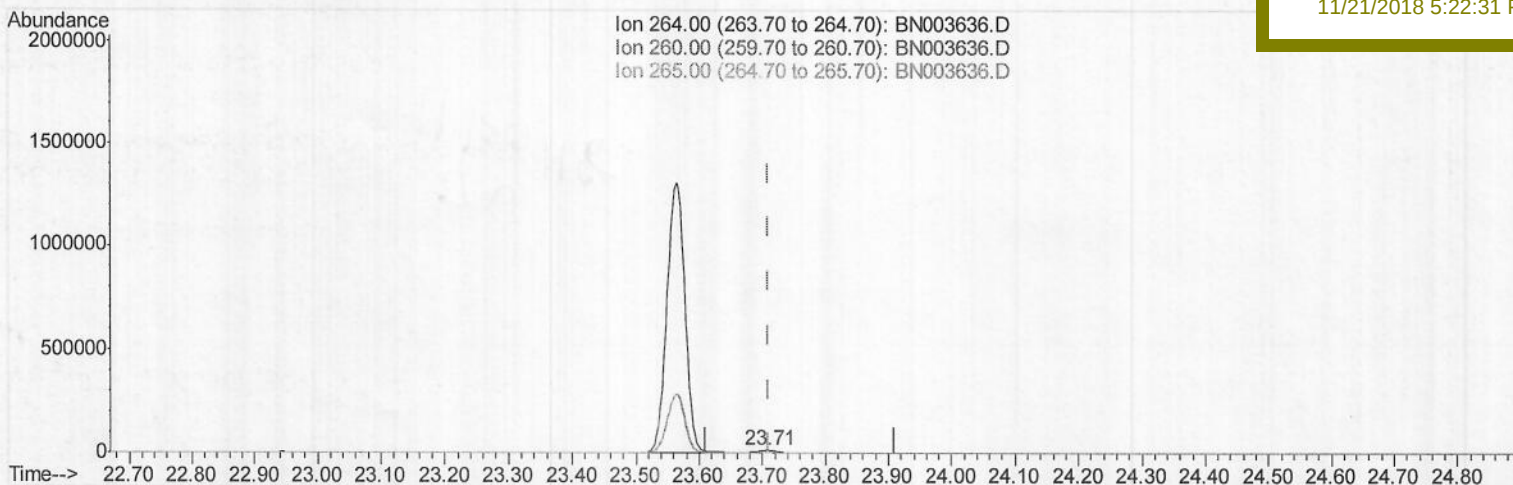

(20) Perylene-d12 (I)

23.708min (-0.003) 0.40ng/ul

response 33364

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.32
265.00	33.50	29.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:23:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

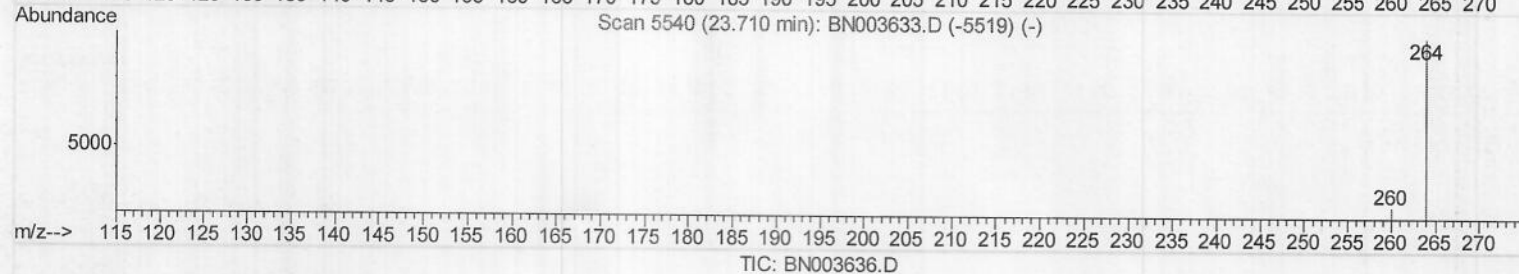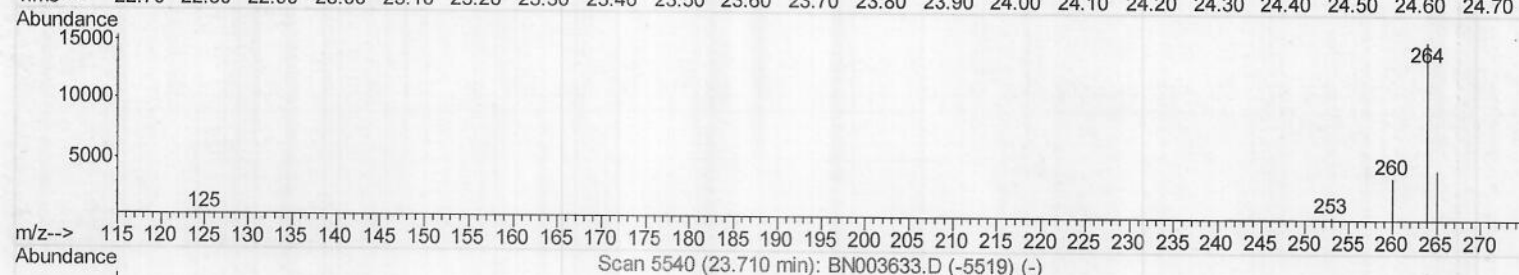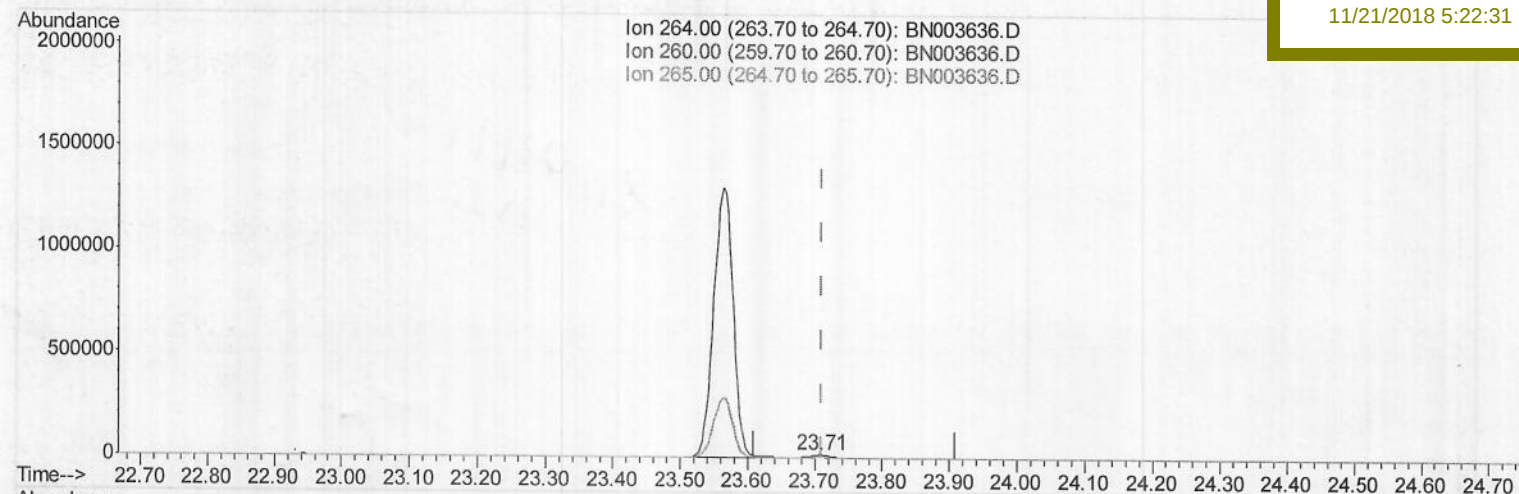

(20) Perylene-d12 (I)

23.708min (-0.003) 0.40ng/ul m

response 26399

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.32
265.00	33.50	29.26
0.00	0.00	0.00

50
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (QT Reviewed)

Data File : BN003636.D
Acq On : 20 Nov 2018 17:58
Operator : MJ/SJ
Sample : J6001-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Nov 21 00:24:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40T8

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:31 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6680	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	27779	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	16313	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	35506m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	33582m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	26399m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	14394	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	35431m	0.34	ng/ul	0.00
Target Compounds	Qvalue					

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} JV
11/20/18