

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (QT Reviewed)


Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:33:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

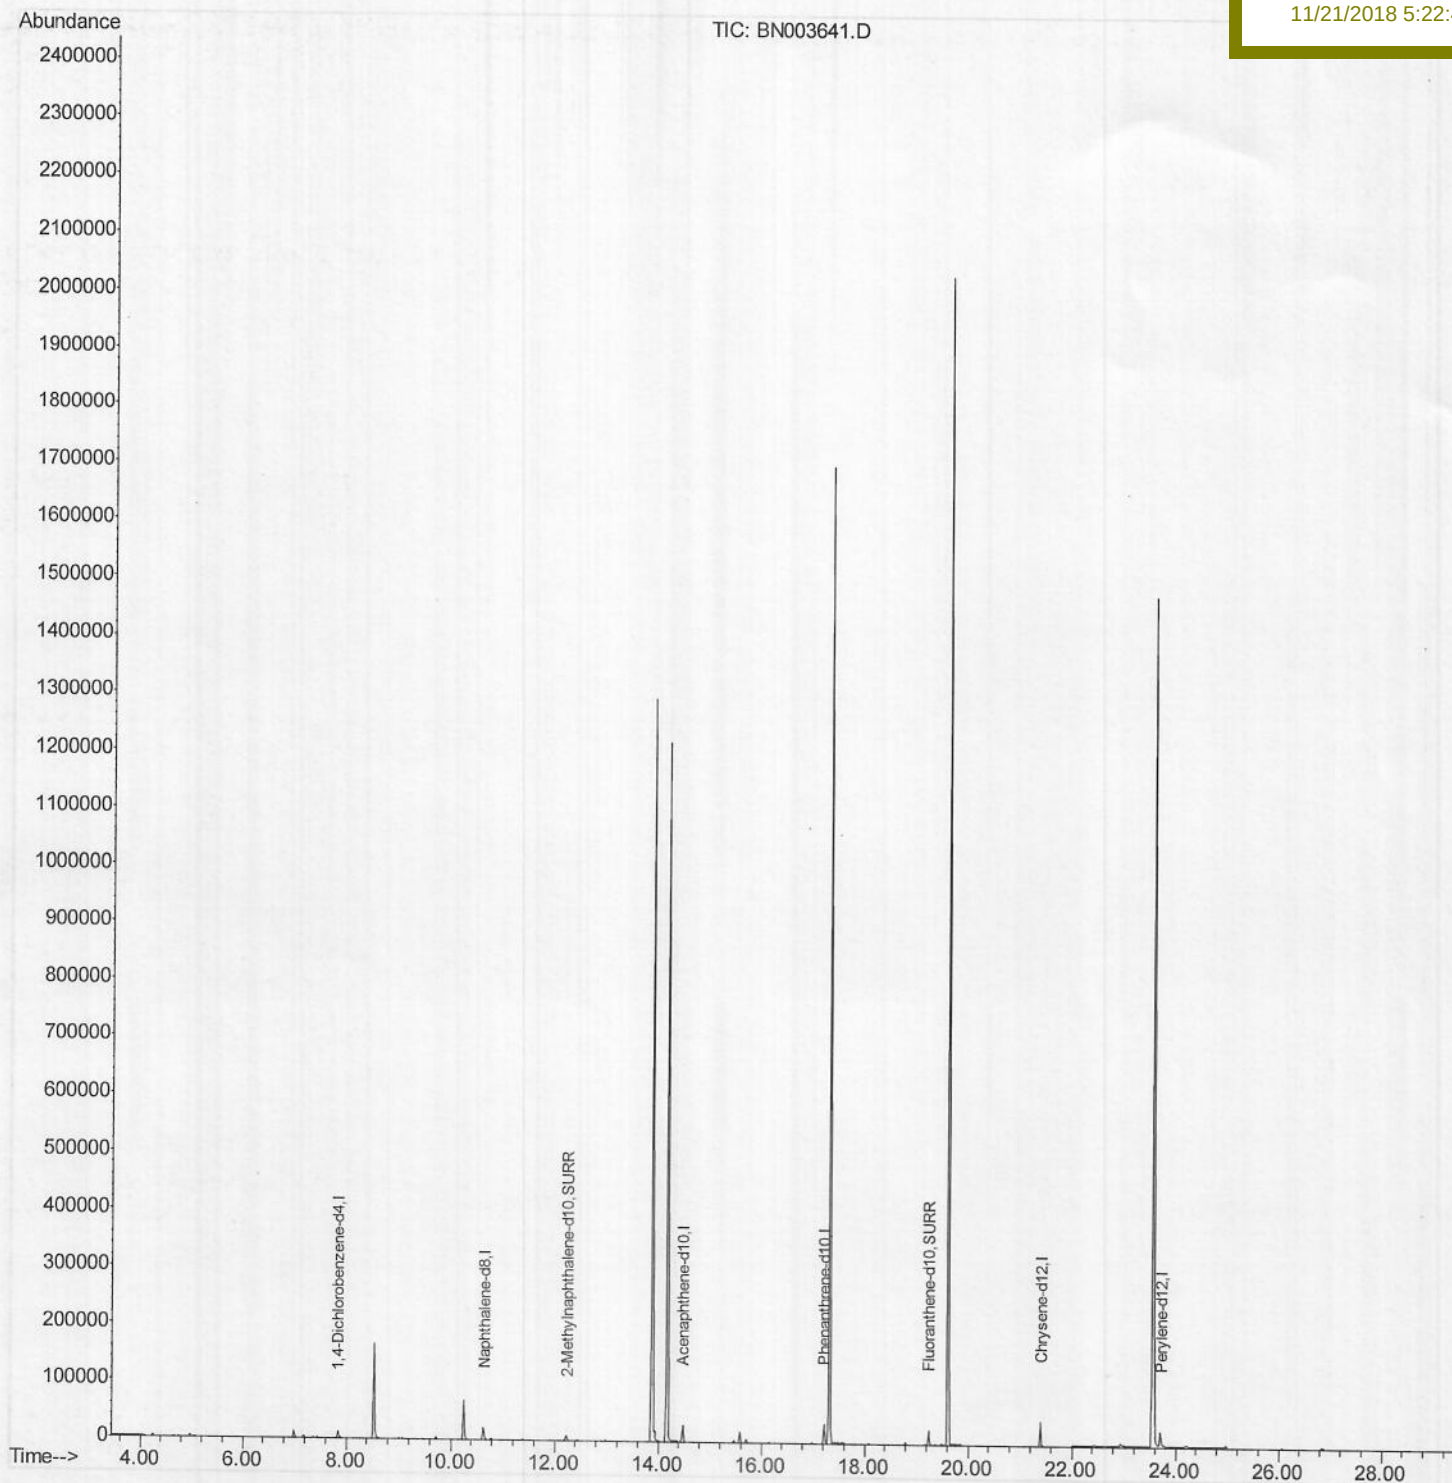

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)



Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:13:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration


Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

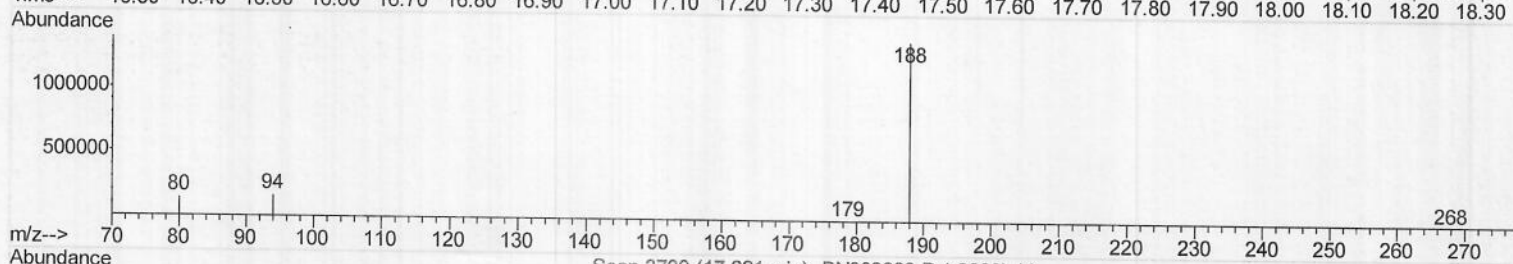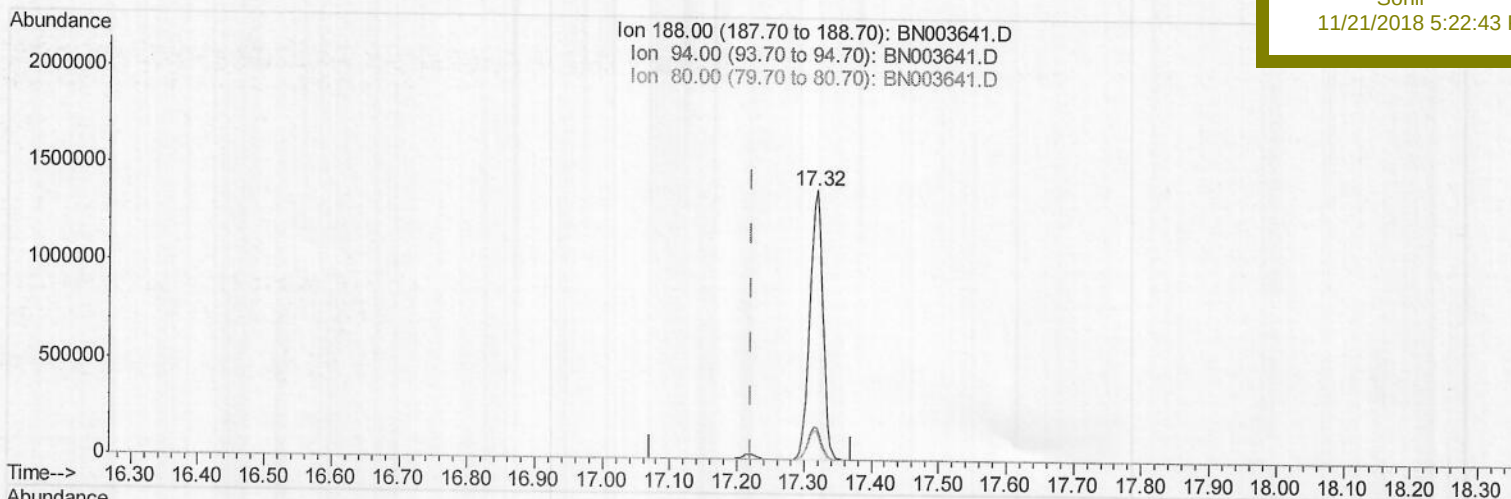

Scan 3709 (17.221 min): BN003633.D (-3699) (-)

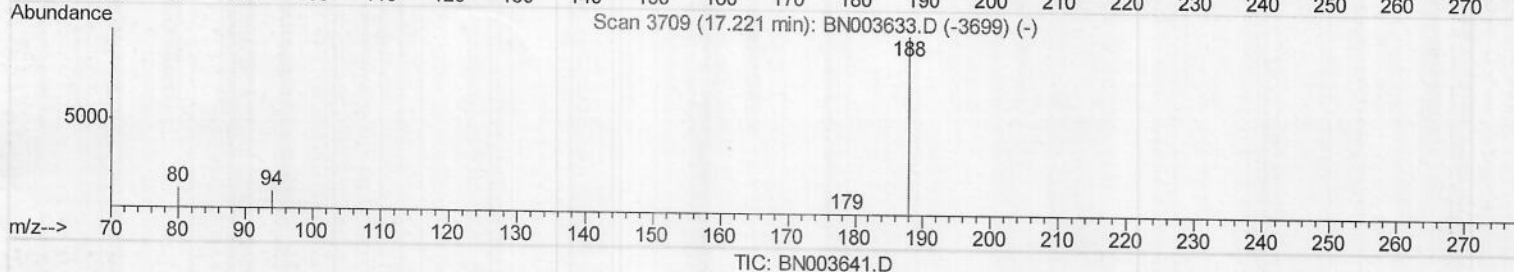

(10) Phenanthrene-d10 (I)

17.318min (+0.097) 0.40ng/ul

response 1909114

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.87
80.00	11.60	10.55
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)



Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:13:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

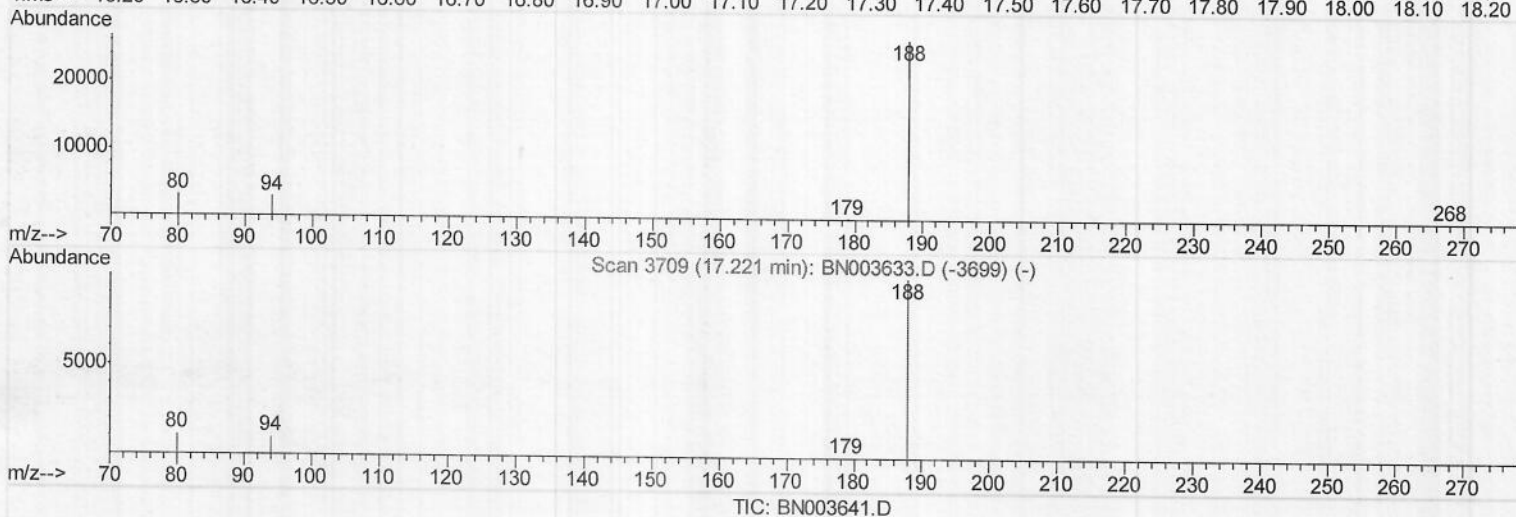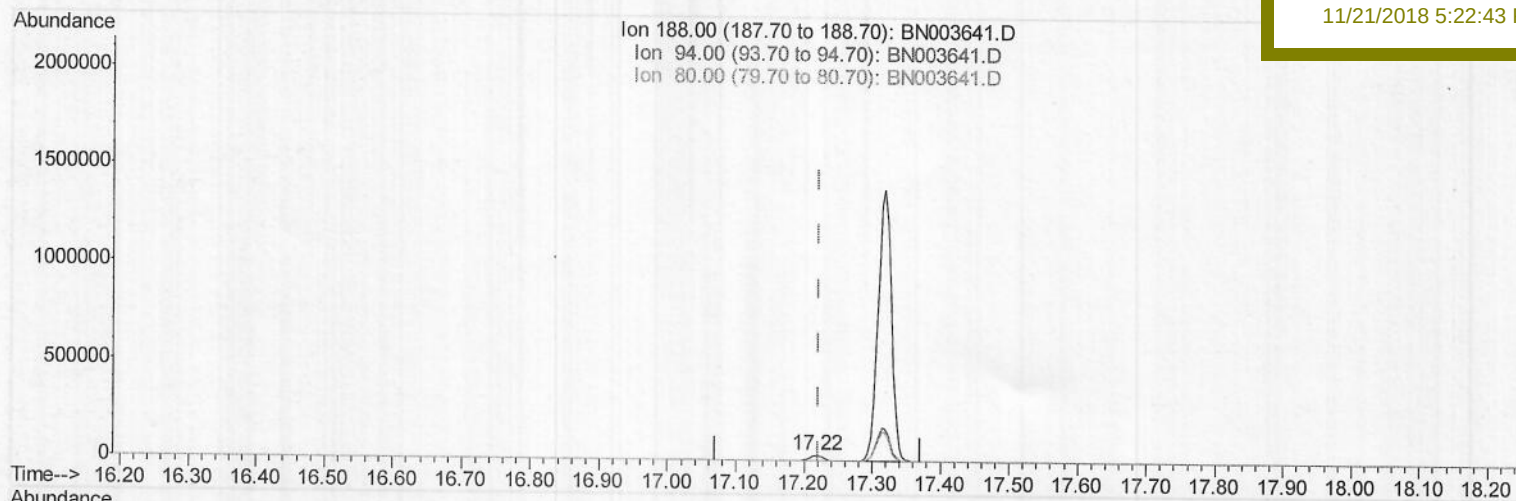

(10) Phenanthrene-d10 (I)

17.217min (-0.004) 0.40ng/ul m

response 36561

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.97
80.00	11.60	11.72
0.00	0.00	0.00

JU
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:32:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

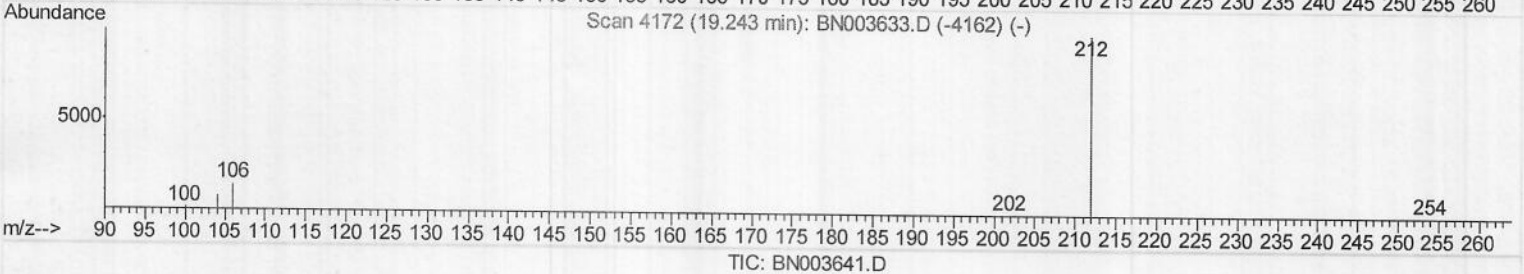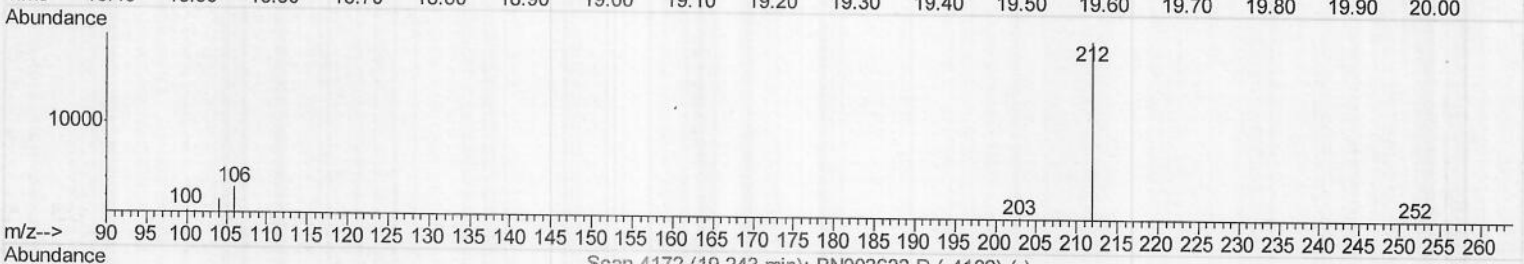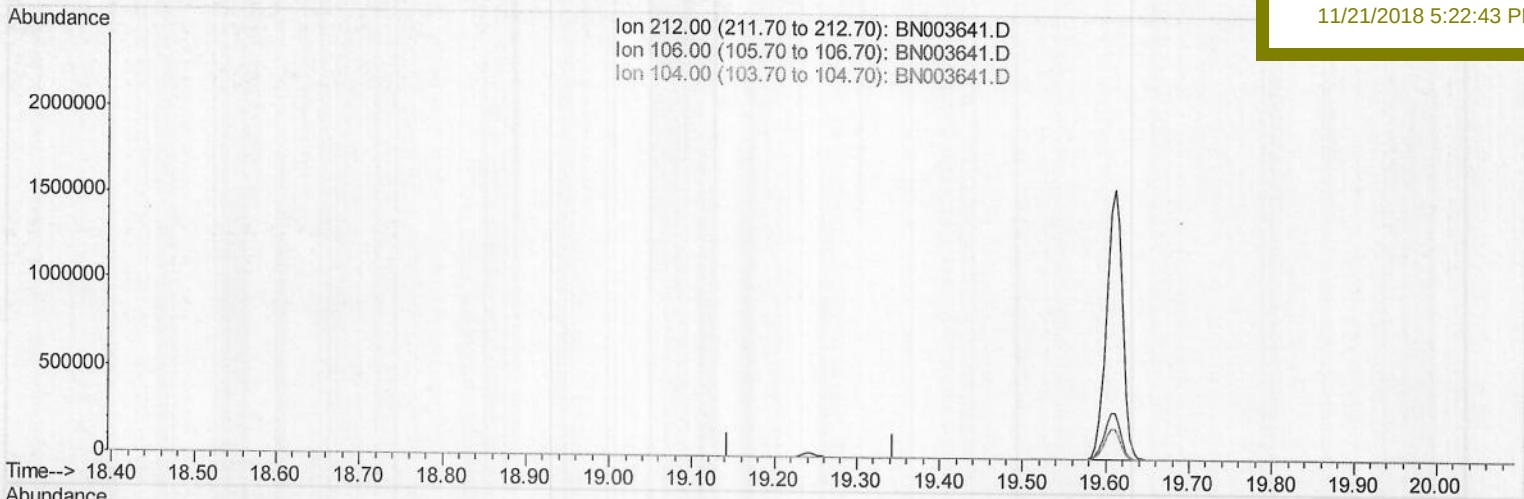

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)



Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:32:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

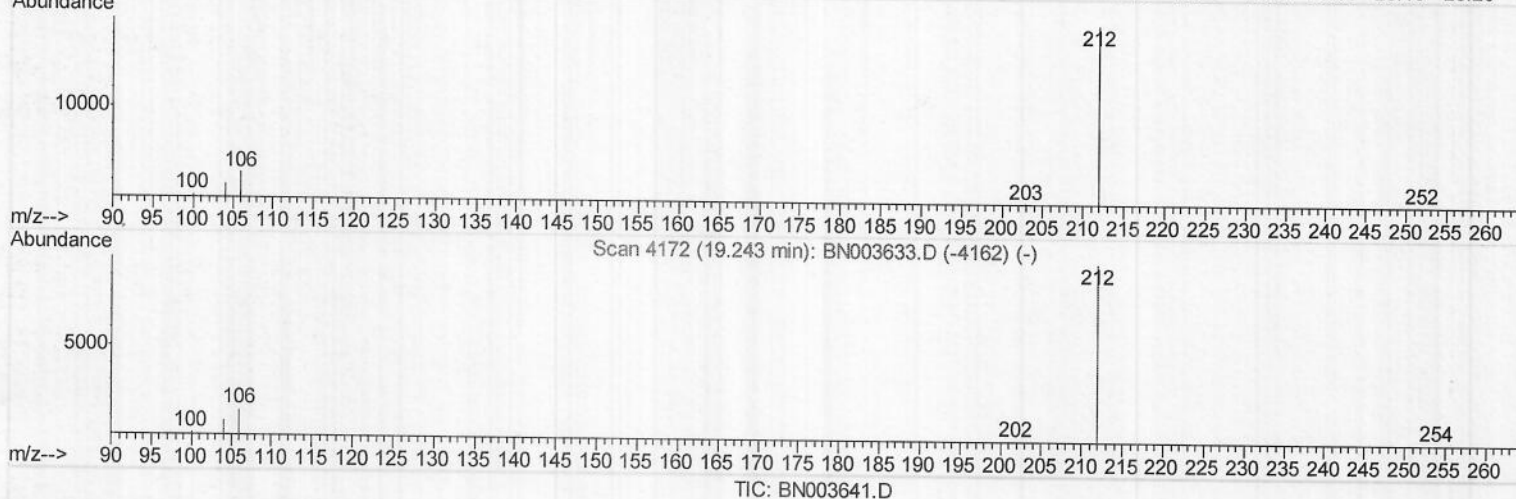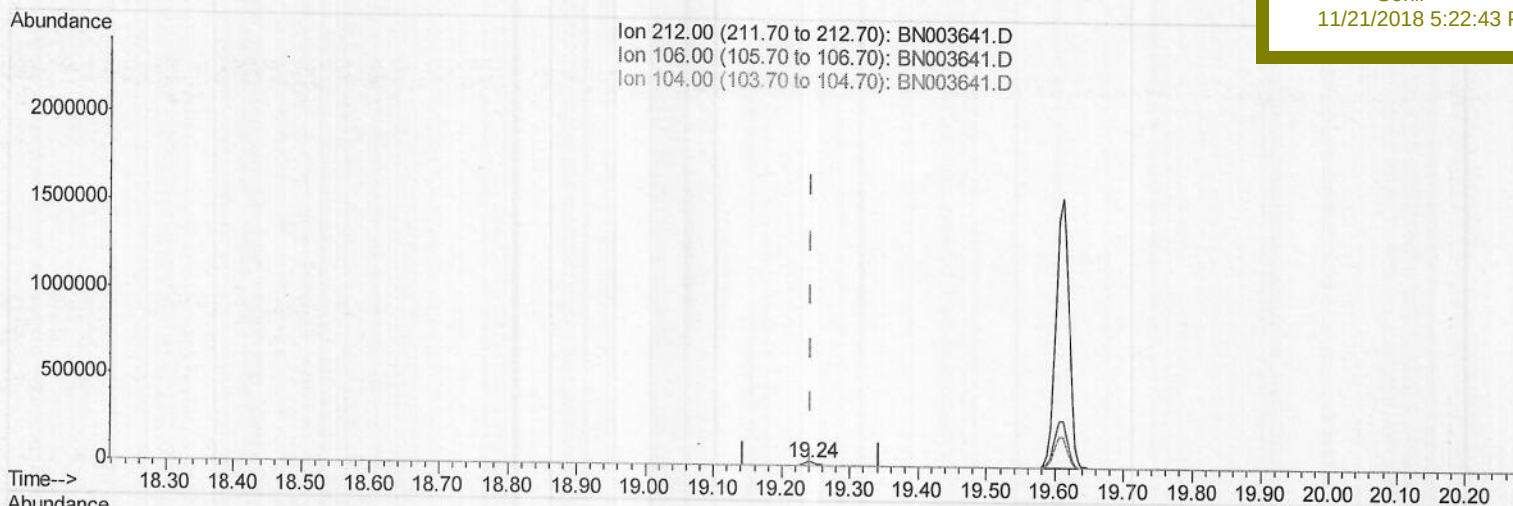

(14) Fluoranthene-d10 (SURR)

19.244min (+0.000) 0.25ng/ul m

response 26355

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

JV
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:32:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

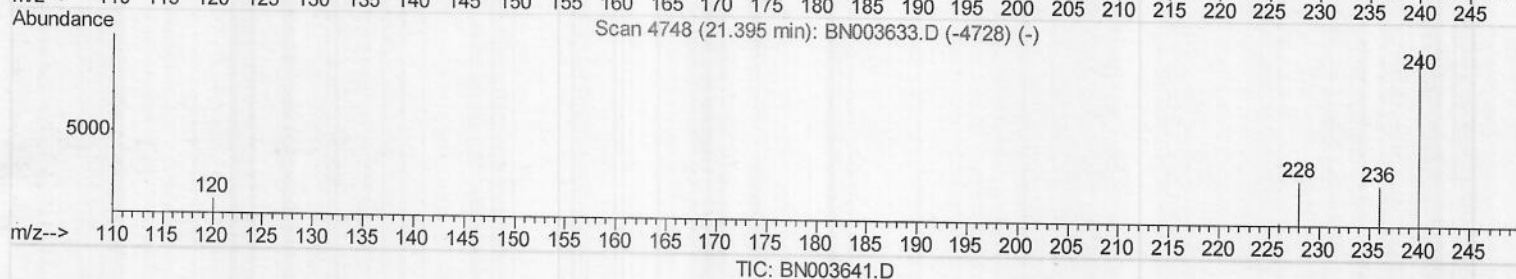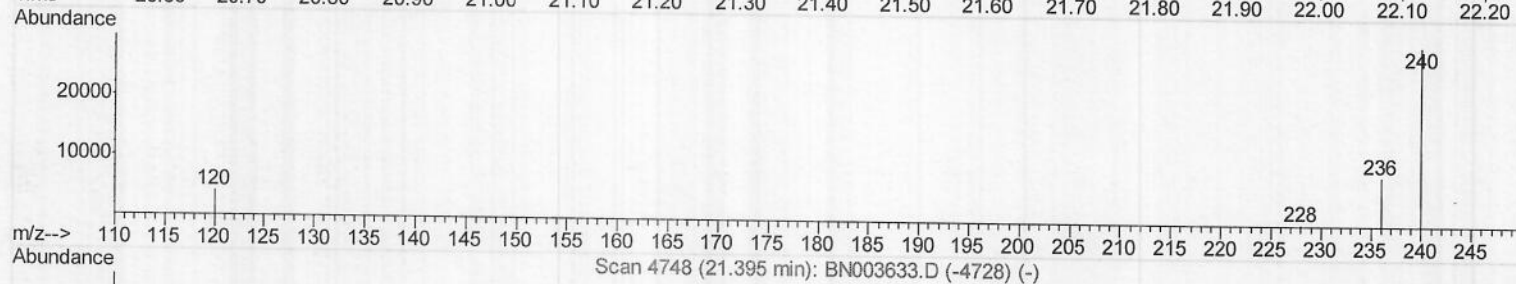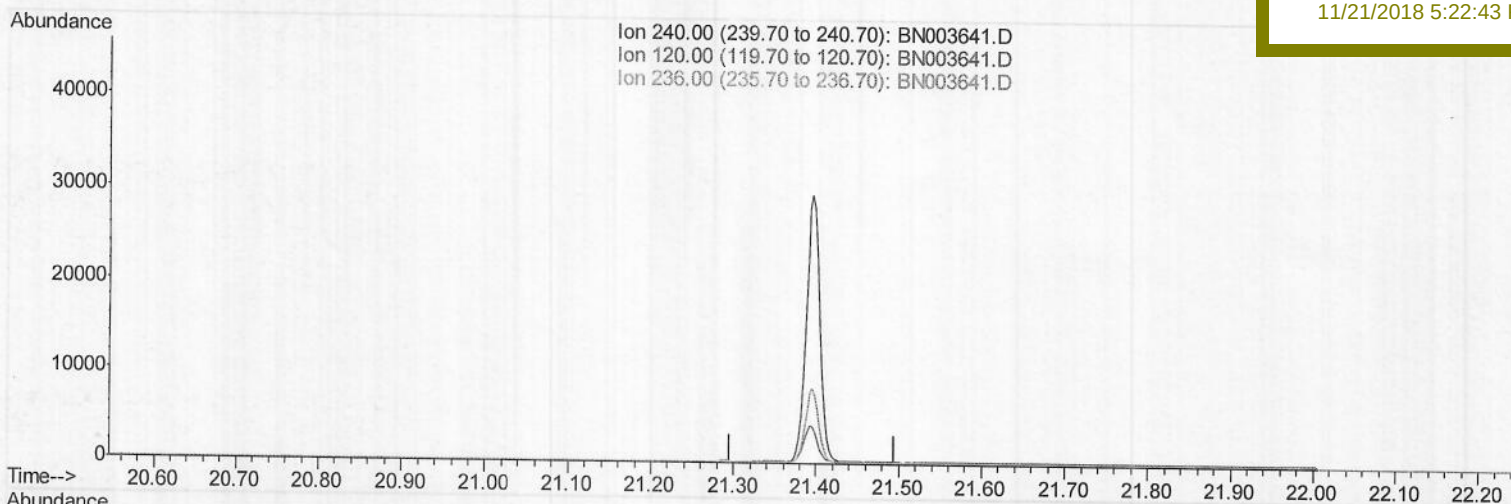

(16) Chrysene-d12 (I)

21.395min (-21.395) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:32:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

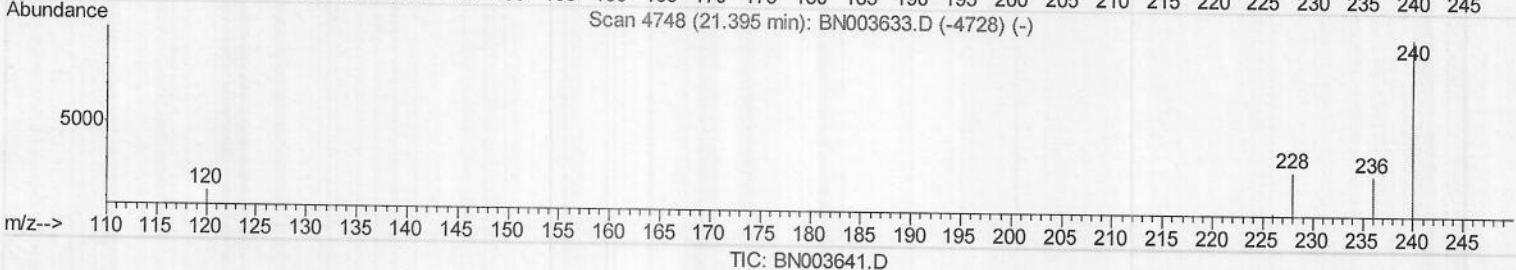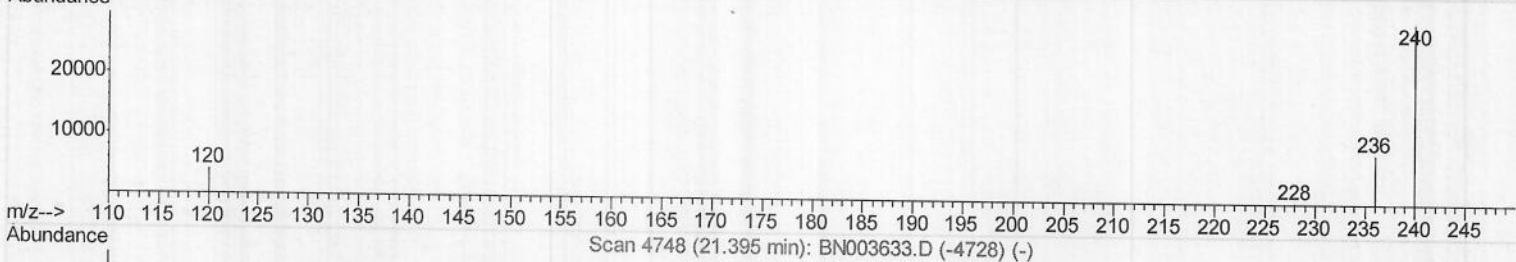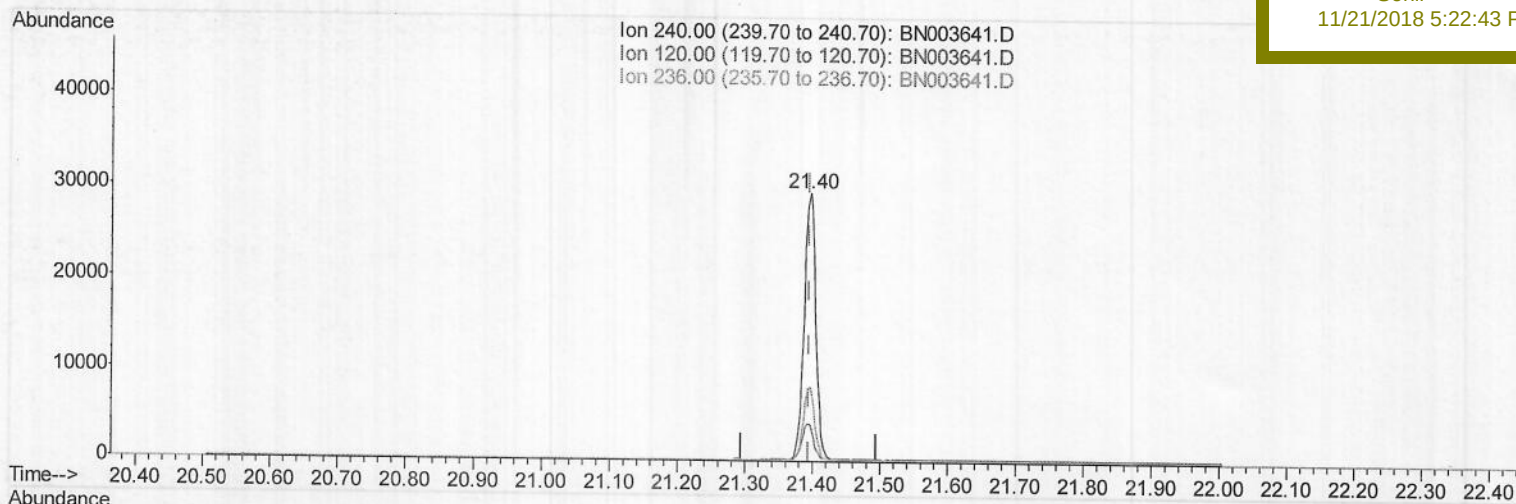

(16) Chrysene-d12 (I)

21.396min (+0.000) 0.40ng/ul m

response 35559

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	13.78
236.00	27.60	27.65
0.00	0.00	0.00

JV
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:32:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

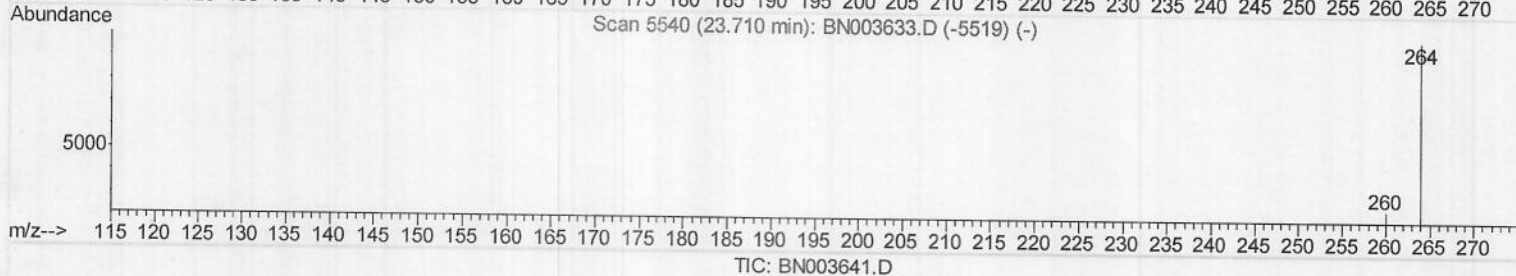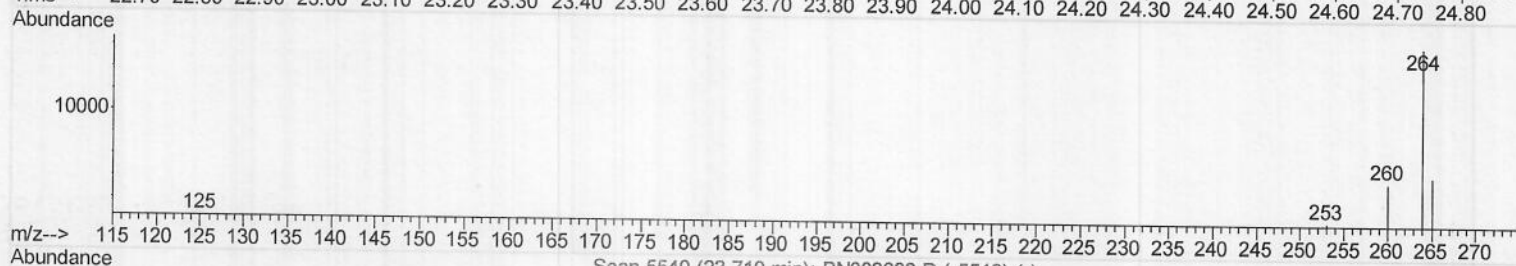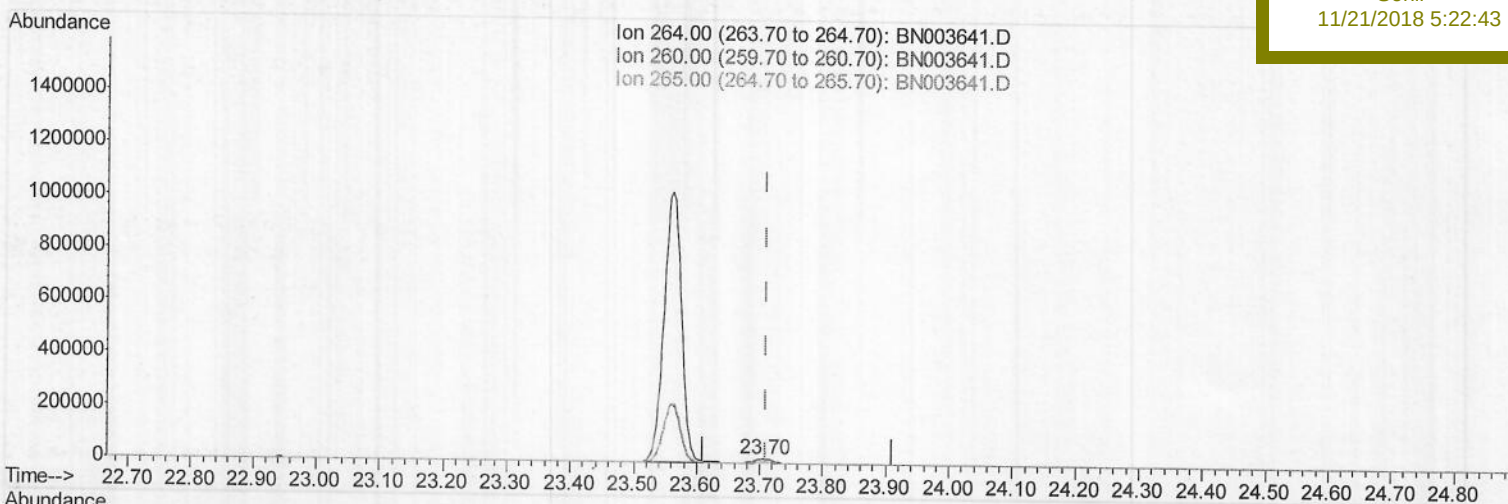

(20) Perylene-d12 (I)

23.705min (-0.006) 0.40ng/ul

response 35088

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.47
265.00	33.50	28.53
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
Quantitation Report (Qedit)




Data File : BN003641.D
Acq On : 20 Nov 2018 20:54
Operator : MJ/SJ
Sample : J5928-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y0

Manual Integrations
APPROVED

Sohil
11/21/2018 5:22:43 PM

Quant Time: Nov 21 00:32:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 21 00:09:42 2018
Response via : Initial Calibration

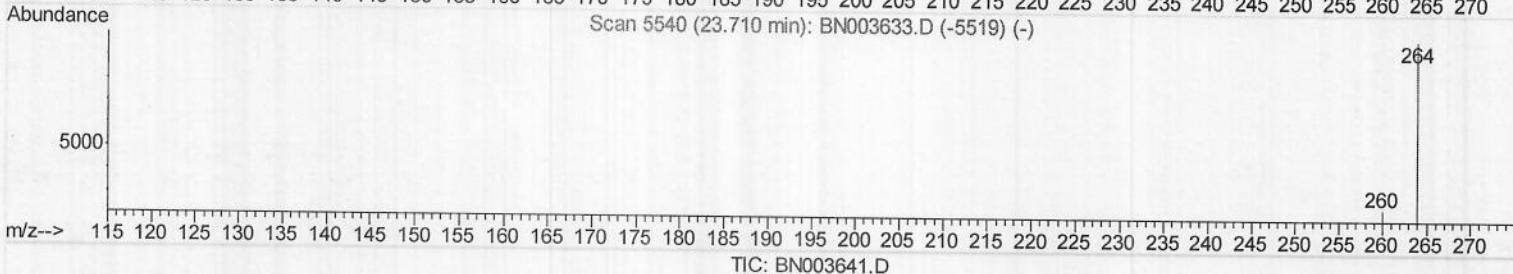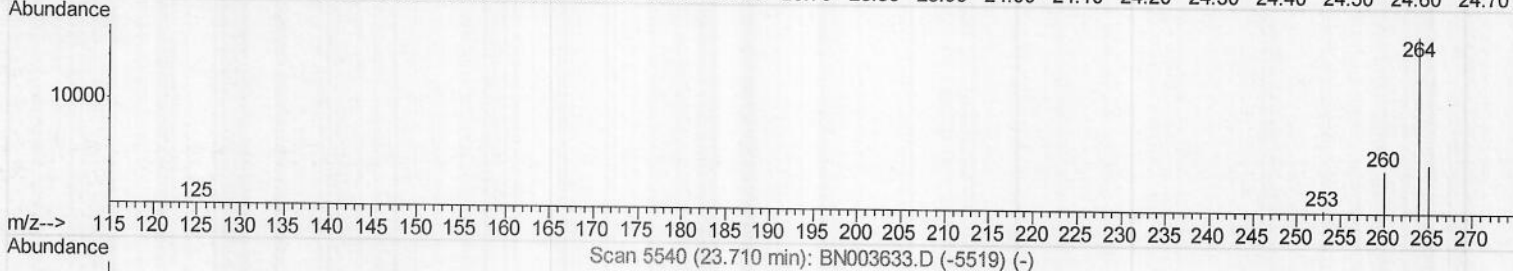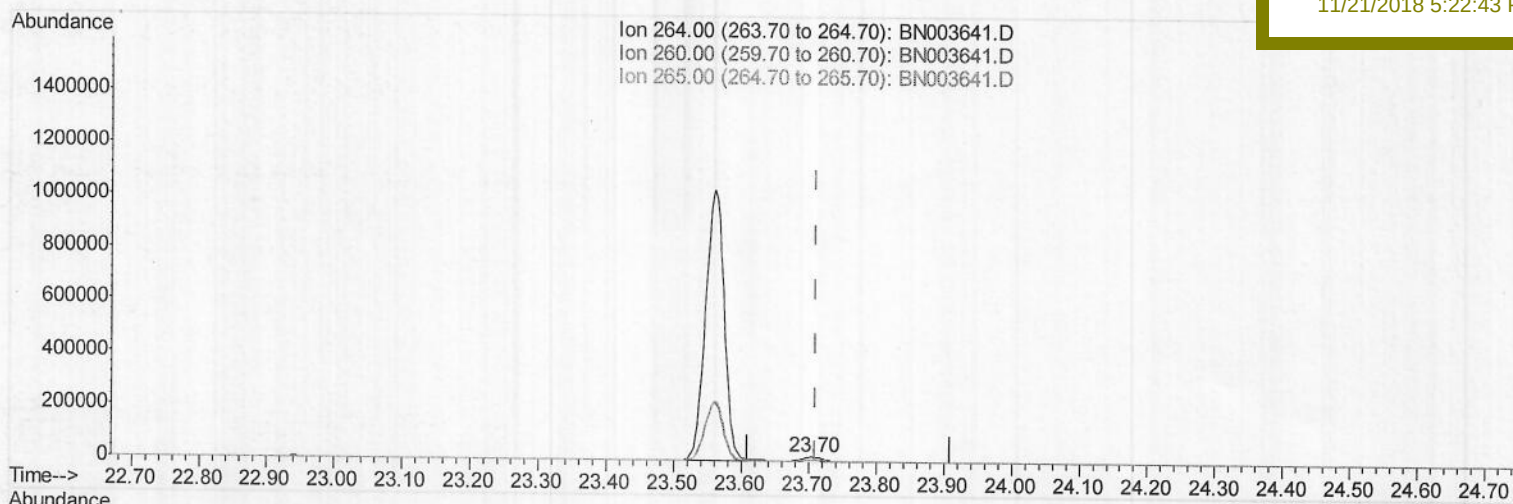

(20) Perylene-d12 (I)

23.705min (-0.006) 0.40ng/ul m

response 30063

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.47
265.00	33.50	28.53
0.00	0.00	0.00

JV
11/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\

Quantitation Report (QT Reviewed)

Data File : BN003641.D

Acq On : 20 Nov 2018 20:54

Operator : MJ/SJ

Sample : J5928-15

Misc :

ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 21 00:33:32 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Nov 21 00:09:42 2018

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A40Y0

Manual Integrations

APPROVED

Sohil

11/21/2018 5:22:43 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6656	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	27892	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	16006	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	36561m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	35559m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	30063m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	10178	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	26355m	0.25	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JV
11/20/18