


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112018\
 Data File : BN003623.D
 Acq On : 20 Nov 2018 08:44
 Operator : MJ/SJ
 Sample : DFTPP55
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP55

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 21 17:33:53 2018

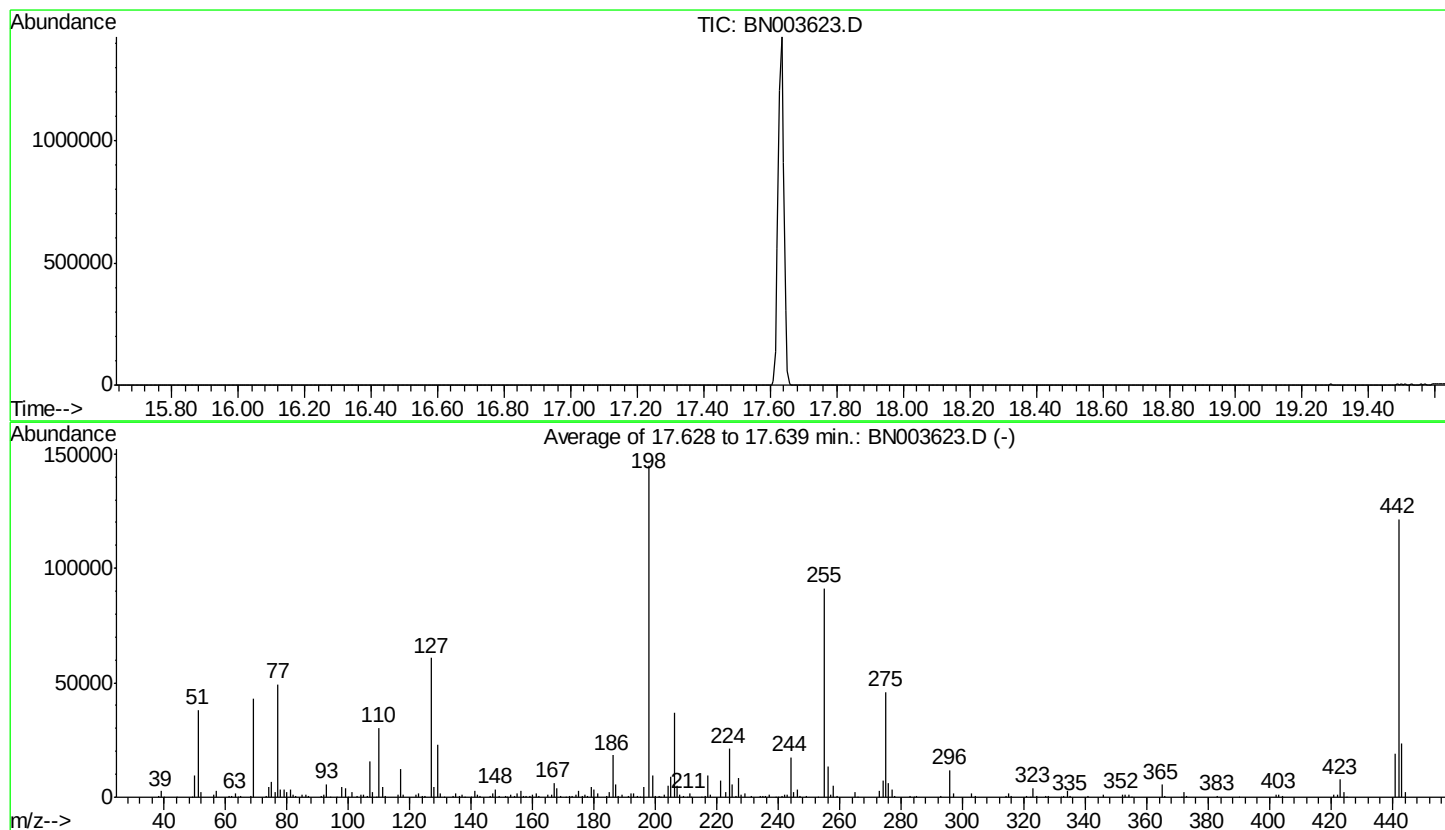

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	38037	PASS
68	69	0.00	2	1.9	798	PASS
69	198	0.00	100	29.7	43050	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	60792	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144845	PASS
199	198	5	9	6.7	9760	PASS
275	198	10	60	31.8	46005	PASS
365	198	1	100	3.9	5580	PASS
441	198	0.01	100	13.3	19258	PASS
442	198	50	100	83.8	121448	PASS
443	442	15	24	19.2	23272	PASS

m/z	Abundance
38.00	493.0
39.00	3198.0
43.90	954.0
49.00	330.0
50.00	11530.0
51.00	44656.0
52.00	2427.0
56.00	1331.0
57.00	3300.0
61.00	686.0
62.00	656.0
63.00	1898.0
65.00	941.0
68.10	993.0
69.00	50248.0
73.00	471.0
74.00	5037.0
75.00	8168.0
76.00	2812.0
77.00	56768.0
78.00	3977.0
79.00	4045.0
80.00	3138.0
81.00	4100.0
81.90	986.0
83.00	891.0
85.00	1040.0
85.90	1226.0
87.00	510.0
91.00	996.0
92.00	1129.0
93.00	6600.0
94.00	478.0
96.00	327.0
98.00	5020.0
99.00	4476.0
99.90	416.0
101.00	2405.0
102.90	779.0
103.90	1511.0
105.00	1299.0
106.00	483.0
107.00	17448.0
108.00	2618.0
110.00	34256.0
111.00	5411.0
111.90	699.0
116.00	1100.0
117.00	13562.0
118.00	1142.0
121.90	1210.0
123.00	1893.0
124.00	888.0
124.90	785.0
127.00	68000.0
128.00	5197.0
129.00	25552.0
130.00	2155.0
130.90	430.0
134.00	798.0
135.00	2045.0
136.00	941.0
137.00	1193.0
141.00	3226.0
141.90	1017.0
143.00	752.0
146.00	646.0
147.00	1691.0
148.00	3680.0
149.00	898.0
151.00	473.0
151.70	325.0
152.90	1158.0
153.90	867.0
155.00	1966.0
156.00	2822.0
157.10	590.0
157.90	682.0
158.90	433.0
159.90	1144.0
161.00	1597.0
162.00	501.0
165.00	1157.0
166.00	988.0
167.00	6659.0
168.00	4422.0
169.00	684.0
172.00	616.0
173.00	873.0
174.00	1574.0
175.00	2713.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

176.10	795.0
177.00	1303.0
178.00	413.0
179.00	5152.0
180.00	4044.0
181.00	1777.0
184.00	419.0
185.00	2480.0
186.00	19496.0
187.00	5681.0
188.00	721.0
188.90	1216.0
191.00	626.0
192.00	1656.0
193.00	1858.0
194.00	376.0
196.00	4490.0
198.00	151488.0
199.00	10443.0
199.90	775.0
201.40	730.0
203.00	941.0
204.00	4932.0
205.00	8837.0
206.00	38248.0
207.00	5253.0
208.00	1316.0
209.00	451.0
210.20	622.0
211.00	1561.0
214.90	390.0
216.00	791.0
217.00	9866.0
218.00	1280.0
221.00	6977.0
223.00	2198.0
224.00	20824.0
225.00	5592.0
226.00	755.0
227.00	8172.0
227.90	1249.0
229.00	1843.0
231.00	666.0
234.00	514.0
235.00	607.0
236.00	421.0
237.00	1068.0
239.00	334.0
241.00	494.0
242.00	1170.0
243.00	1437.0
244.00	17760.0
245.10	2339.0
246.00	3360.0
247.00	671.0
249.00	686.0
252.90	346.0
255.00	88288.0
256.00	12999.0
256.90	1136.0
258.00	4829.0
259.00	849.0
265.00	2012.0
273.00	2705.0
274.00	6993.0
275.00	44248.0
276.00	6002.0
277.00	3266.0
278.00	666.0
283.00	370.0
284.90	638.0
293.00	828.0
296.00	11184.0
297.00	1647.0
303.00	1369.0
304.00	363.0
313.90	577.0
315.00	1268.0
316.00	827.0
321.00	374.0
323.00	3648.0
324.00	686.0
326.90	699.0
327.90	328.0
333.00	412.0
334.00	2430.0
335.00	700.0
340.90	442.0
346.00	949.0
352.00	1117.0
353.00	819.0
354.00	1146.0
365.00	4722.0
366.00	720.0
372.00	1782.0

Instrument :

BNA_N

ClientSampleId :

DFTPP55

373.00	459.0
383.00	450.0
402.00	700.0
403.00	1118.0
404.00	420.0
420.90	925.0
422.10	841.0
423.00	6426.0
424.00	2025.0
425.00	327.0
441.10	15280.0
442.00	94712.0
443.00	18800.0
444.00	1899.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

m/z	Abundance
38.00	536.0
39.00	3032.0
39.90	382.0
44.00	972.0
49.00	377.0
50.00	11031.0
51.00	44936.0
52.00	2237.0
56.00	1346.0
57.00	3052.0
61.00	564.0
62.00	618.0
63.00	1927.0
64.00	309.0
65.00	1048.0
68.00	943.0
69.00	50464.0
73.00	504.0
74.00	4939.0
75.00	8191.0
76.00	2802.0
77.00	58800.0
78.00	3783.0
79.00	3831.0
80.00	2876.0
81.00	4215.0
82.00	1044.0
83.00	960.0
85.00	1211.0
86.00	1119.0
87.00	526.0
90.90	1061.0
92.00	1114.0
93.00	6661.0
93.90	310.0
98.00	5247.0
99.00	4556.0
100.00	395.0
101.00	2316.0
102.90	914.0
103.90	1575.0
104.90	1524.0
106.00	571.0
107.00	18408.0
108.00	3084.0
109.10	557.0
110.00	35960.0
111.00	5431.0
112.00	700.0
116.10	1078.0
117.00	14758.0
118.00	1202.0
122.00	1339.0
123.00	2020.0
123.90	938.0
125.00	839.0
127.00	72400.0
128.00	5447.0
129.00	28120.0
130.00	2325.0
131.00	441.0
134.00	810.0
134.90	2167.0
136.00	929.0
137.00	1218.0
138.00	302.0
140.00	361.0
141.00	3783.0
142.00	1134.0
143.00	798.0
145.90	705.0
147.00	1956.0
148.00	3941.0
149.00	882.0
151.00	522.0
151.70	306.0
153.00	1055.0
154.00	1003.0
155.00	2049.0
156.00	2934.0
157.00	597.0
158.00	686.0
158.90	584.0
160.00	1259.0
161.00	1852.0
161.90	541.0
165.00	1372.0
166.00	1177.0
167.00	7485.0
168.00	4249.0
169.00	838.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

170.90	379.0
171.90	686.0
173.00	879.0
174.00	1639.0
175.00	3100.0
176.00	903.0
177.00	1554.0
178.00	555.0
179.00	5672.0
180.00	4401.0
181.00	1853.0
184.00	475.0
185.00	2702.0
186.00	22136.0
187.00	6553.0
188.00	734.0
189.00	1497.0
191.00	749.0
192.00	1778.0
193.00	2142.0
194.10	474.0
195.00	345.0
196.00	5345.0
198.00	173440.0
199.00	11636.0
200.00	984.0
201.60	883.0
203.00	1172.0
204.00	6028.0
205.00	10784.0
206.00	44368.0
207.00	5878.0
208.00	1575.0
209.00	472.0
211.00	1810.0
211.80	441.0
215.00	516.0
216.10	992.0
217.00	11417.0
218.00	1565.0
221.00	8707.0
223.00	2884.0
224.00	26152.0
225.00	6636.0
226.00	803.0
227.00	9803.0
228.00	1515.0
229.00	2176.0
231.00	948.0
234.00	602.0
234.90	830.0
235.90	423.0
237.00	1152.0
239.00	465.0
240.00	335.0
241.00	546.0
242.00	1451.0
243.00	1412.0
244.00	21176.0
245.00	2978.0
246.00	4058.0
247.00	740.0
248.90	807.0
253.00	392.0
255.00	110016.0
256.00	16384.0
257.00	1435.0
258.00	6150.0
259.00	911.0
265.00	2595.0
265.90	332.0
273.00	3246.0
274.00	9142.0
275.00	56040.0
276.00	7079.0
277.00	4354.0
278.00	731.0
283.00	482.0
284.00	363.0
285.00	740.0
293.00	992.0
296.00	14212.0
297.00	2025.0
303.00	1829.0
304.00	513.0
314.00	823.0
315.00	1741.0
316.00	966.0
321.00	503.0
322.00	326.0
323.00	5220.0
324.00	993.0
327.00	952.0
327.90	502.0
332.00	345.0

Instrument :

BNA_N

ClientSampleId :

DFTPP55

333.00	467.0
334.00	3231.0
335.00	750.0
341.00	612.0
345.90	1075.0
352.00	1540.0
353.00	956.0
354.00	1797.0
355.00	355.0
365.00	6826.0
366.00	950.0
371.00	474.0
372.00	2837.0
373.10	733.0
383.00	808.0
390.10	361.0
402.00	1037.0
403.00	1600.0
404.10	564.0
421.00	1330.0
422.10	1224.0
423.00	9477.0
424.00	2535.0
425.10	379.0
441.10	23336.0
442.00	150528.0
443.10	28648.0
444.10	2575.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

m/z	Abundance
39.00	1752.0
39.90	306.0
44.00	977.0
50.00	6380.0
51.00	24520.0
52.00	1350.0
56.00	767.0
57.00	1708.0
61.00	446.0
62.00	307.0
63.00	1073.0
65.00	492.0
68.10	460.0
69.00	28440.0
74.00	2724.0
75.00	4530.0
76.00	1630.0
77.00	32480.0
78.00	2284.0
79.00	2326.0
80.00	1576.0
81.00	2275.0
81.90	576.0
83.00	565.0
84.90	627.0
86.00	755.0
86.90	344.0
91.00	518.0
92.00	661.0
93.00	4013.0
98.00	2863.0
99.00	2597.0
101.00	1450.0
102.90	441.0
103.90	817.0
105.00	812.0
106.00	308.0
107.00	11008.0
108.00	1619.0
109.10	329.0
110.00	20944.0
111.00	3089.0
112.00	443.0
116.00	685.0
117.00	8672.0
118.00	717.0
122.00	796.0
122.90	1143.0
123.90	520.0
124.90	510.0
127.00	41976.0
128.00	3092.0
129.00	15782.0
130.00	1280.0
133.90	496.0
135.00	1437.0
136.00	549.0
137.00	758.0
141.00	2254.0
142.00	700.0
142.90	498.0
146.00	384.0
147.00	1103.0
148.00	2482.0
148.90	476.0
152.90	690.0
154.00	569.0
155.00	1184.0
156.00	1950.0
157.10	443.0
157.90	446.0
159.90	635.0
161.00	993.0
161.90	314.0
164.90	883.0
166.00	686.0
167.00	4316.0
168.00	2817.0
169.00	353.0
171.90	432.0
173.00	550.0
173.90	915.0
175.00	1890.0
176.00	571.0
177.00	892.0
178.00	316.0
179.00	3474.0
180.00	2494.0
180.90	1192.0
184.00	307.0
185.00	1734.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

186.00	13649.0
187.00	3959.0
188.00	424.0
188.90	931.0
191.00	428.0
192.00	1132.0
193.00	1281.0
193.90	310.0
196.00	3307.0
198.00	109608.0
199.00	7201.0
199.90	540.0
201.30	505.0
202.90	768.0
204.00	3706.0
205.00	6543.0
206.00	27816.0
207.00	3843.0
208.00	960.0
208.90	421.0
211.00	1275.0
216.00	631.0
217.00	6979.0
218.00	1000.0
221.00	5569.0
223.00	1640.0
224.00	16075.0
225.00	4028.0
226.00	422.0
227.00	6441.0
228.00	940.0
229.00	1426.0
231.00	604.0
233.80	389.0
235.00	533.0
236.00	303.0
237.00	594.0
241.00	394.0
242.00	866.0
242.90	1020.0
244.00	13840.0
245.10	1801.0
246.00	2613.0
247.00	568.0
249.00	464.0
255.00	75152.0
256.00	10597.0
257.00	945.0
258.00	3991.0
259.00	571.0
265.00	1718.0
273.00	2257.0
274.00	6104.0
275.00	37728.0
276.00	4783.0
277.00	2981.0
278.00	510.0
282.90	383.0
284.90	517.0
293.00	720.0
296.00	10181.0
297.00	1404.0
303.00	1180.0
304.00	331.0
314.00	601.0
314.90	1239.0
316.00	696.0
321.00	428.0
323.00	3539.0
324.00	571.0
327.00	730.0
328.00	377.0
332.90	343.0
334.00	2376.0
335.00	547.0
341.00	437.0
345.90	742.0
352.00	1107.0
353.10	858.0
354.00	1118.0
365.00	5193.0
365.90	656.0
371.10	306.0
372.00	2103.0
373.10	514.0
383.00	585.0
402.00	890.0
403.00	1351.0
403.90	397.0
421.00	1007.0
422.10	1169.0
423.00	7551.0
424.00	1818.0
441.00	19160.0
442.00	119104.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

443.1022368.0

444.101899.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55

m/z	Abundance
43.90	948.0

Instrument :
BNA_N
ClientSampleId :
DFTPP55