




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
Data File : BN028804.D
Acq On : 20 Nov 2023 10:45
Operator : MA/JU
Sample : PB156953BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK953

Manual IntegrationsAPPROVED

Quant Time: Nov 20 15:30:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 06:42:12 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :mohammad ahmed 11/21/2023

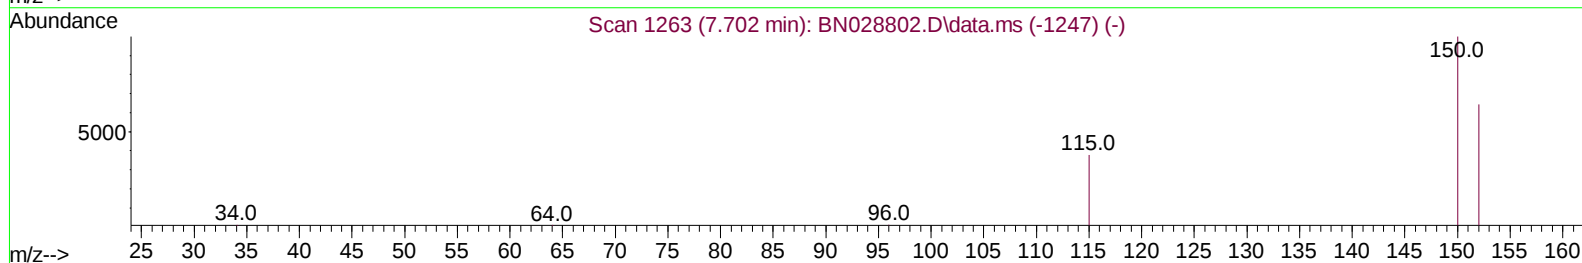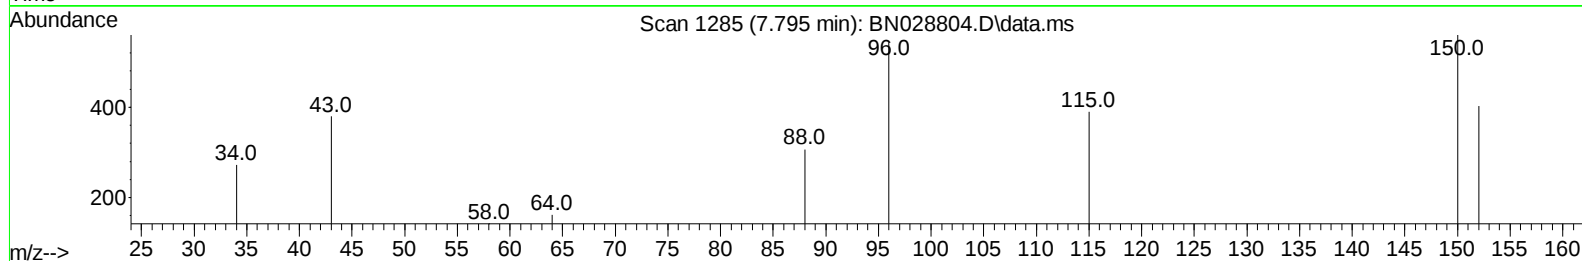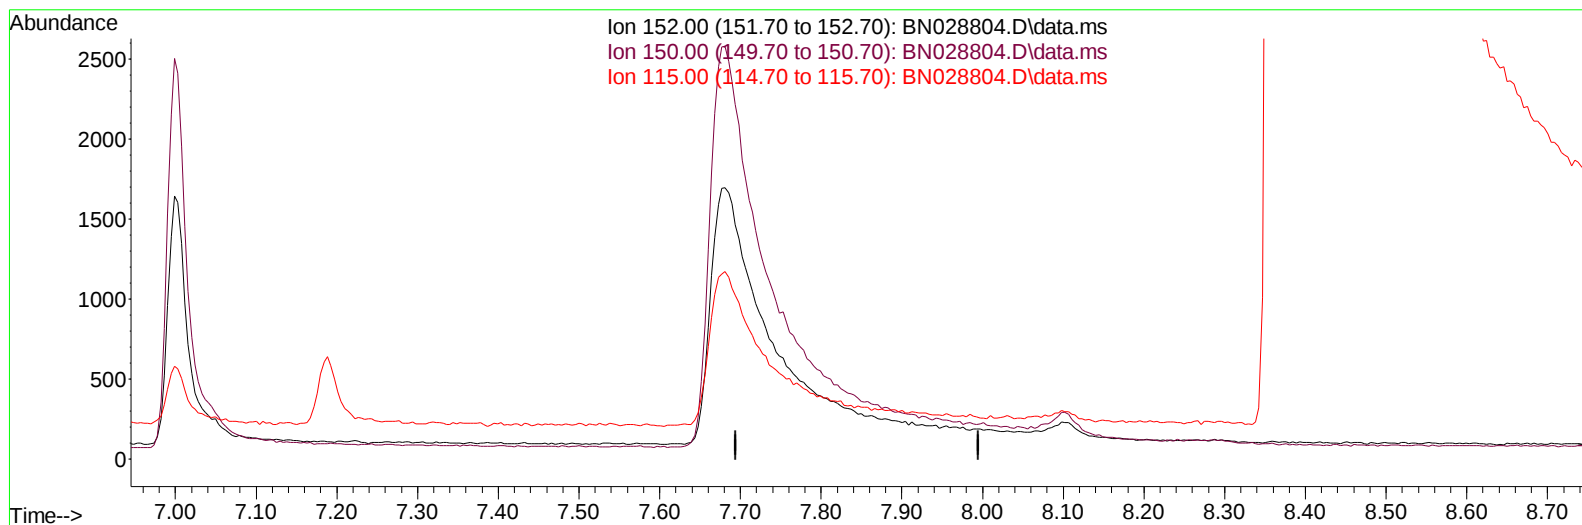

TIC: BN028804.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
Data File : BN028804.D
Acq On : 20 Nov 2023 10:45
Operator : MA/JU
Sample : PB156953BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK953

Manual IntegrationsAPPROVED

Quant Time: Nov 20 15:30:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 06:42:12 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :mohammad ahmed 11/21/2023

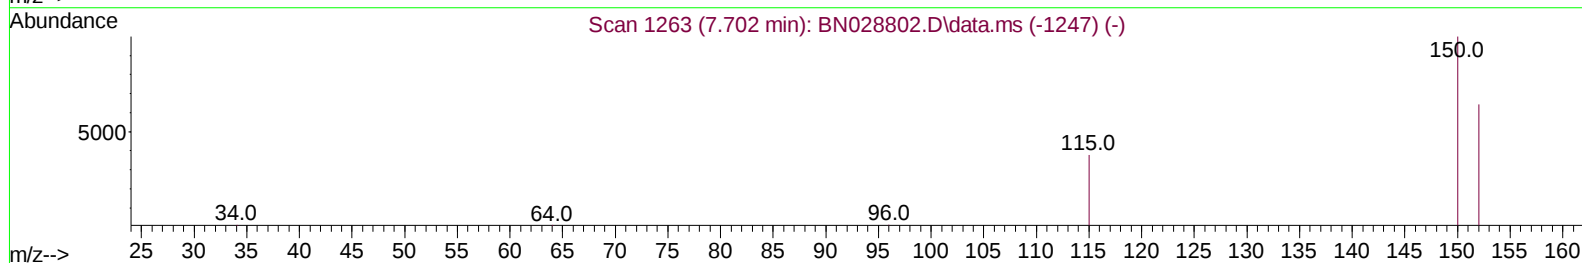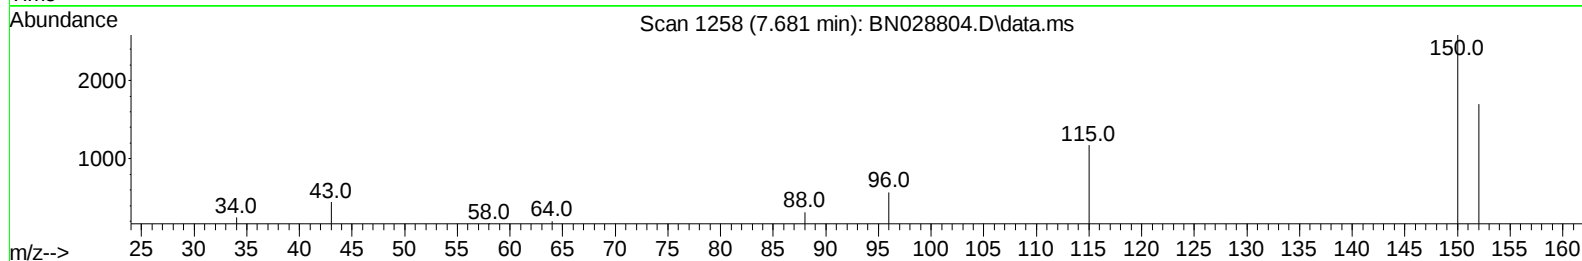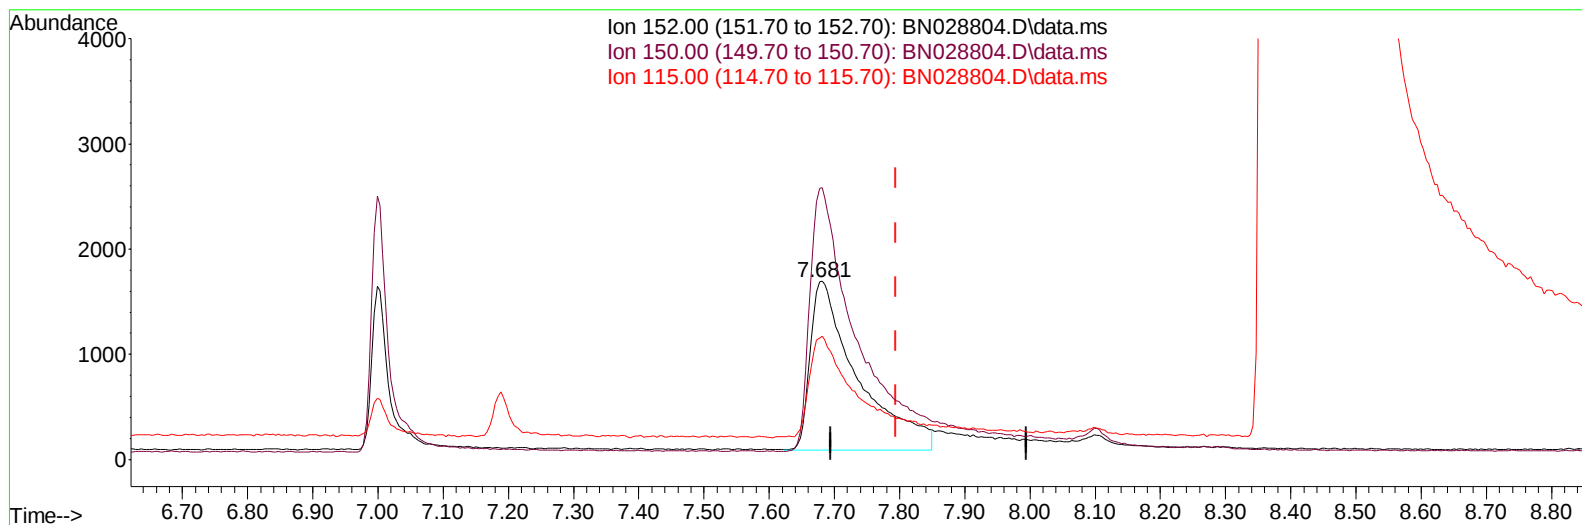

TIC: BN028804.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.681min (-0.114) 0.40 ng/ul m

response 8112

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	152.27
115.00	62.20	69.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
 Data File : BN028804.D
 Acq On : 20 Nov 2023 10:45
 Operator : MA/JU
 Sample : PB156953BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK953

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :mohammad ahmed 11/21/2023

Quant Time: Nov 20 15:30:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 06:42:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	8112m	0.400	ng/ul	-0.11
4) Naphthalene-d8	10.451	136	33088	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.311	164	17947	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.064	188	33260	0.400	ng/ul	-0.03
17) Chrysene-d12	21.284	240	18963	0.400	ng/ul	-0.01
23) Perylene-d12	23.563	264	26335	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	46954	5.237	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.074	152	7187	0.144	ng/ul	-0.04
18) Fluoranthene-d10	19.103	212	18256	0.299	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
Data File : BN028804.D
Acq On : 20 Nov 2023 10:45
Operator : MA/JU
Sample : PB156953BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK953

Manual IntegrationsAPPROVED

Quant Time: Nov 20 15:30:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 06:42:12 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :mohammad ahmed 11/21/2023

