




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
Data File : BN028806.D
Acq On : 20 Nov 2023 11:56
Operator : MA/JU
Sample : 05239-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ0

Manual IntegrationsAPPROVED

Quant Time: Nov 20 15:30:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 06:42:12 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :mohammad ahmed 11/21/2023

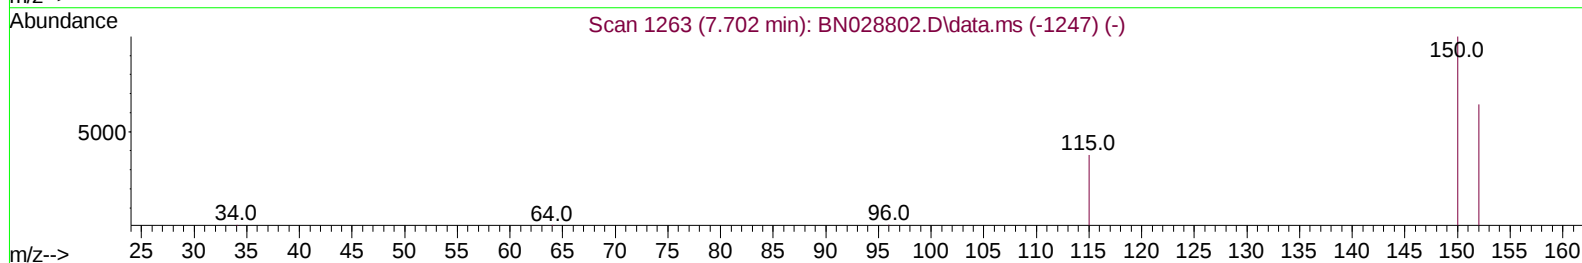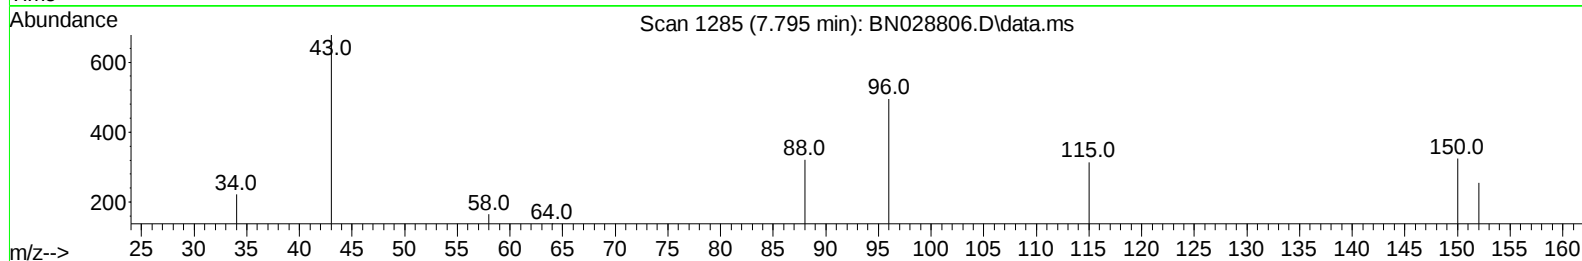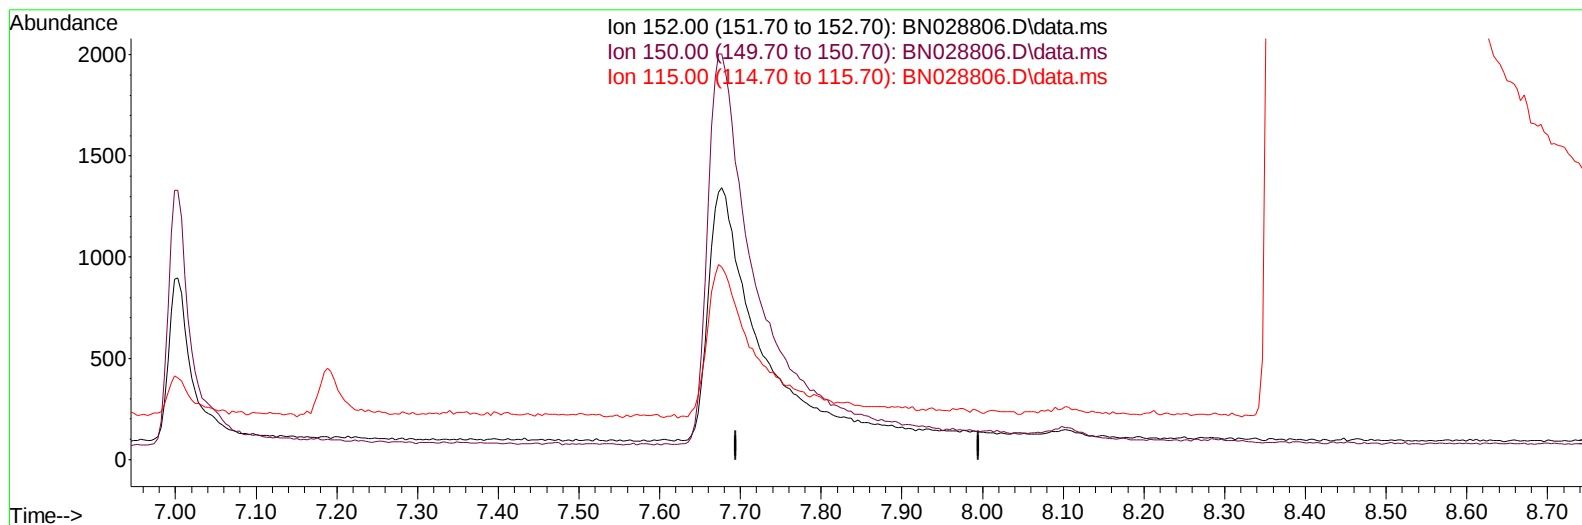

TIC: BN028806.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
Data File : BN028806.D
Acq On : 20 Nov 2023 11:56
Operator : MA/JU
Sample : 05239-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ0

Manual IntegrationsAPPROVED

Quant Time: Nov 20 15:30:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 06:42:12 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :mohammad ahmed 11/21/2023

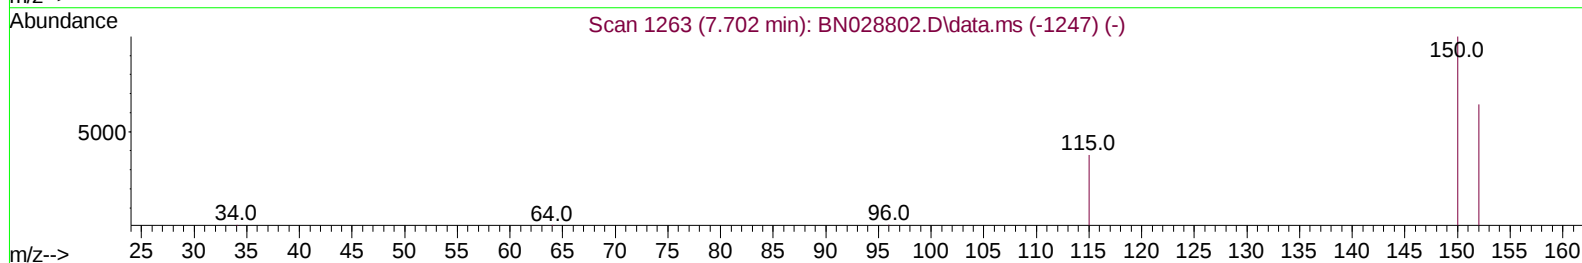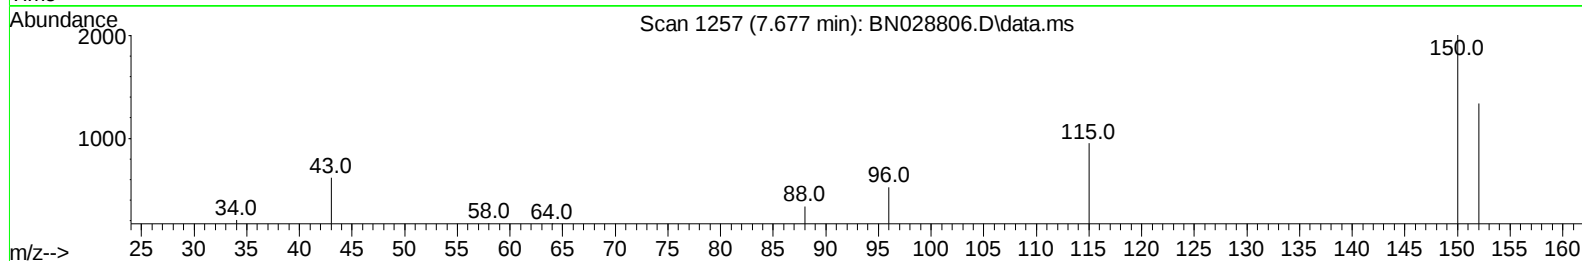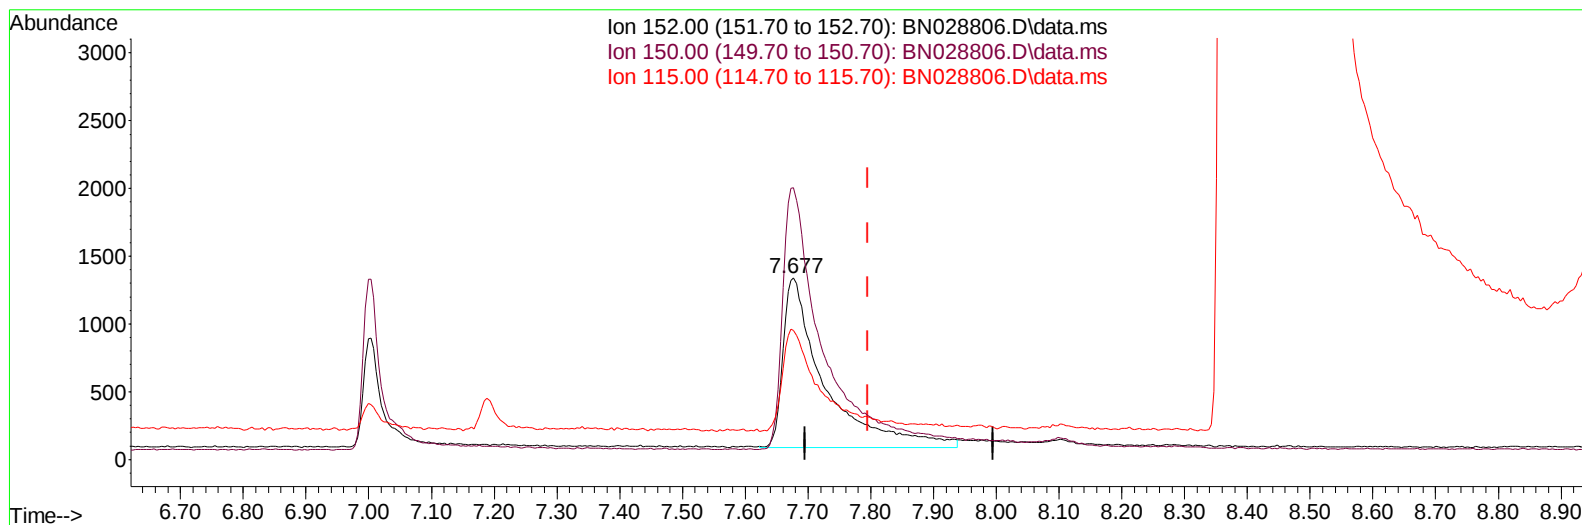

TIC: BN028806.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.677min (-0.118) 0.40 ng/ul m

response 5767

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	149.33
115.00	62.20	70.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
 Data File : BN028806.D
 Acq On : 20 Nov 2023 11:56
 Operator : MA/JU
 Sample : 05239-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :mohammad ahmed 11/21/2023

Quant Time: Nov 20 15:30:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 06:42:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.677	152	5767m	0.400	ng/ul	-0.12
4) Naphthalene-d8	10.450	136	20187	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.310	164	10425	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.067	188	18868	0.400	ng/ul	-0.02
17) Chrysene-d12	21.285	240	11377	0.400	ng/ul	#-0.01
23) Perylene-d12	23.562	264	15175	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.108	96	44484	6.979	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.067	152	5008	0.165	ng/ul	-0.05
18) Fluoranthene-d10	19.106	212	12345	0.337	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112023\
Data File : BN028806.D
Acq On : 20 Nov 2023 11:56
Operator : MA/JU
Sample : 05239-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ0

Manual IntegrationsAPPROVED

Quant Time: Nov 20 15:30:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 06:42:12 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :mohammad ahmed 11/21/2023

