
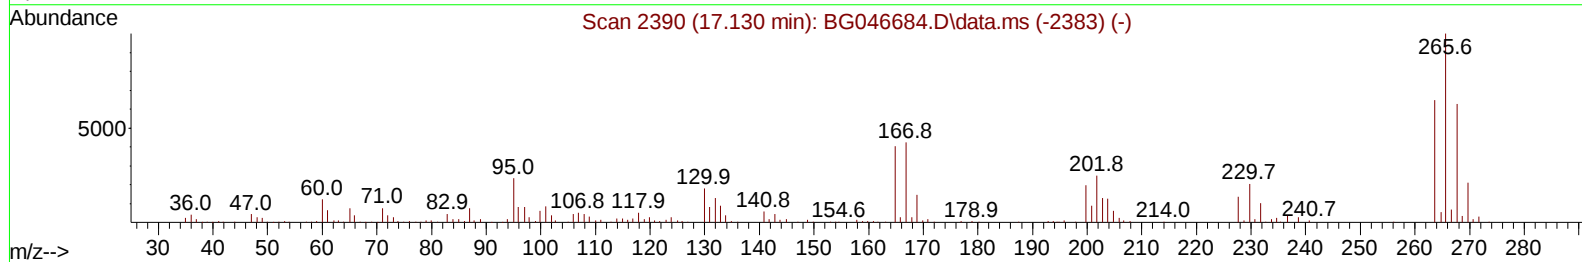
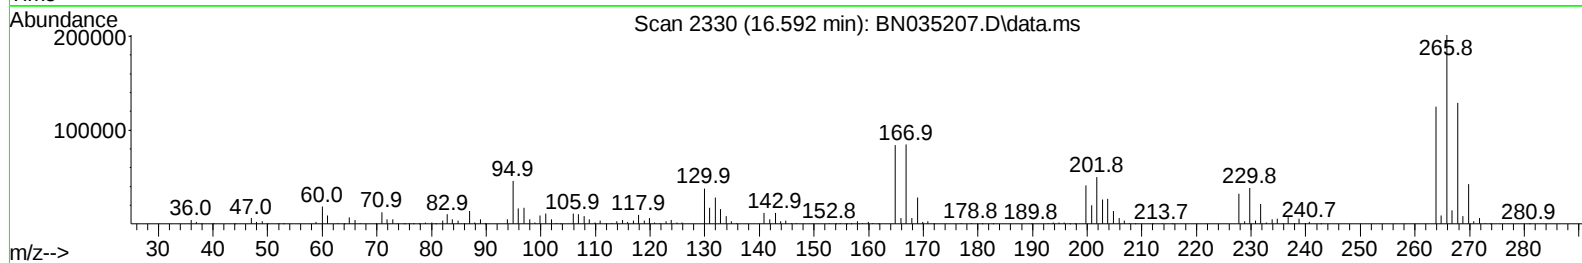


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
Data File : BN035207.D
Acq On : 20 Nov 2024 21:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 03:22:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

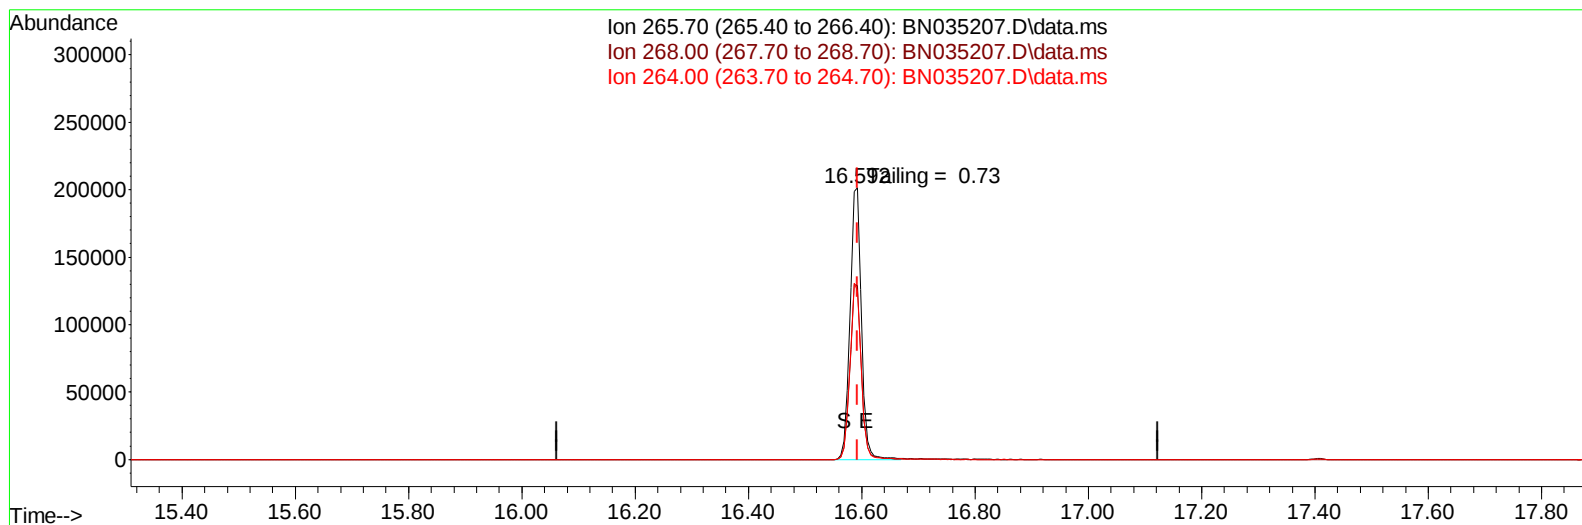




TIC: BN035207.D\data.ms

(70) Pentachlorophenol (C)**16.592min (0.000) 20960.50 ng****response 284079**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.09
264.00	61.60	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
Data File : BN035207.D
Acq On : 20 Nov 2024 21:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 03:22:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

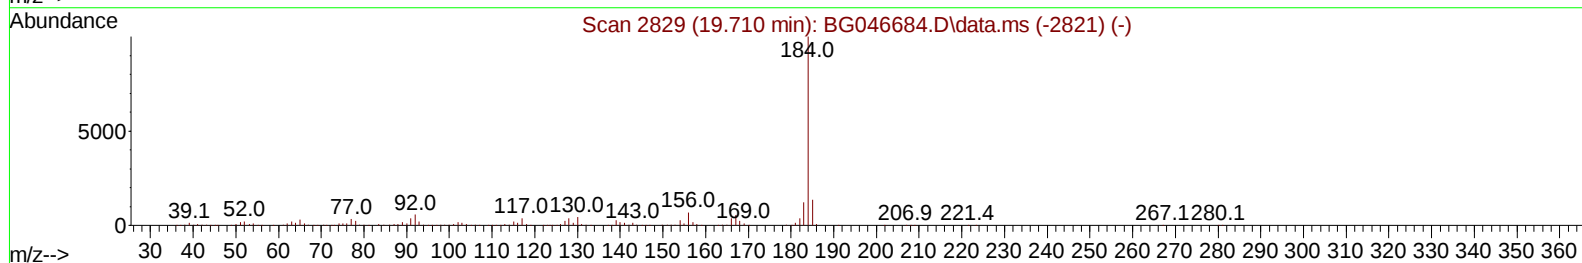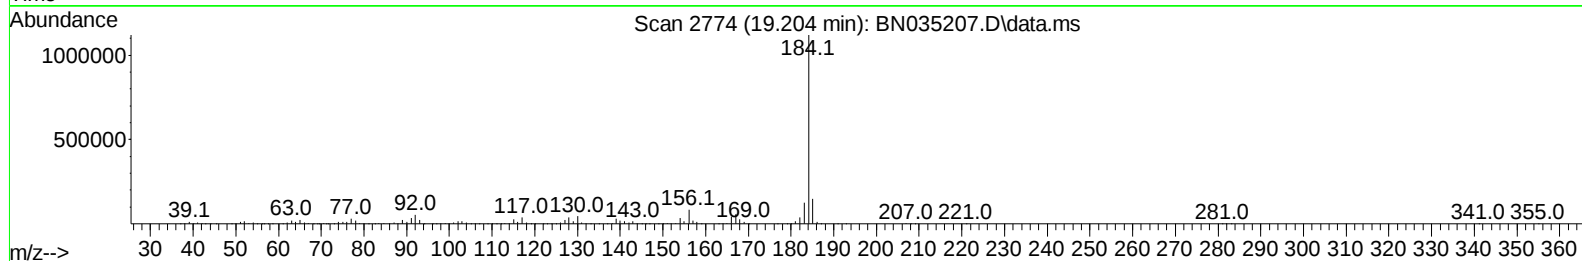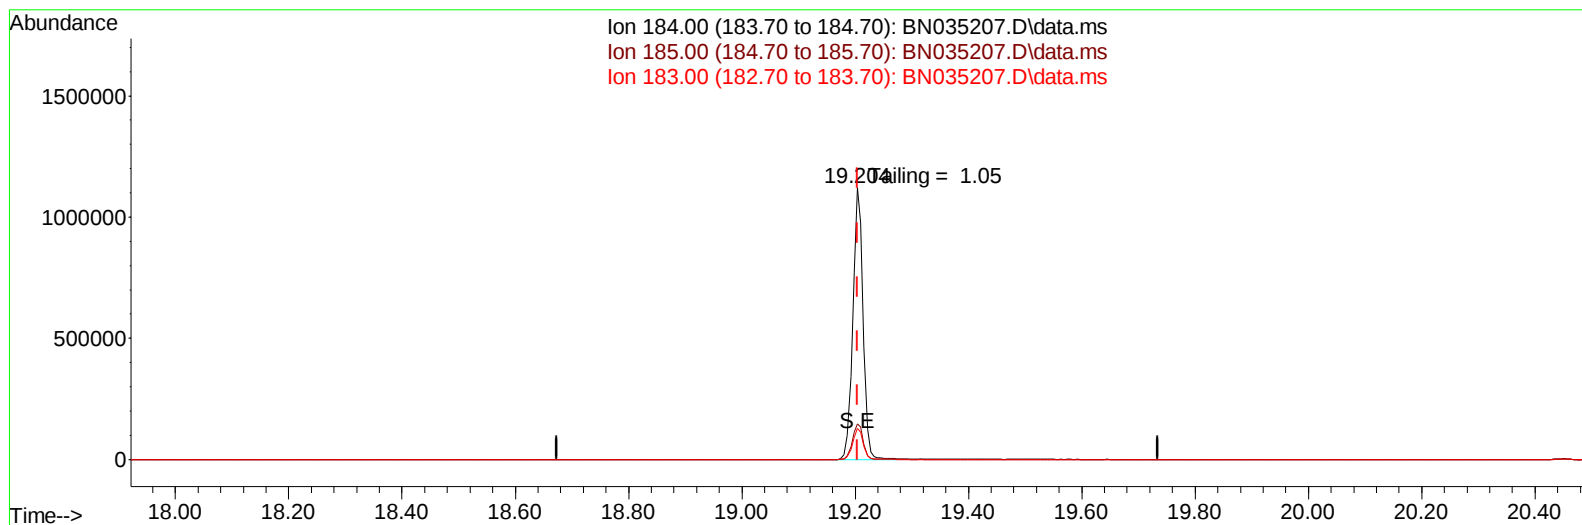

TIC: BN035207.D\data.ms

(77) Benzidine

19.204min (0.000) 0.00 ng

response 1412217

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.20
183.00	13.20	11.37
0.00	0.00	0.00