

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
 Data File : BN035215.D
 Acq On : 21 Nov 2024 02:37
 Operator : RC/JU
 Sample : P4868-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RW5-SP201-20241114

Quant Time: Nov 21 03:05:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 20 23:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	2985	0.400	ng	0.00
7) Naphthalene-d8	10.298	136	6800	0.400	ng	# 0.00
13) Acenaphthene-d10	14.179	164	2509	0.400	ng	0.00
19) Phenanthrene-d10	16.933	188	8217	0.400	ng	# 0.00
29) Chrysene-d12	21.151	240	1355	0.400	ng	# 0.00
35) Perylene-d12	23.320	264	327	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.170	112	980	0.129	ng	0.00
5) Phenol-d6	6.723	99	1359	0.143	ng	0.00
8) Nitrobenzene-d5	8.675	82	2136	0.361	ng	0.00
11) 2-Methylnaphthalene-d10	11.901	152	3820	0.315	ng	0.00
14) 2,4,6-Tribromophenol	15.679	330	850	0.470	ng	0.00
15) 2-Fluorobiphenyl	12.790	172	8110	0.796	ng	0.00
27) Fluoranthene-d10	18.973	212	5721	0.227	ng	0.00
31) Terphenyl-d14	19.587	244	8309	2.922	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.184	88	340	0.125	ng	# 78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
Data File : BN035215.D
Acq On : 21 Nov 2024 02:37
Operator : RC/JU
Sample : P4868-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RW5-SP201-20241114


Quant Time: Nov 21 03:05:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 20 23:40:20 2024
Response via : Initial Calibration

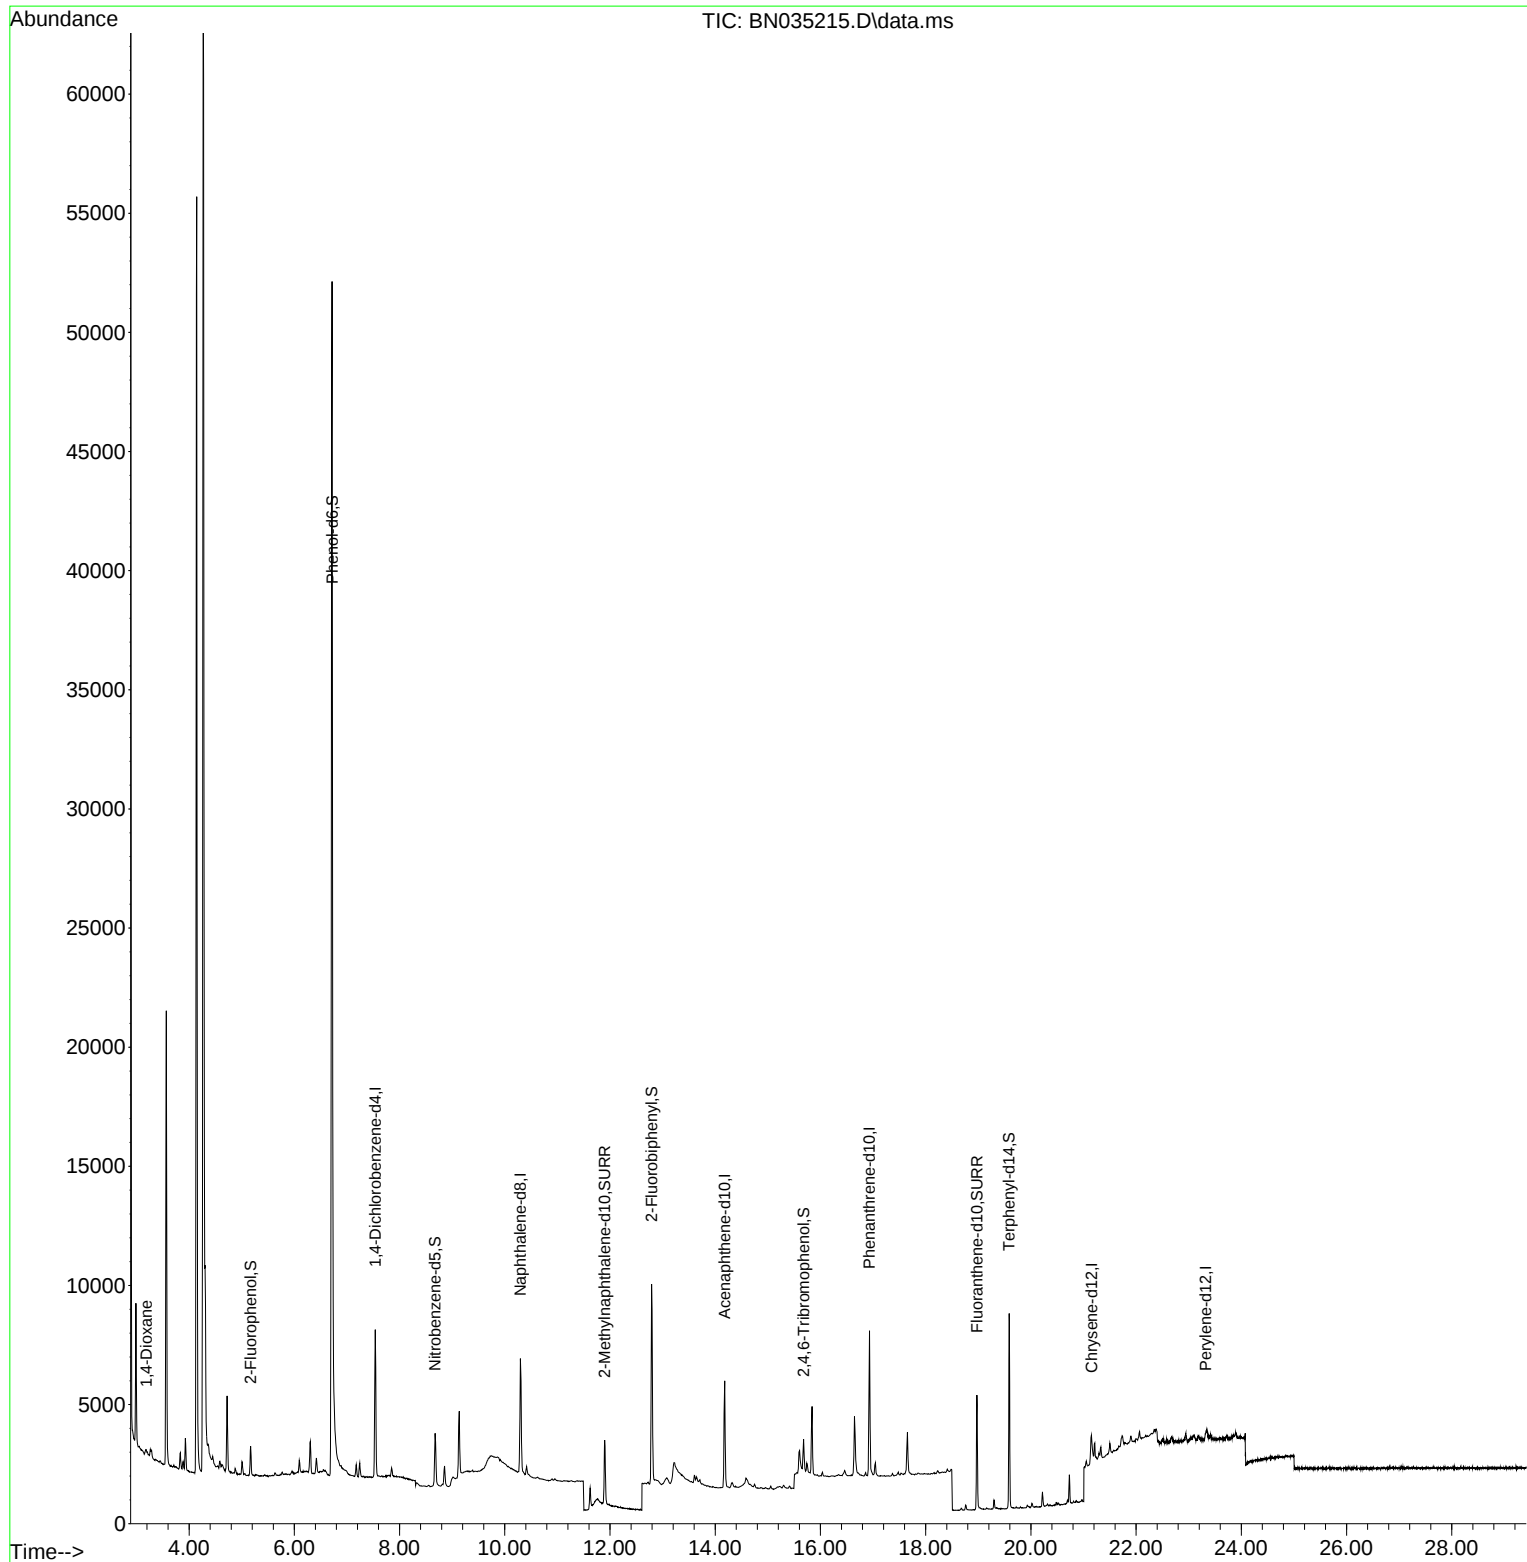






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.539 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN035215.D
 Acq: 21 Nov 2024 02:37

Instrument :
 BNA_N
 ClientSampleId :
 RW5-SP201-20241114



Tgt Ion:152 Resp: 2985




Ion	Ratio	Lower	Upper
152	100		
150	151.1	124.5	186.7
115	64.3	47.8	71.6

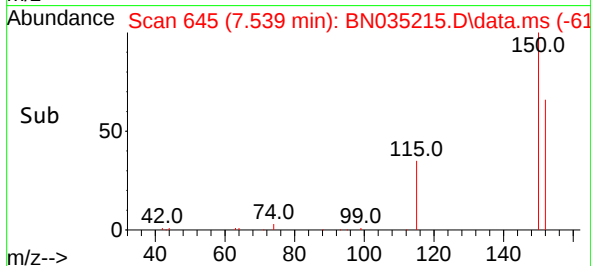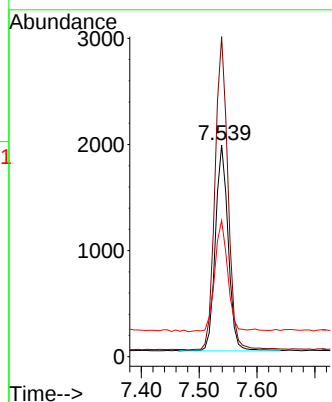


#2
 1,4-Dioxane
 Concen: 0.125 ng
 RT: 3.184 min Scan# 42
 Delta R.T. 0.014 min
 Lab File: BN035215.D
 Acq: 21 Nov 2024 02:37

Tgt Ion: 88 Resp: 340

Ion	Ratio	Lower	Upper
88	100		
43	0.0	16.9	25.3#
58	57.1	39.0	58.4


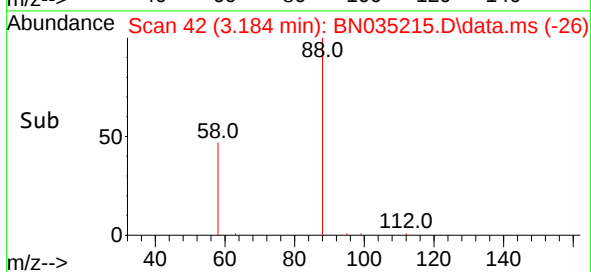
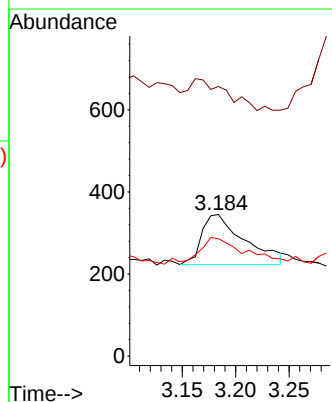
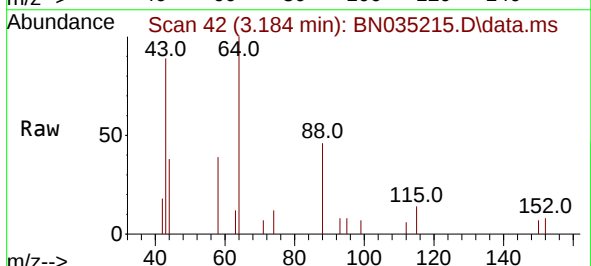


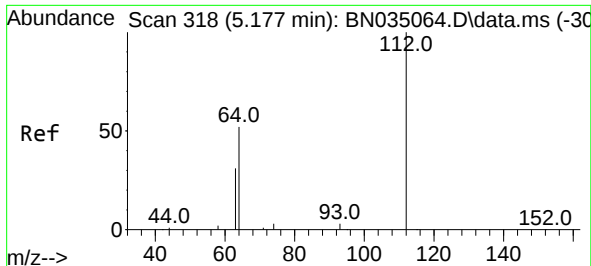

#4
2-Fluorophenol
Concen: 0.129 ng
RT: 5.170 min Scan# 31
Delta R.T. 0.000 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37




Instrument :
BNA_N
ClientSampleId :
RW5-SP201-20241114


Tgt Ion:112 Resp: 980
Ion Ratio Lower Upper
112 100
64 52.3 39.7 59.5
63 32.1 23.0 34.4

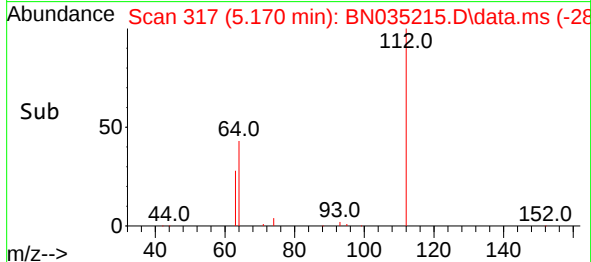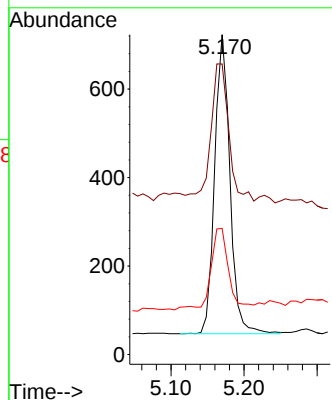

#5
Phenol-d6
Concen: 0.143 ng
RT: 6.723 min Scan# 532
Delta R.T. 0.000 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37

Tgt Ion: 99 Resp: 1359
Ion Ratio Lower Upper
99 100
42 55.3 11.4 17.0#
71 266.3 34.6 51.8#

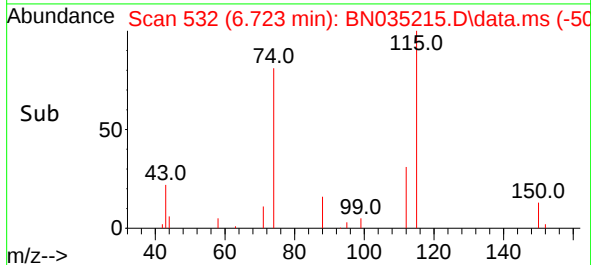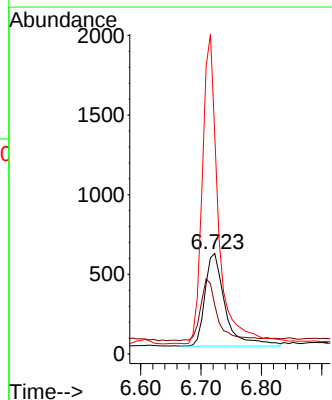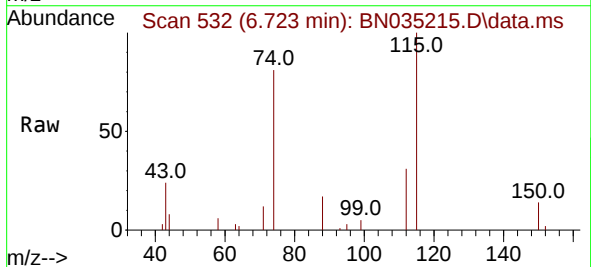



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.298 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN035215.D

Acq: 21 Nov 2024 02:37

Instrument :

BNA_N

ClientSampleId :

RW5-SP201-20241114

Tgt Ion:136 Resp: 6800





Ion Ratio Lower Upper

136 100

137 25.1 9.8 14.8#

54 6.4 4.0 6.0#

68 6.2 4.2 6.2

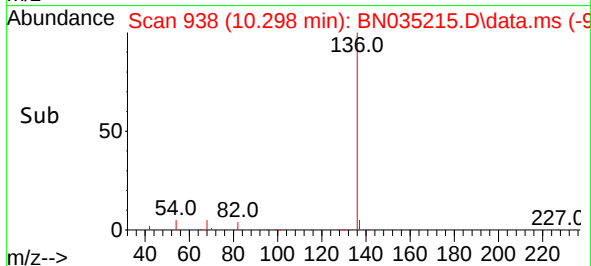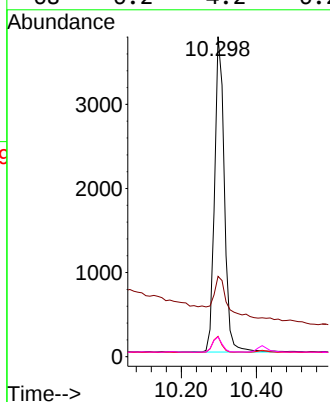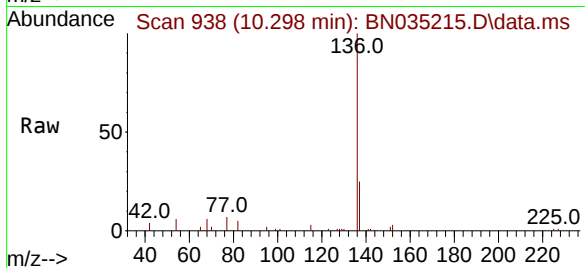

#8

Nitrobenzene-d5

Concen: 0.361 ng

RT: 8.675 min Scan# 786

Delta R.T. 0.000 min

Lab File: BN035215.D

Acq: 21 Nov 2024 02:37




Tgt Ion: 82 Resp: 2136


Ion Ratio Lower Upper

82 100

128 38.5 36.5 54.7


54 38.3 28.7 43.1

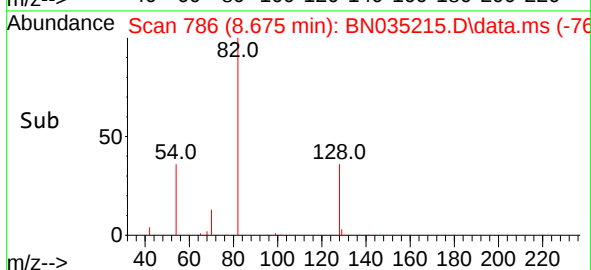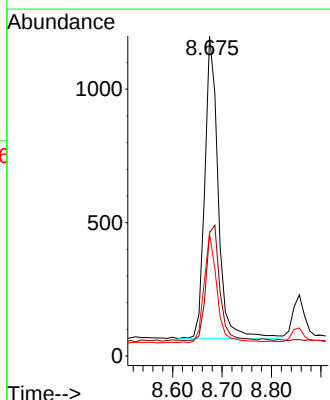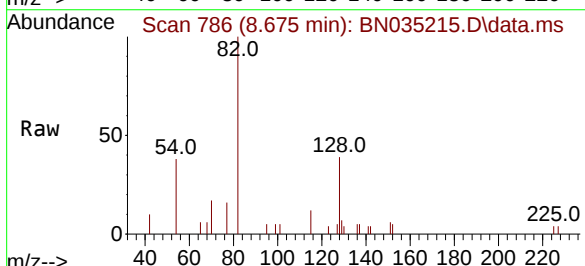



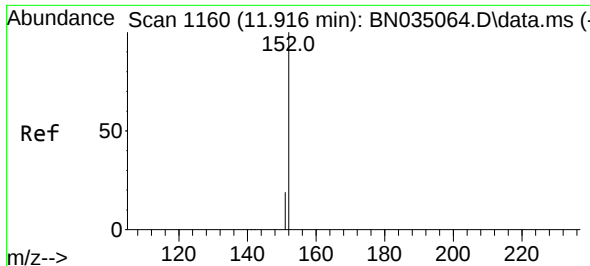


#11
2-Methylnaphthalene-d10
Concen: 0.315 ng
RT: 11.901 min Scan# 1156
Delta R.T. 0.004 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37

Instrument :
BNA_N
ClientSampleId :
RW5-SP201-20241114



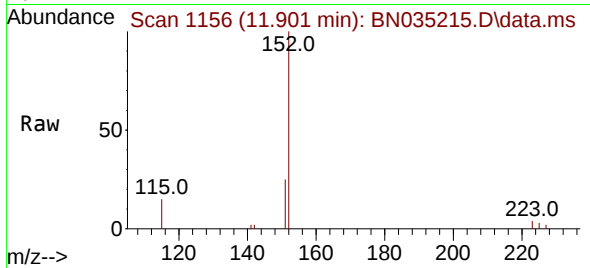



Tgt Ion:152 Resp: 3820
Ion Ratio Lower Upper
152 100
151 22.9 16.2 24.4

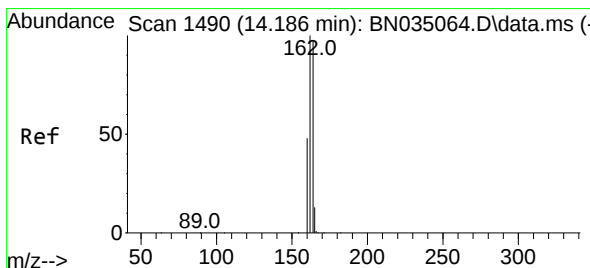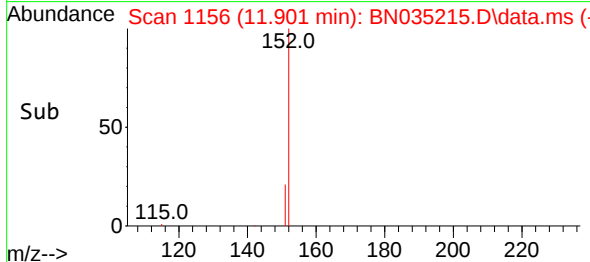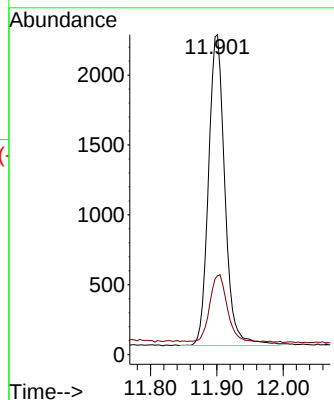

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.179 min Scan# 1490
Delta R.T. 0.004 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37

Tgt Ion:164 Resp: 2509
Ion Ratio Lower Upper
164 100
162 103.9 82.2 123.2
160 52.1 40.2 60.4


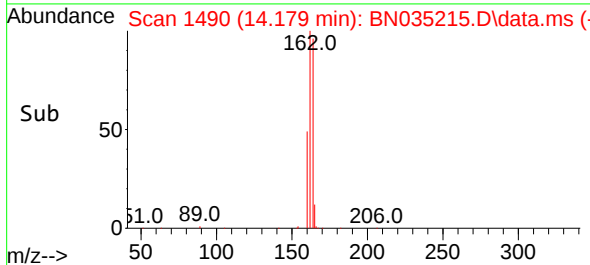
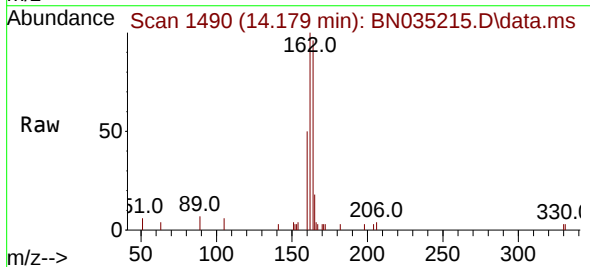
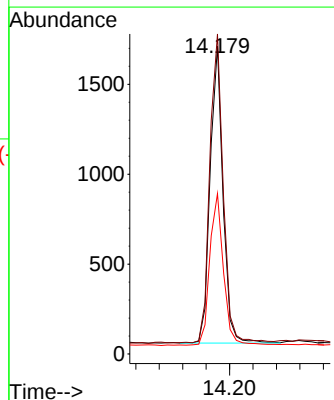


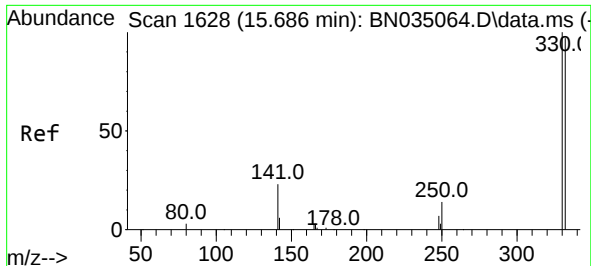

#14
2,4,6-Tribromophenol
Concen: 0.470 ng
RT: 15.679 min Scan# 1
Delta R.T. 0.006 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37




Instrument :
BNA_N
ClientSampleId :
RW5-SP201-20241114


Tgt Ion:330 Resp: 850
Ion Ratio Lower Upper
330 100
332 93.2 76.9 115.3
141 36.2 29.6 44.4

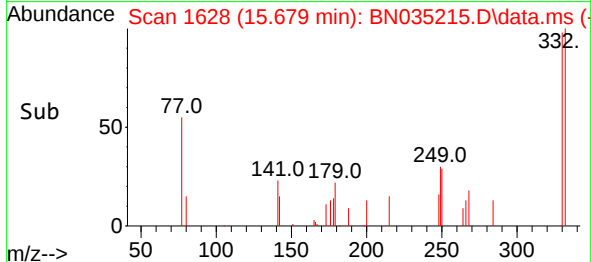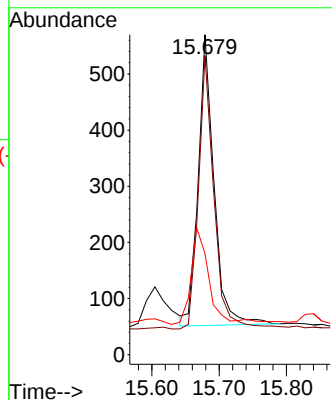

#15
2-Fluorobiphenyl
Concen: 0.796 ng
RT: 12.790 min Scan# 1360
Delta R.T. -0.007 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37

Tgt Ion:172 Resp: 8110
Ion Ratio Lower Upper
172 100
171 35.6 28.2 42.4
170 24.4 19.0 28.6


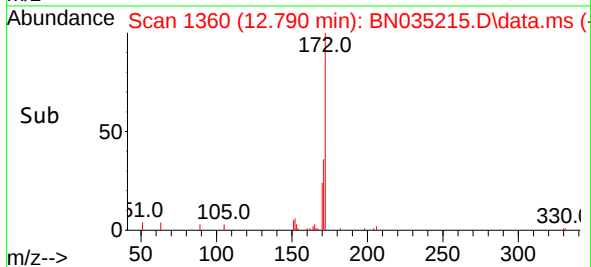
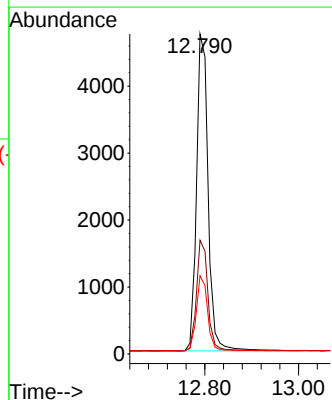
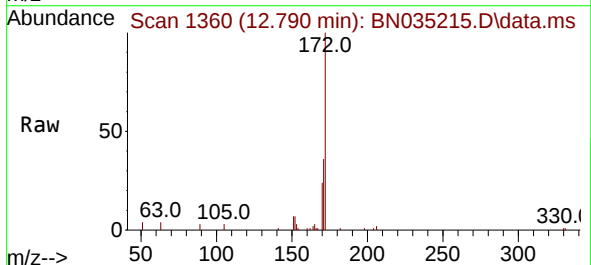


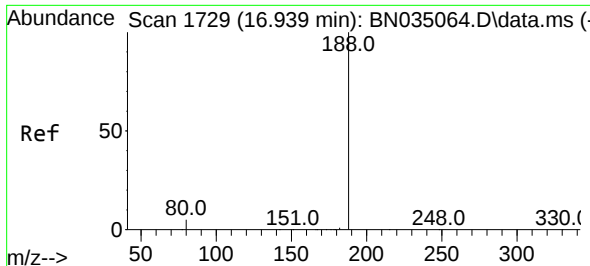

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.933 min Scan# 1729
Delta R.T. 0.006 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37




Instrument :
BNA_N
ClientSampleId :
RW5-SP201-20241114


Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.5	4.3	6.5

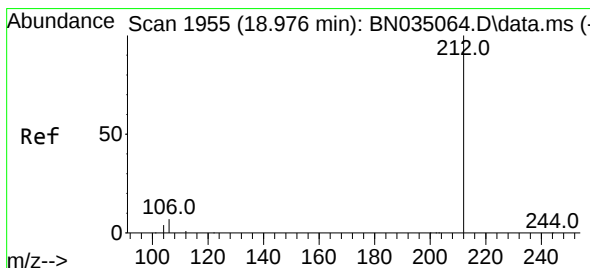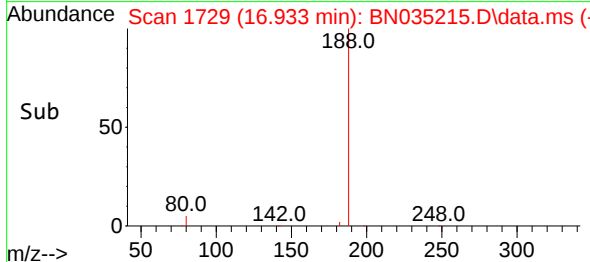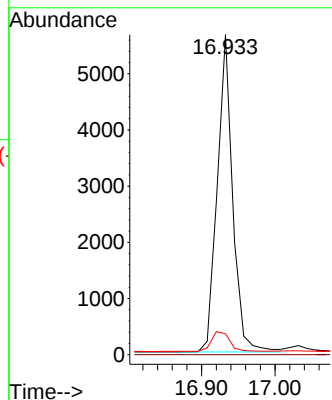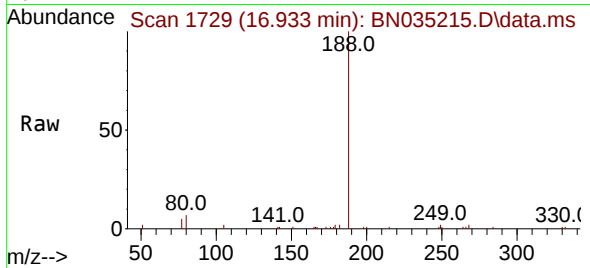

#27
Fluoranthene-d10
Concen: 0.227 ng
RT: 18.973 min Scan# 1956
Delta R.T. -0.002 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37

Tgt Ion	Ratio	Lower	Upper
212	100		
106	8.0	6.0	9.0
104	5.2	3.5	5.3

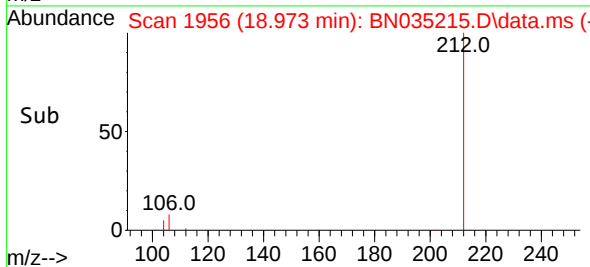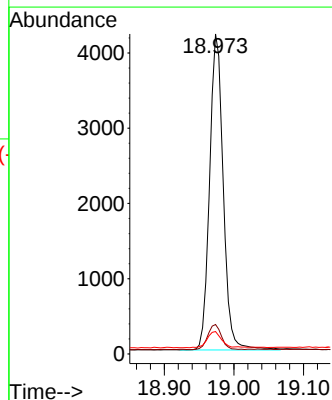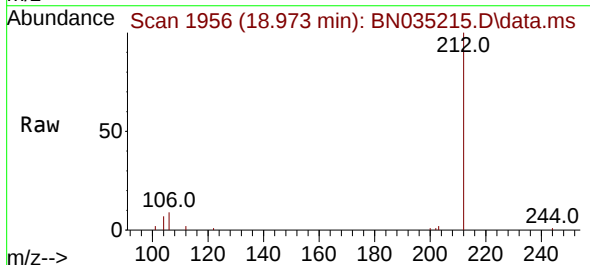



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.151 min Scan# 2410

Delta R.T. 0.002 min

Lab File: BN035215.D

Acq: 21 Nov 2024 02:37

Instrument :

BNA_N

ClientSampleId :

RW5-SP201-20241114





Tgt Ion:240 Resp: 1355

Ion Ratio Lower Upper

240 100

120 24.4 3.8 5.6#

236 50.3 22.2 33.2#

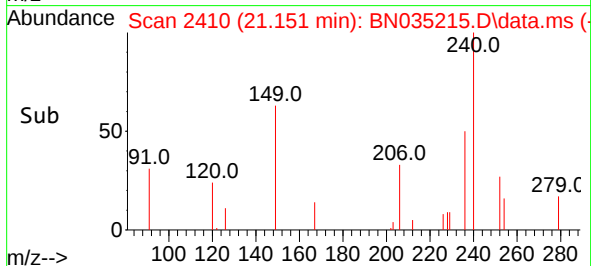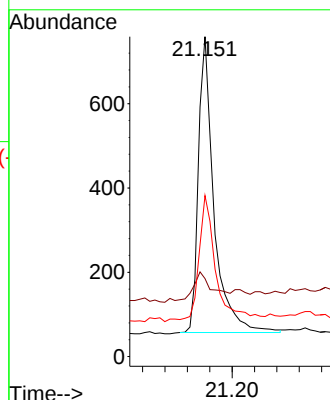

#31

Terphenyl-d14

Concen: 2.922 ng

RT: 19.587 min Scan# 2088

Delta R.T. -0.002 min

Lab File: BN035215.D

Acq: 21 Nov 2024 02:37




Tgt Ion:244 Resp: 8309


Ion Ratio Lower Upper

244 100

212 10.1 7.6 11.4


122 10.1 6.1 9.1#

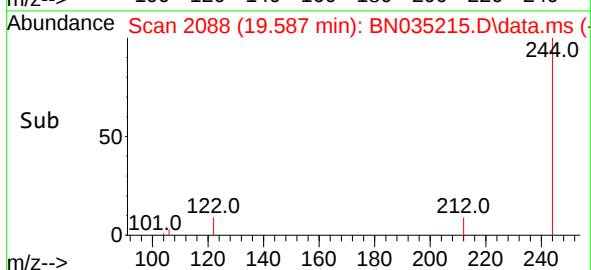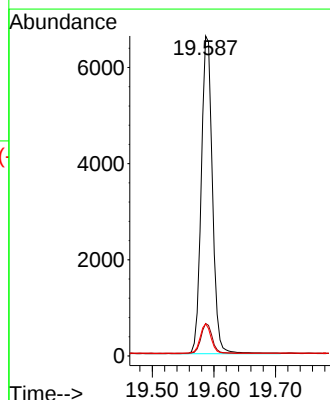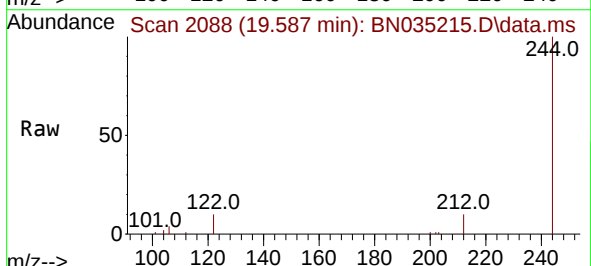

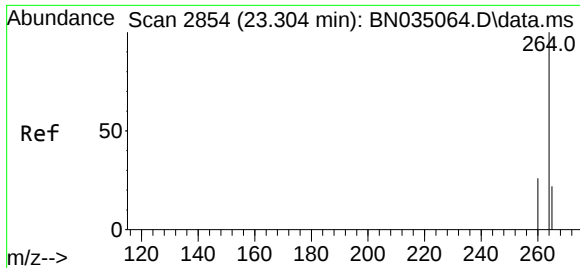

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.320 min Scan# 21
Delta R.T. -0.001 min
Lab File: BN035215.D
Acq: 21 Nov 2024 02:37

Instrument :
BNA_N
ClientSampleId :
RW5-SP201-20241114

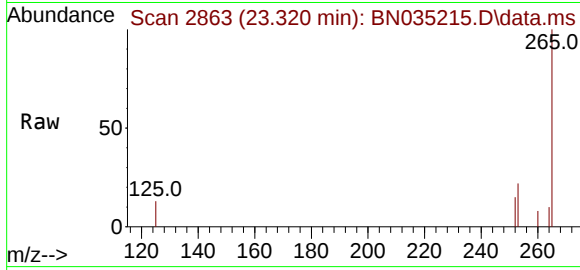

Tgt Ion:264 Resp: 327
Ion Ratio Lower Upper
264 100
260 81.8 20.9 31.3#
265 1025.9 35.4 53.2#

