
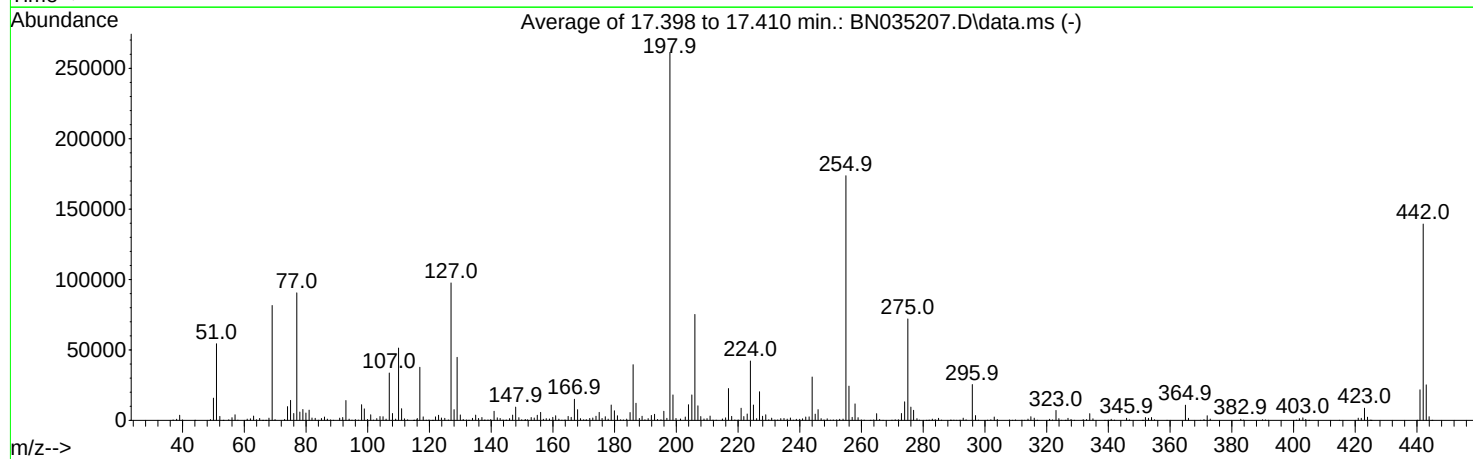


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
Data File : BN035207.D
Acq On : 20 Nov 2024 21:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 14:00:03 2024

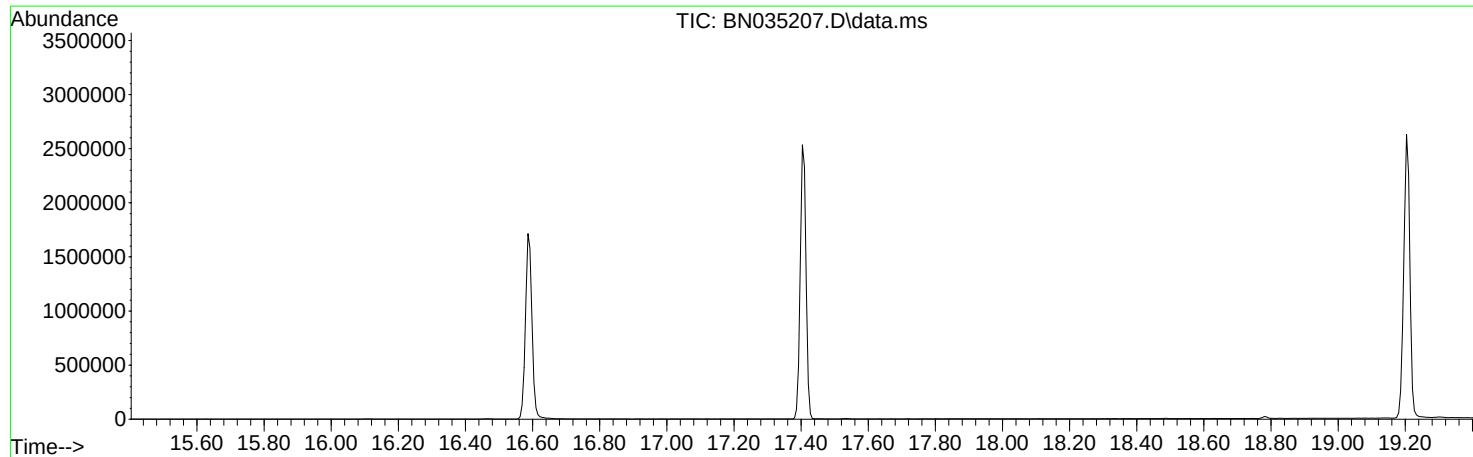




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	54397	PASS
68	69	0.00	2	1.9	1589	PASS
69	198	0.00	100	31.2	81528	PASS
70	69	0.00	2	0.7	544	PASS
127	198	10	80	37.4	97579	PASS
197	198	0.00	2	0.5	1425	PASS
198	198	100	100	100.0	261205	PASS
199	198	5	9	6.9	18036	PASS
275	198	10	60	27.6	72059	PASS
365	198	1	100	4.1	10827	PASS
441	198	0.01	100	8.3	21691	PASS
442	442	50	100	100.0	139451	PASS
443	442	15	24	18.1	25218	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
Data File : BN035207.D
Acq On : 20 Nov 2024 21:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 21 03:22:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

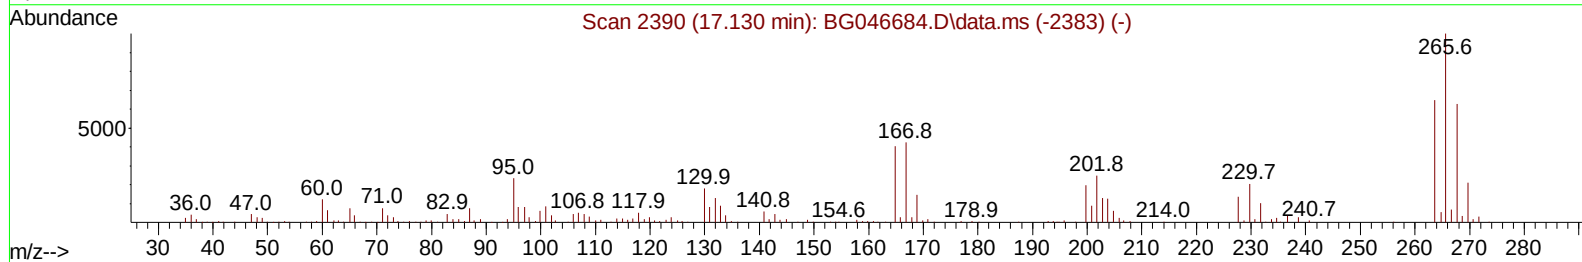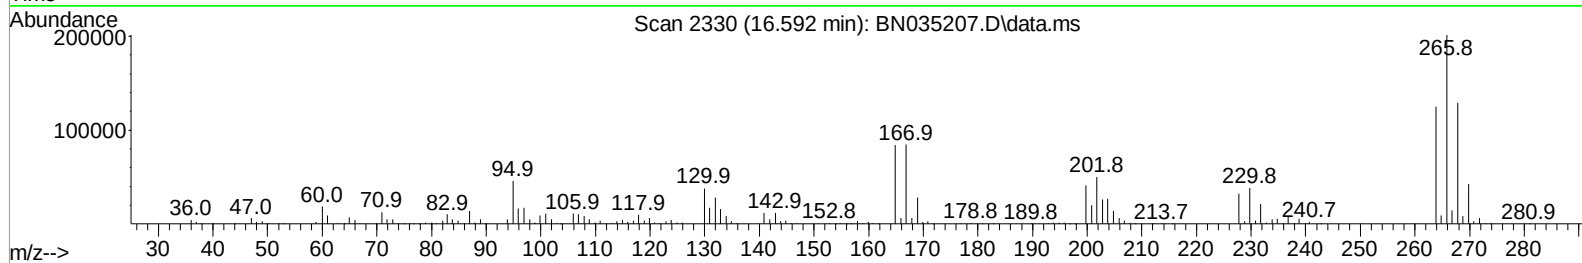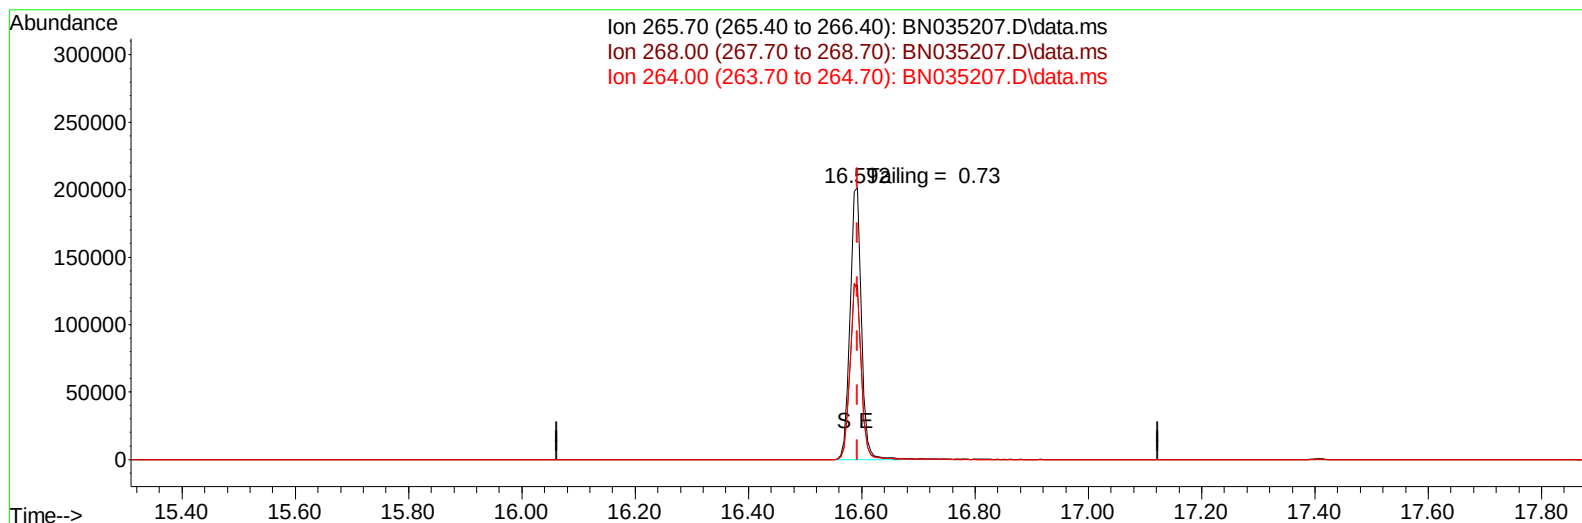

TIC: BN035207.D\data.ms

(70) Pentachlorophenol (C)

16.592min (0.000) 20960.50 ng




response 284079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.09
264.00	61.60	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112024\
Data File : BN035207.D
Acq On : 20 Nov 2024 21:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 21 03:22:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

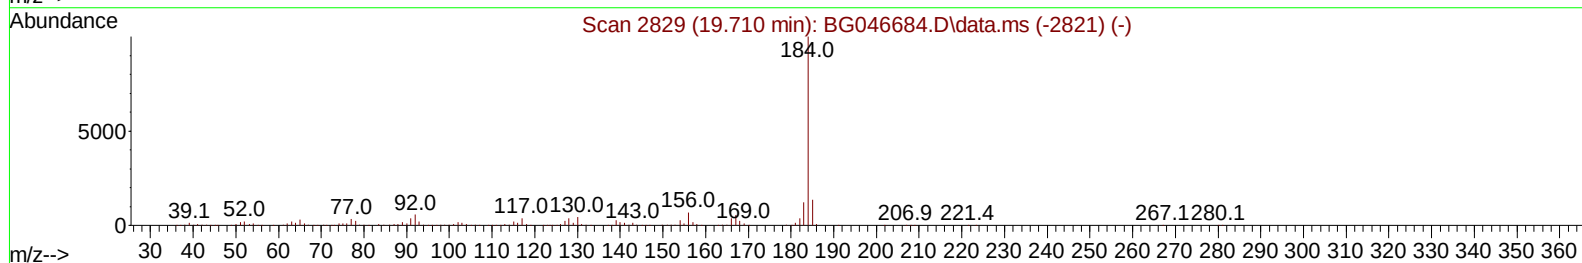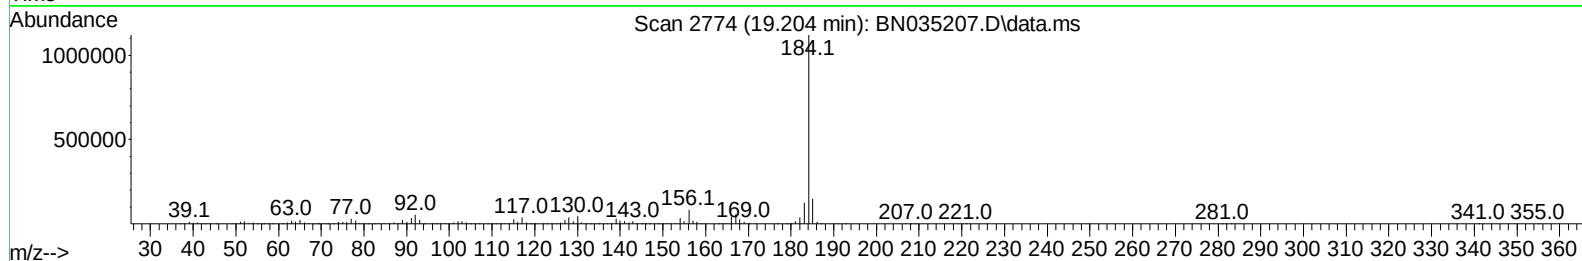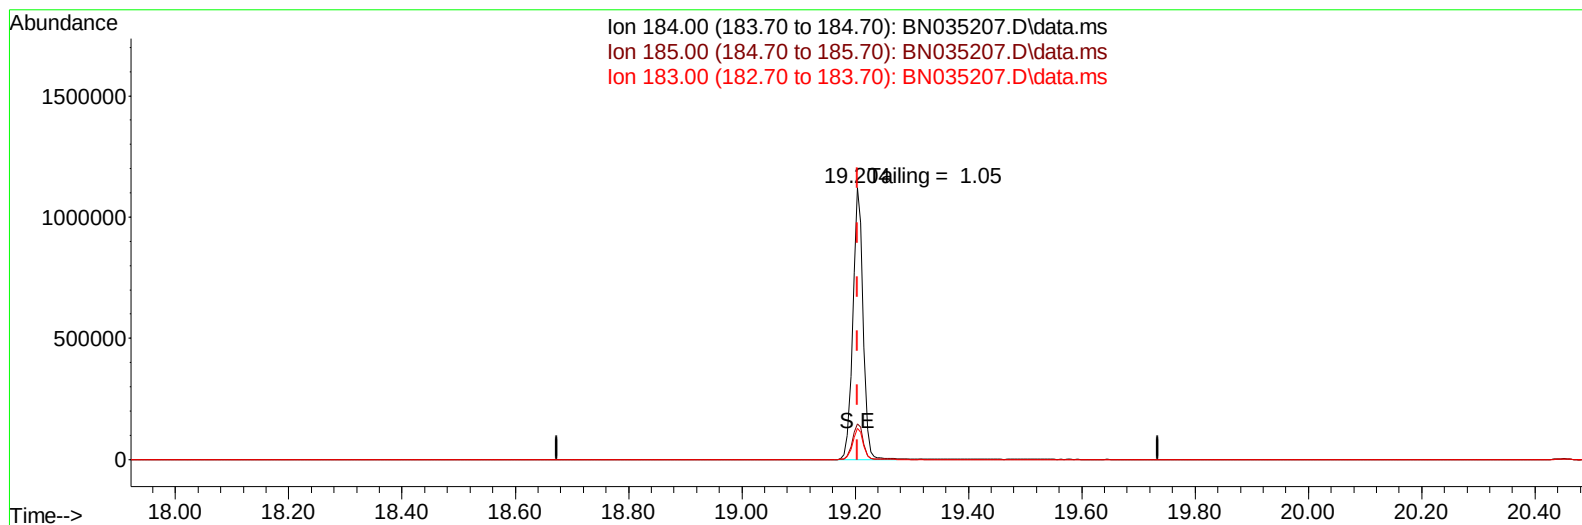

TIC: BN035207.D\data.ms

(77) Benzidine

19.204min (0.000) 0.00 ng

response 1412217

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.20
183.00	13.20	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/20/2024	BNA_N	<u>BN035207.D</u>
Compound Name	Response	Retention Time
DDT	763652	20.451
DDD	32070	20.01
DDE	860	19.498
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32930	796582	4.13

Instrument :
BNA_N
ClientSampleId :
DFTPP