
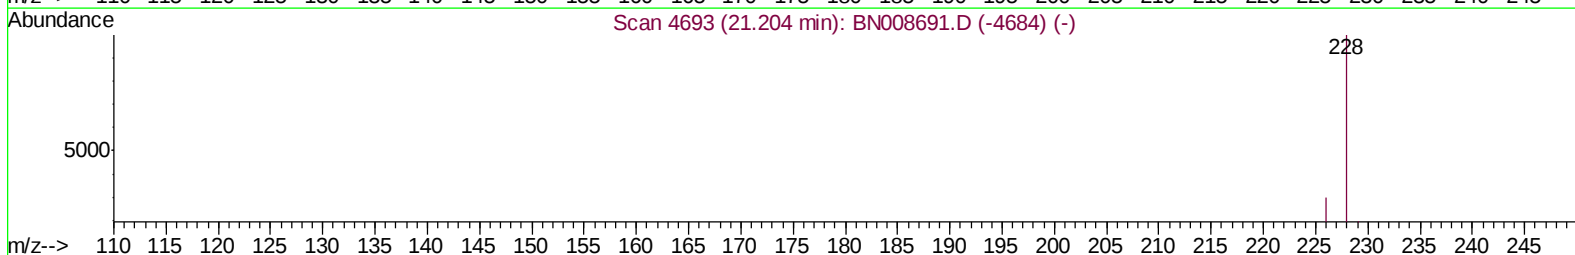
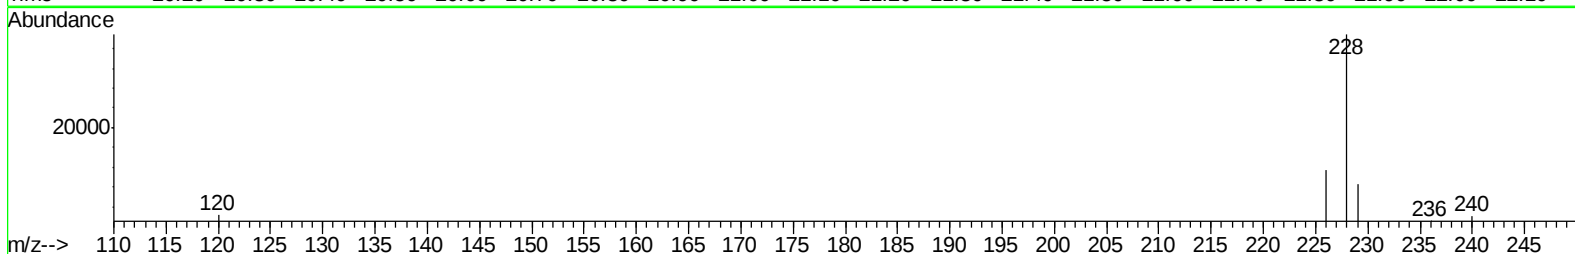


Data File : BN008702.D
Acq On : 22 Nov 2019 07:16
Operator : JU
Sample : K5854-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Nov 22 08:08:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 07:12:34 2019
Response via : Initial Calibration

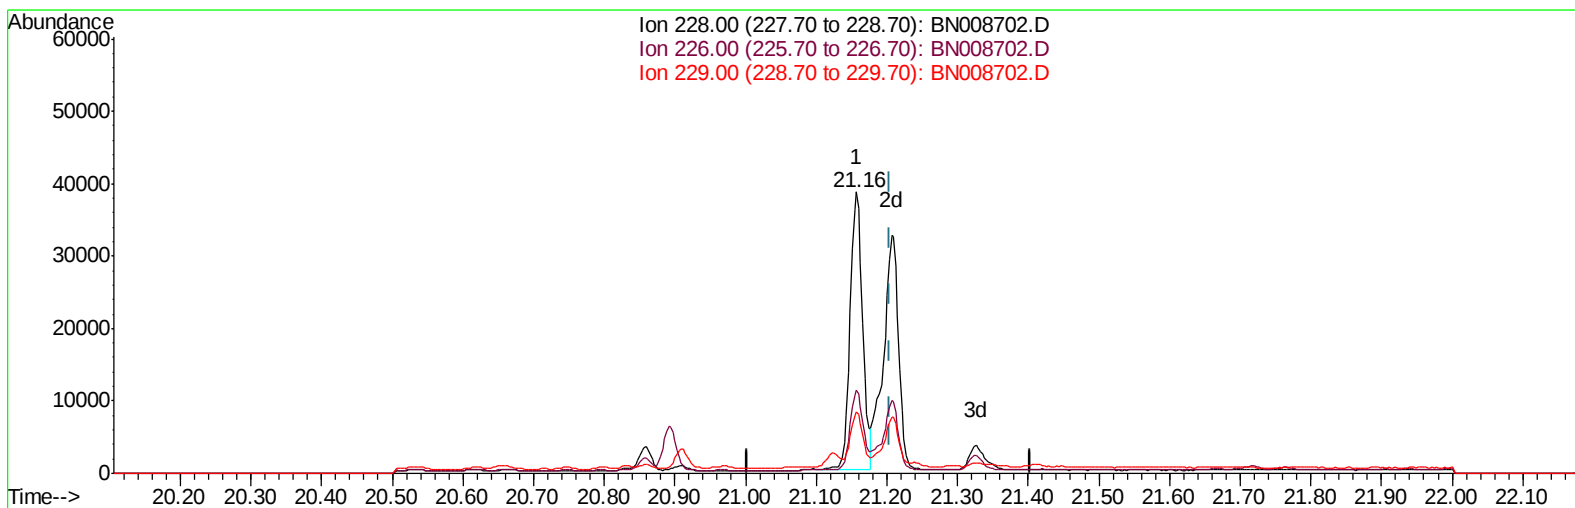

TIC: BN008702.D

(19) Chrysene

21.157min (-0.047) 0.81ng/ul

response 47540

Ion	Exp%	Act%
228.00	100	100
226.00	30.60	29.44
229.00	19.40	21.85
0.00	0.00	0.00