
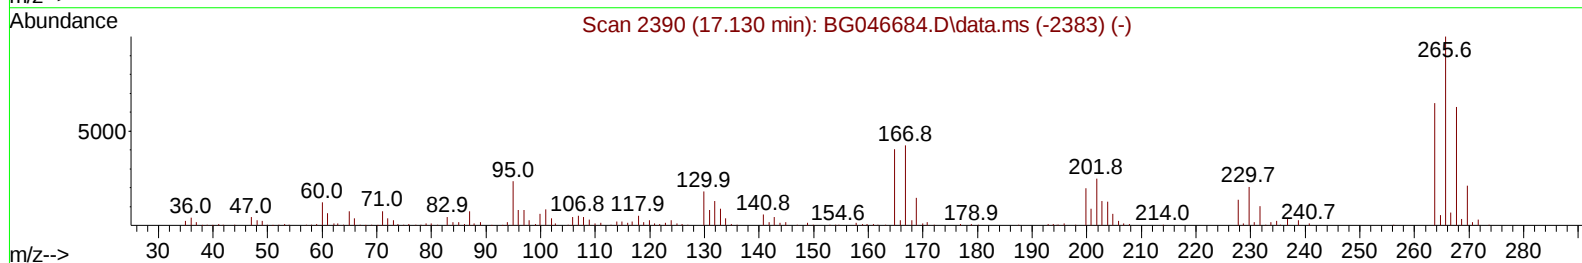
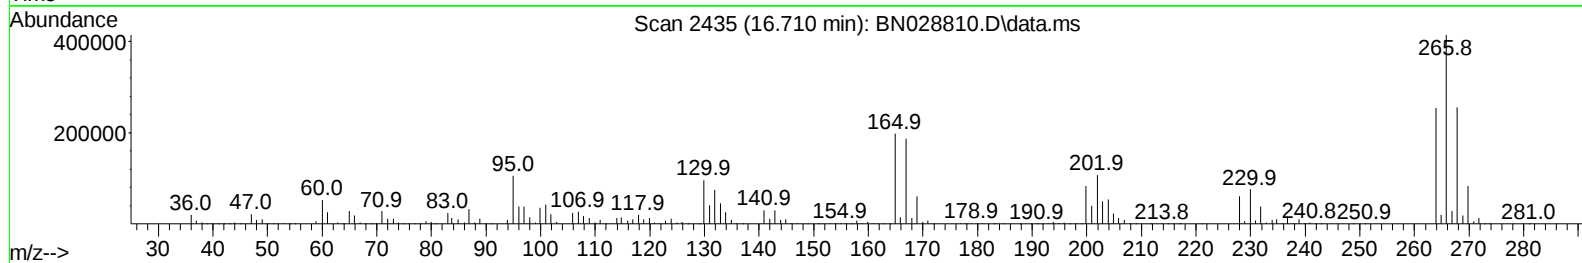


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112123\
Data File : BN028810.D
Acq On : 20 Nov 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 02:58:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 02:58:24 2023
Response via : Initial Calibration

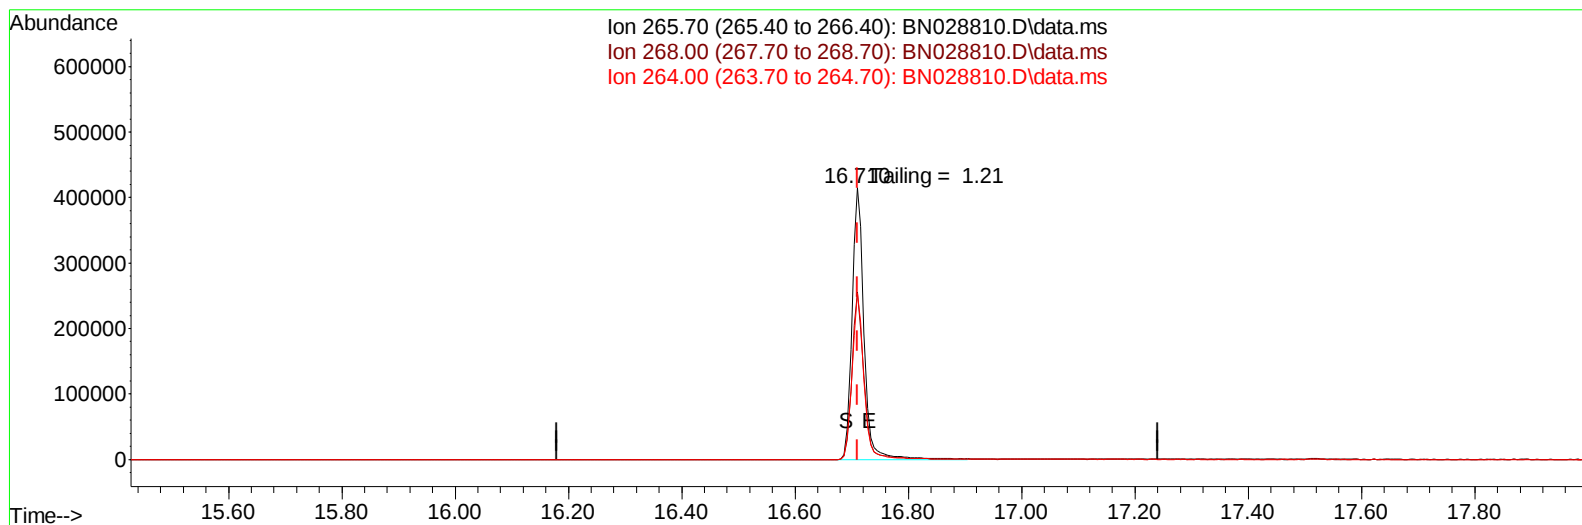




TIC: BN028810.D\data.ms

(70) Pentachlorophenol (C)**16.710min (0.000) 22337.90 ng****response 611980**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.55
264.00	61.60	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112123\
 Data File : BN028810.D
 Acq On : 20 Nov 2023 16:14
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 02:58:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 02:58:24 2023
 Response via : Initial Calibration

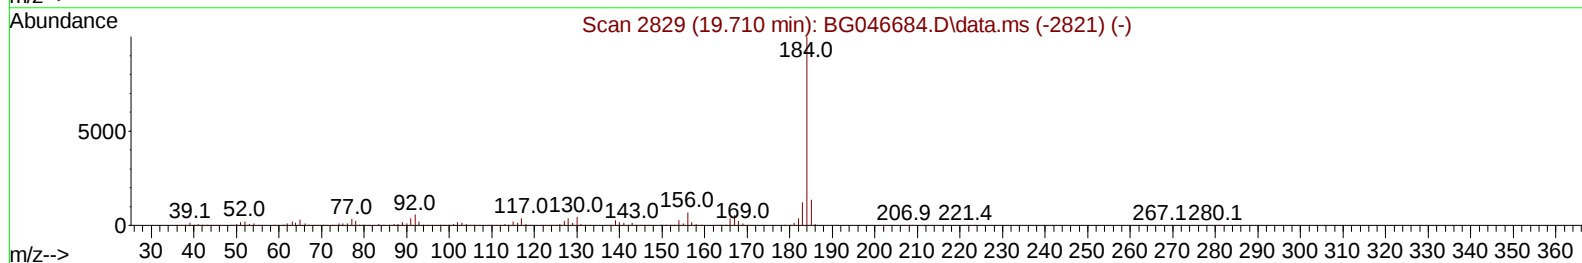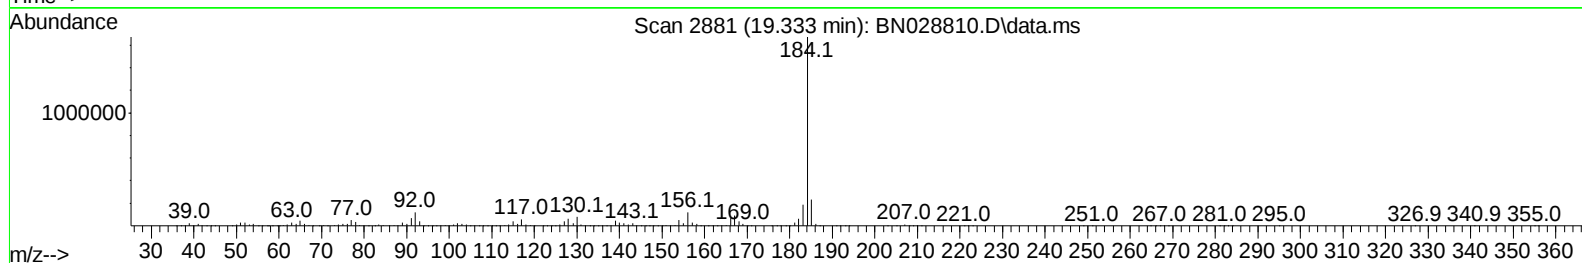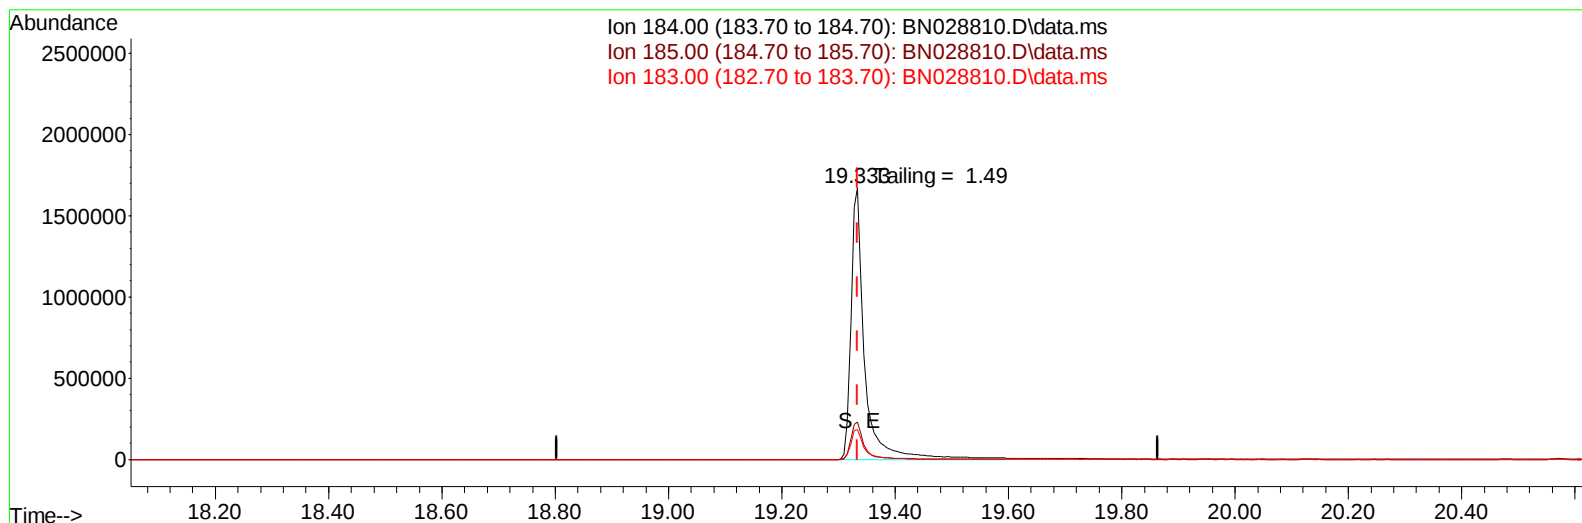

TIC: BN028810.D\data.ms

(77) Benzidine**19.333min (0.000) 1581704.22 ng****response 2827884**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.04
0.00	0.00	0.00