
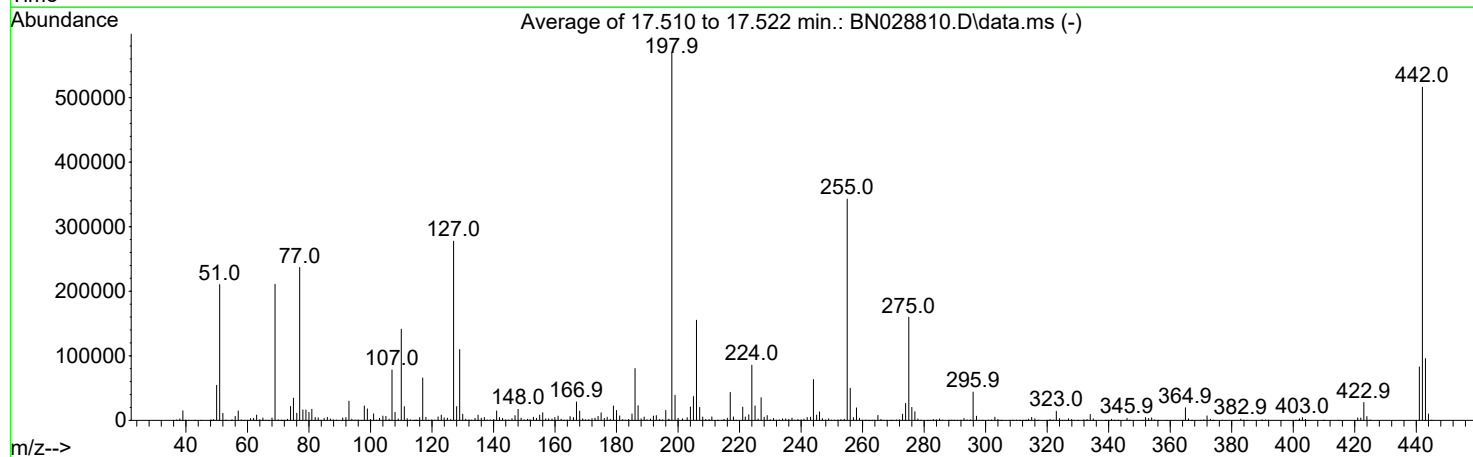


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112123\
Data File : BN028810.D
Acq On : 20 Nov 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 21 01:23:43 2023

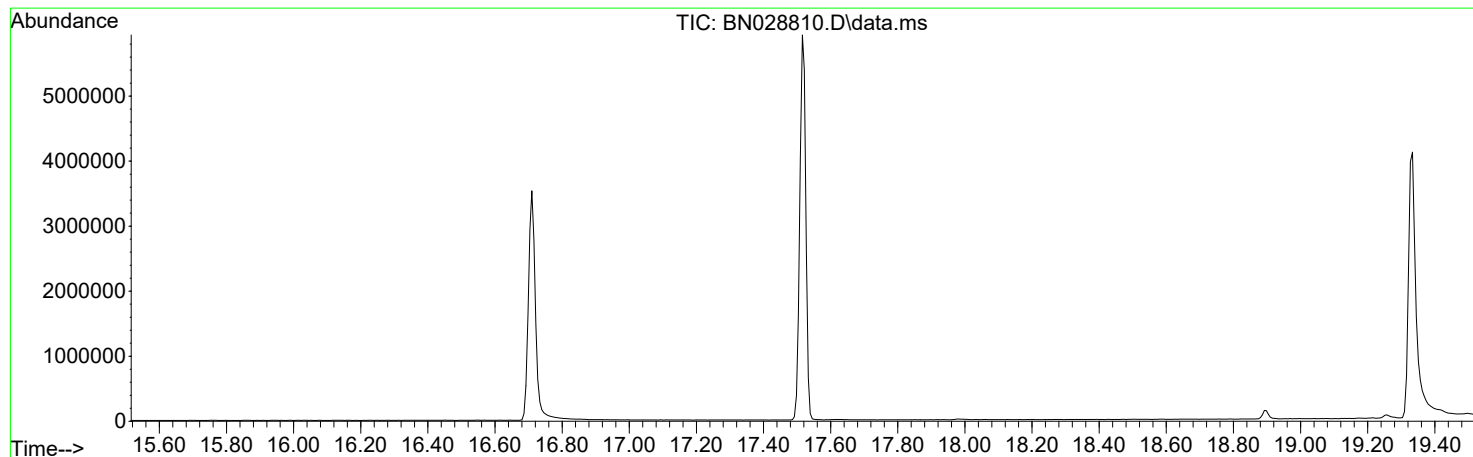

AutoFind: Scans 2571, 2572, 2573; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	210558	PASS
68	69	0.00	2	1.8	3715	PASS
69	198	0.00	100	37.0	210859	PASS
70	69	0.00	2	0.5	1148	PASS
127	198	10	80	48.7	277632	PASS
197	198	0.00	2	0.3	1989	PASS
198	198	100	100	100.0	569813	PASS
199	198	5	9	6.8	39029	PASS
275	198	10	60	28.0	159536	PASS
365	198	1	100	3.4	19645	PASS
441	198	0.01	100	14.5	82848	PASS
442	442	50	100	100.0	515904	PASS
443	442	15	24	18.6	95792	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/21/2023	BNA_N	<u>BN028810.D</u>
Compound Name	Response	Retention Time
DDT	1108045	20.574
DDD	321706	20.127
DDE	1948	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
323654	1431699	22.61

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112123\
 Data File : BN028810.D
 Acq On : 20 Nov 2023 16:14
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 21 02:58:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 02:58:24 2023
 Response via : Initial Calibration

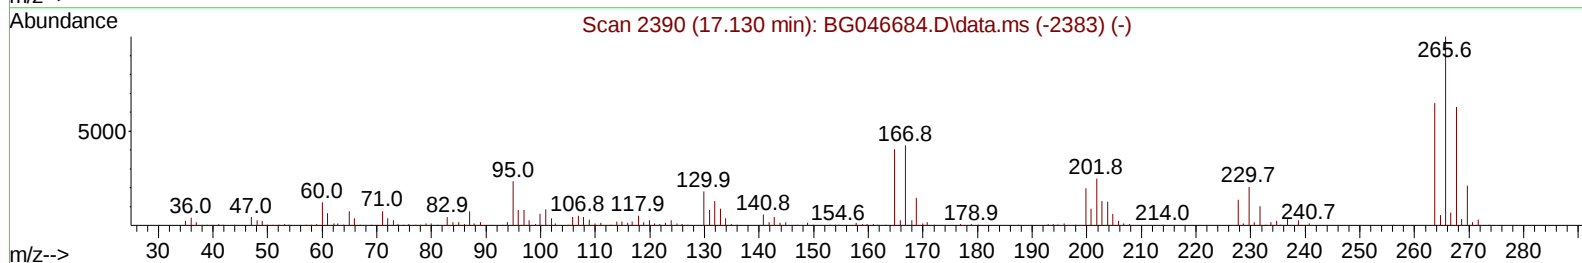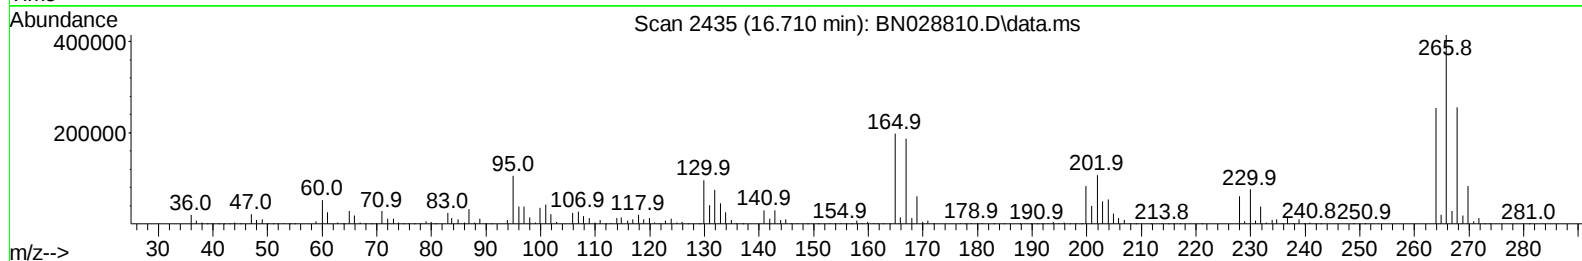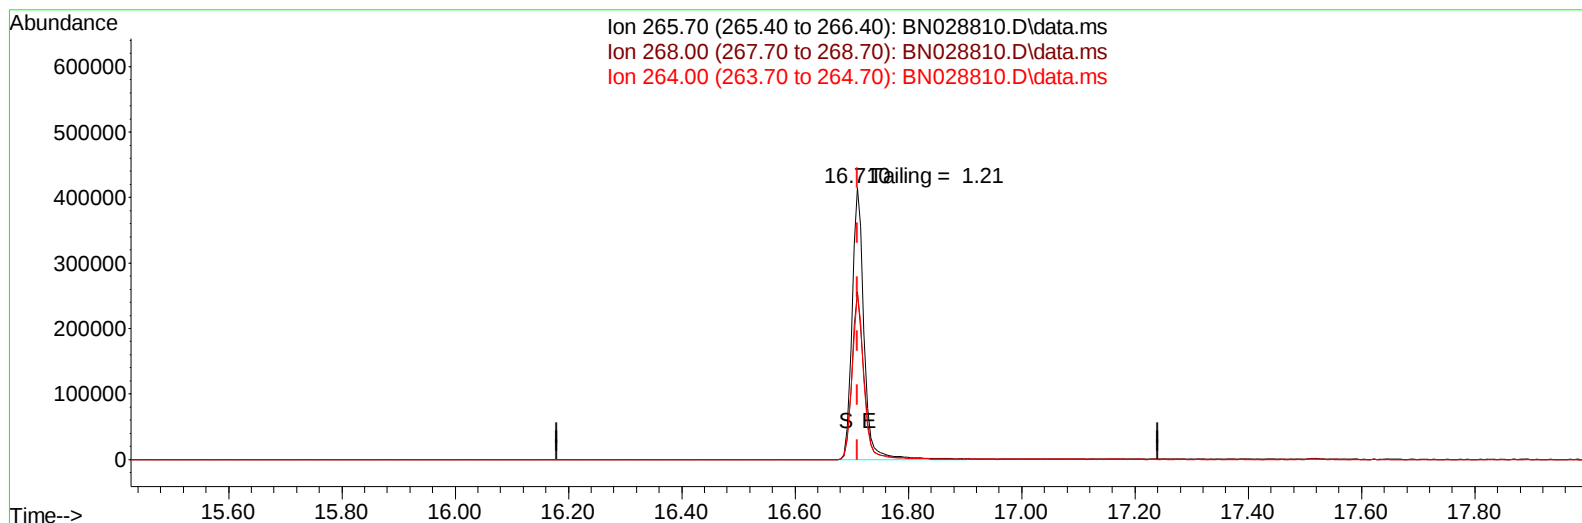

TIC: BN028810.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 22337.90 ng




response 611980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.55
264.00	61.60	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112123\
Data File : BN028810.D
Acq On : 20 Nov 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 21 02:58:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 02:58:24 2023
Response via : Initial Calibration

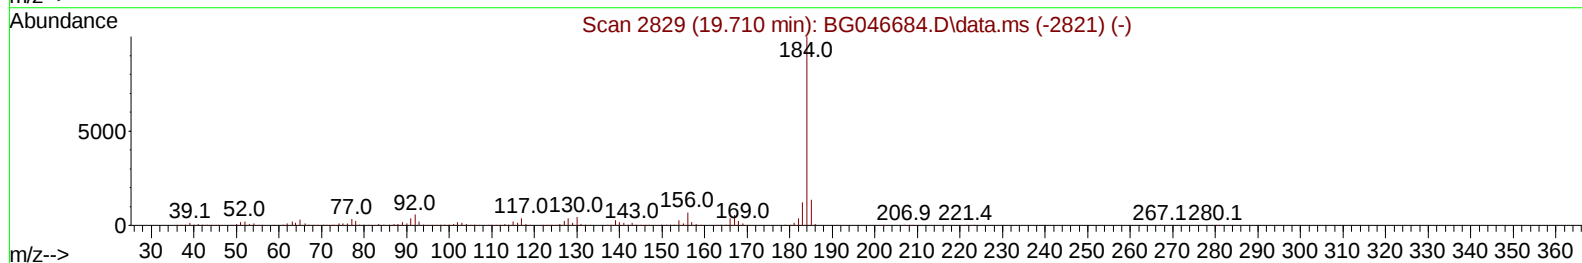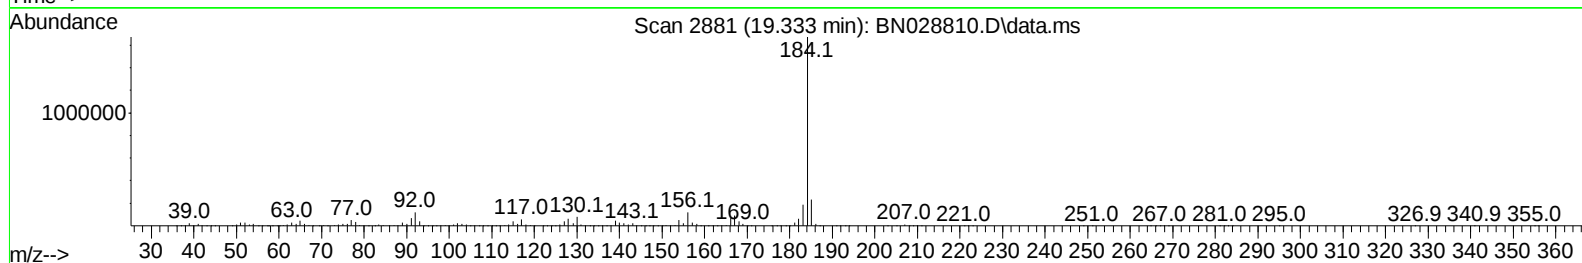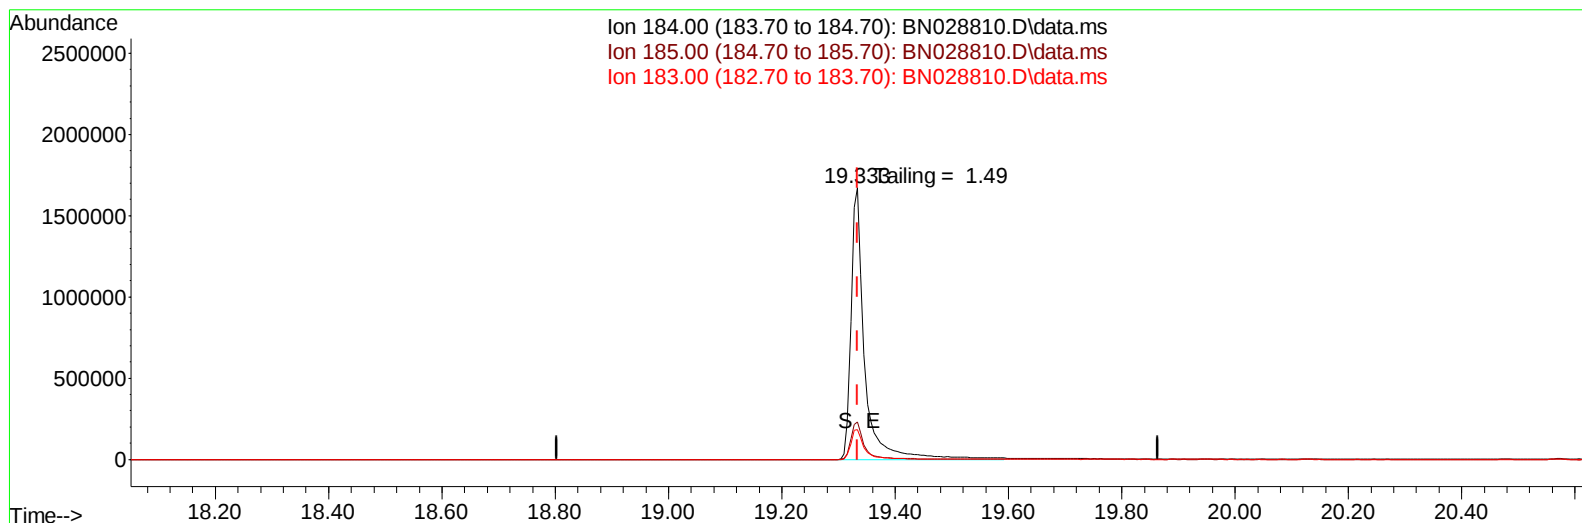

TIC: BN028810.D\data.ms

(77) Benzidine

19.333min (0.000) 1581704.22 ng

response 2827884

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.04
0.00	0.00	0.00