


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112219\
 Data File : BN008713.D
 Acq On : 22 Nov 2019 18:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 25 10:49:40 2019

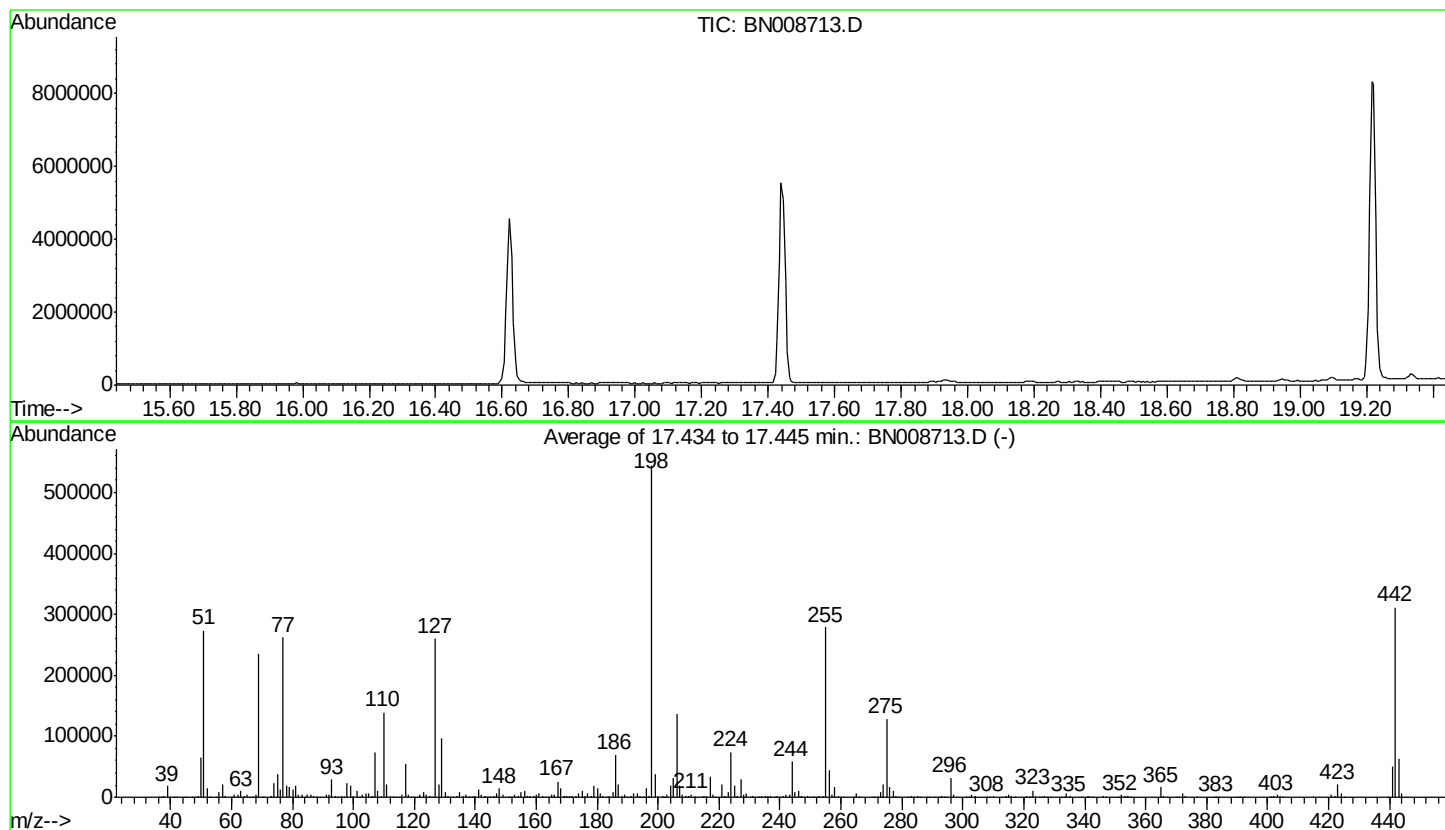

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	273889	PASS
68	69	0.00	2	1.9	4569	PASS
69	198	0.00	100	43.4	236050	PASS
70	69	0.00	2	0.4	830	PASS
127	198	10	80	47.8	260160	PASS
197	198	0.00	2	0.4	2131	PASS
198	198	100	100	100.0	544128	PASS
199	198	5	9	7.1	38770	PASS
275	198	10	60	23.6	128621	PASS
365	198	1	100	2.9	15978	PASS
441	198	0.01	100	9.2	50032	PASS
442	198	50	100	57.2	311317	PASS
443	442	15	24	20.4	63578	PASS