


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112319\
 Data File : BN008722.D
 Acq On : 23 Nov 2019 10:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN112219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 25 10:49:40 2019

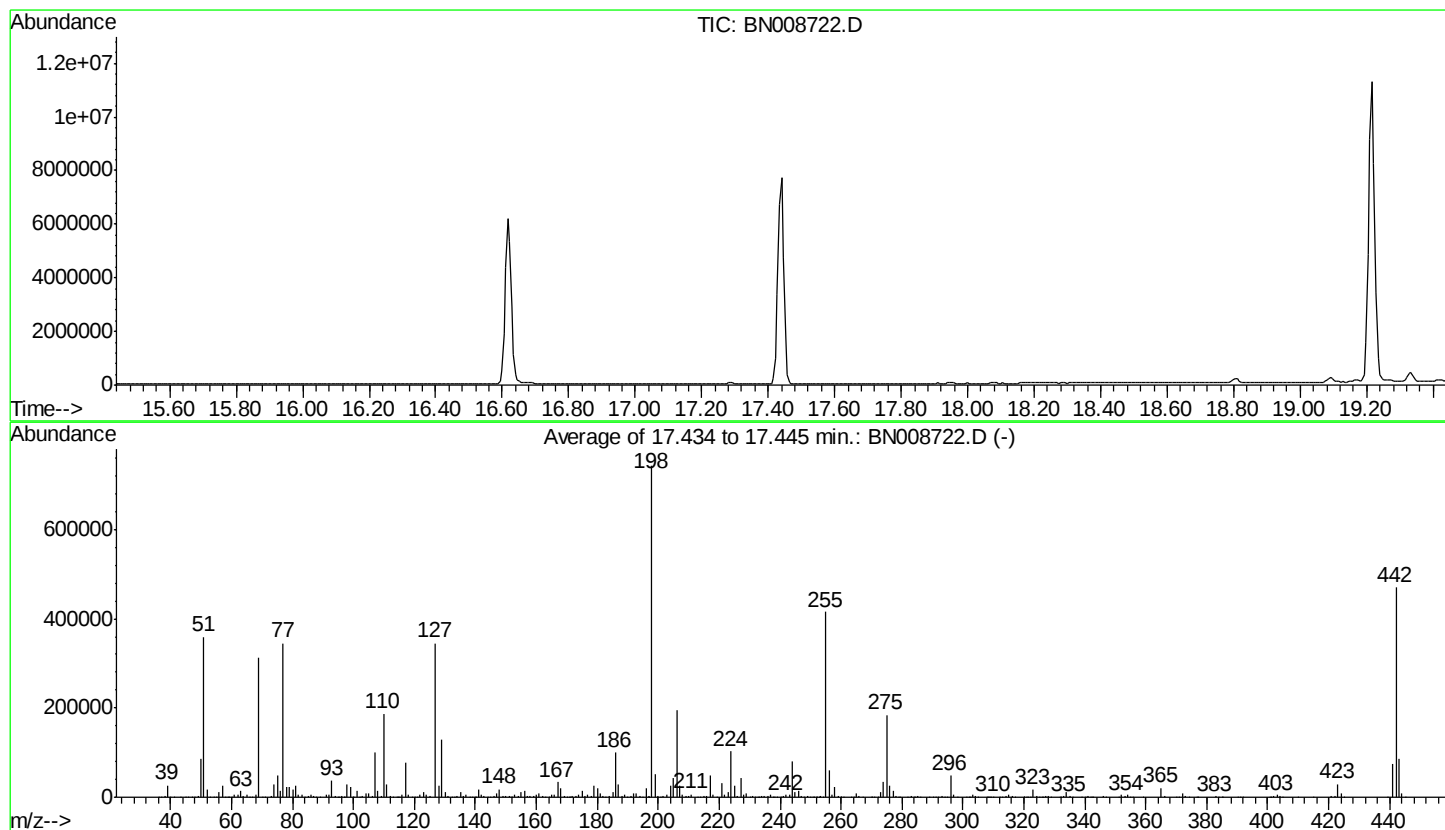

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	358704	PASS
68	69	0.00	2	2.0	6171	PASS
69	198	0.00	100	42.0	311829	PASS
70	69	0.00	2	0.5	1496	PASS
127	198	10	80	46.4	344746	PASS
197	198	0.00	2	0.2	1613	PASS
198	198	100	100	100.0	743189	PASS
199	198	5	9	6.9	50949	PASS
275	198	10	60	24.9	185130	PASS
365	198	1	100	2.8	20562	PASS
441	198	0.01	100	10.2	75762	PASS
442	198	50	100	63.1	469205	PASS
443	442	15	24	18.5	86984	PASS