
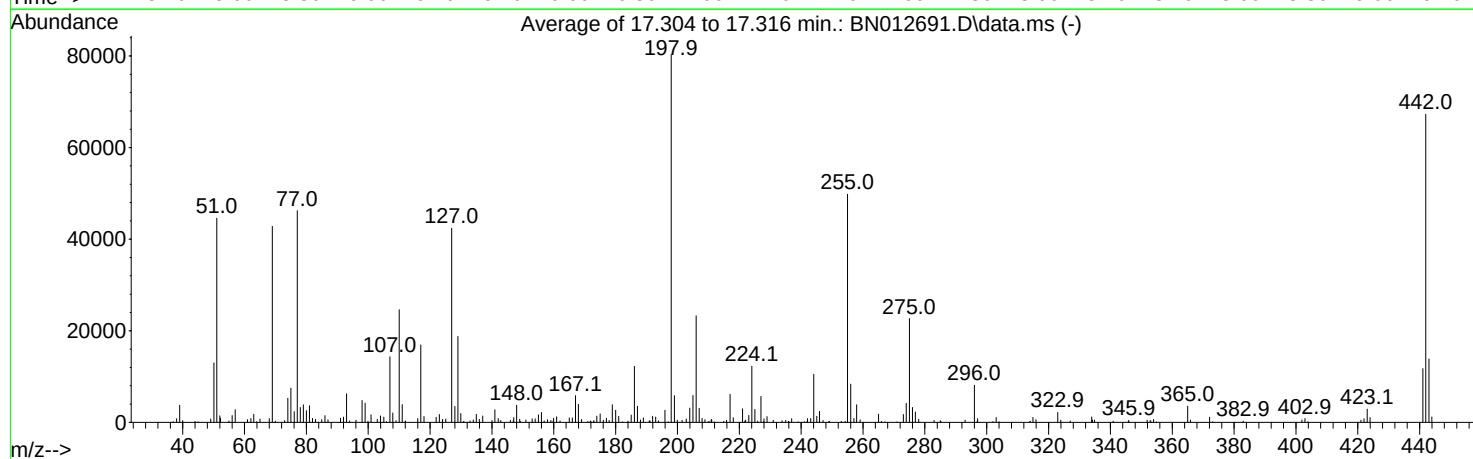


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112320\
Data File : BN012691.D
Acq On : 23 Nov 2020 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110420.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 23 12:44:50 2020

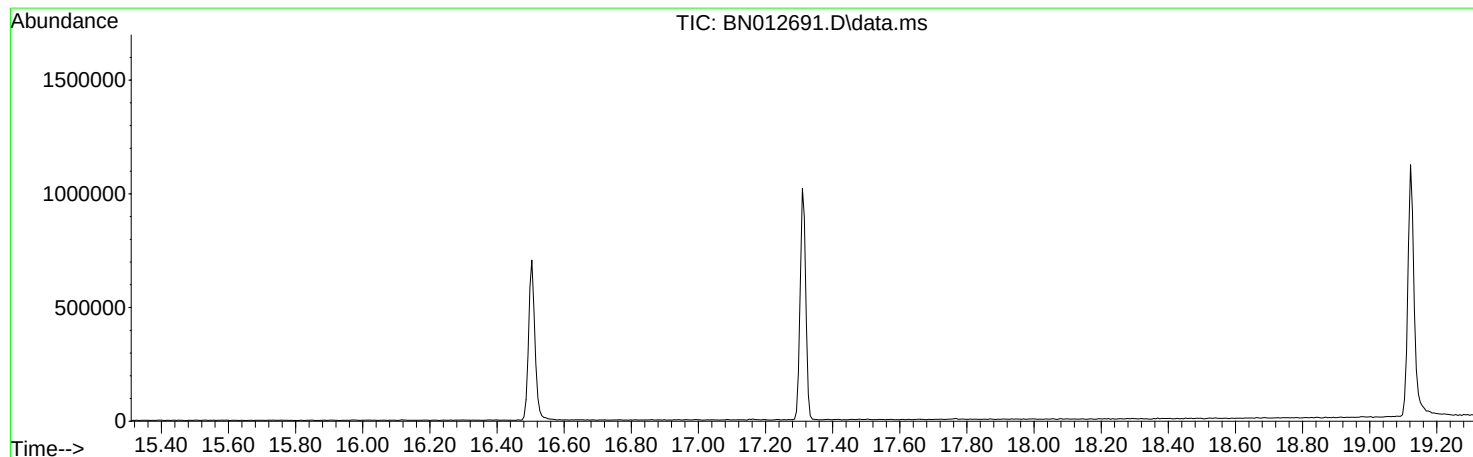

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.5	44597	PASS
68	69	0.00	2	1.9	814	PASS
69	198	0.00	100	53.3	42808	PASS
70	69	0.00	2	0.7	285	PASS
127	198	10	80	52.8	42389	PASS
197	198	0.00	2	0.2	159	PASS
198	198	100	100	100.0	80333	PASS
199	198	5	9	7.3	5832	PASS
275	198	10	60	28.2	22682	PASS
365	198	1	100	4.4	3523	PASS
441	198	0.01	100	14.6	11758	PASS
442	442	100	100	100.0	67267	PASS
443	442	15	24	20.6	13843	PASS