

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028853.D
 Acq On : 24 Nov 2023 11:47
 Operator : MA/JU
 Sample : 05268-22
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKB7

Quant Time: Nov 25 01:01:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.686	152	5048	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.440	136	19568	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.297	164	9385	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.060	188	16401	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.281	240	11334	0.400	ng/ul	# 0.01
23) Perylene-d12	23.546	264	15636	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	28454	5.100	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.096	152	2470	0.084	ng/ul	0.02
18) Fluoranthene-d10	19.094	212	12677	0.348	ng/ul	0.00
Target Compounds						Qvalue
16) Anthracene	17.182	178	2451	0.053	ng/ul#	66
20) Pyrene	19.452	202	2283	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.388	252	4456	0.080	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028853.D
Acq On : 24 Nov 2023 11:47
Operator : MA/JU
Sample : 05268-22
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCKB7

Quant Time: Nov 25 01:01:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration




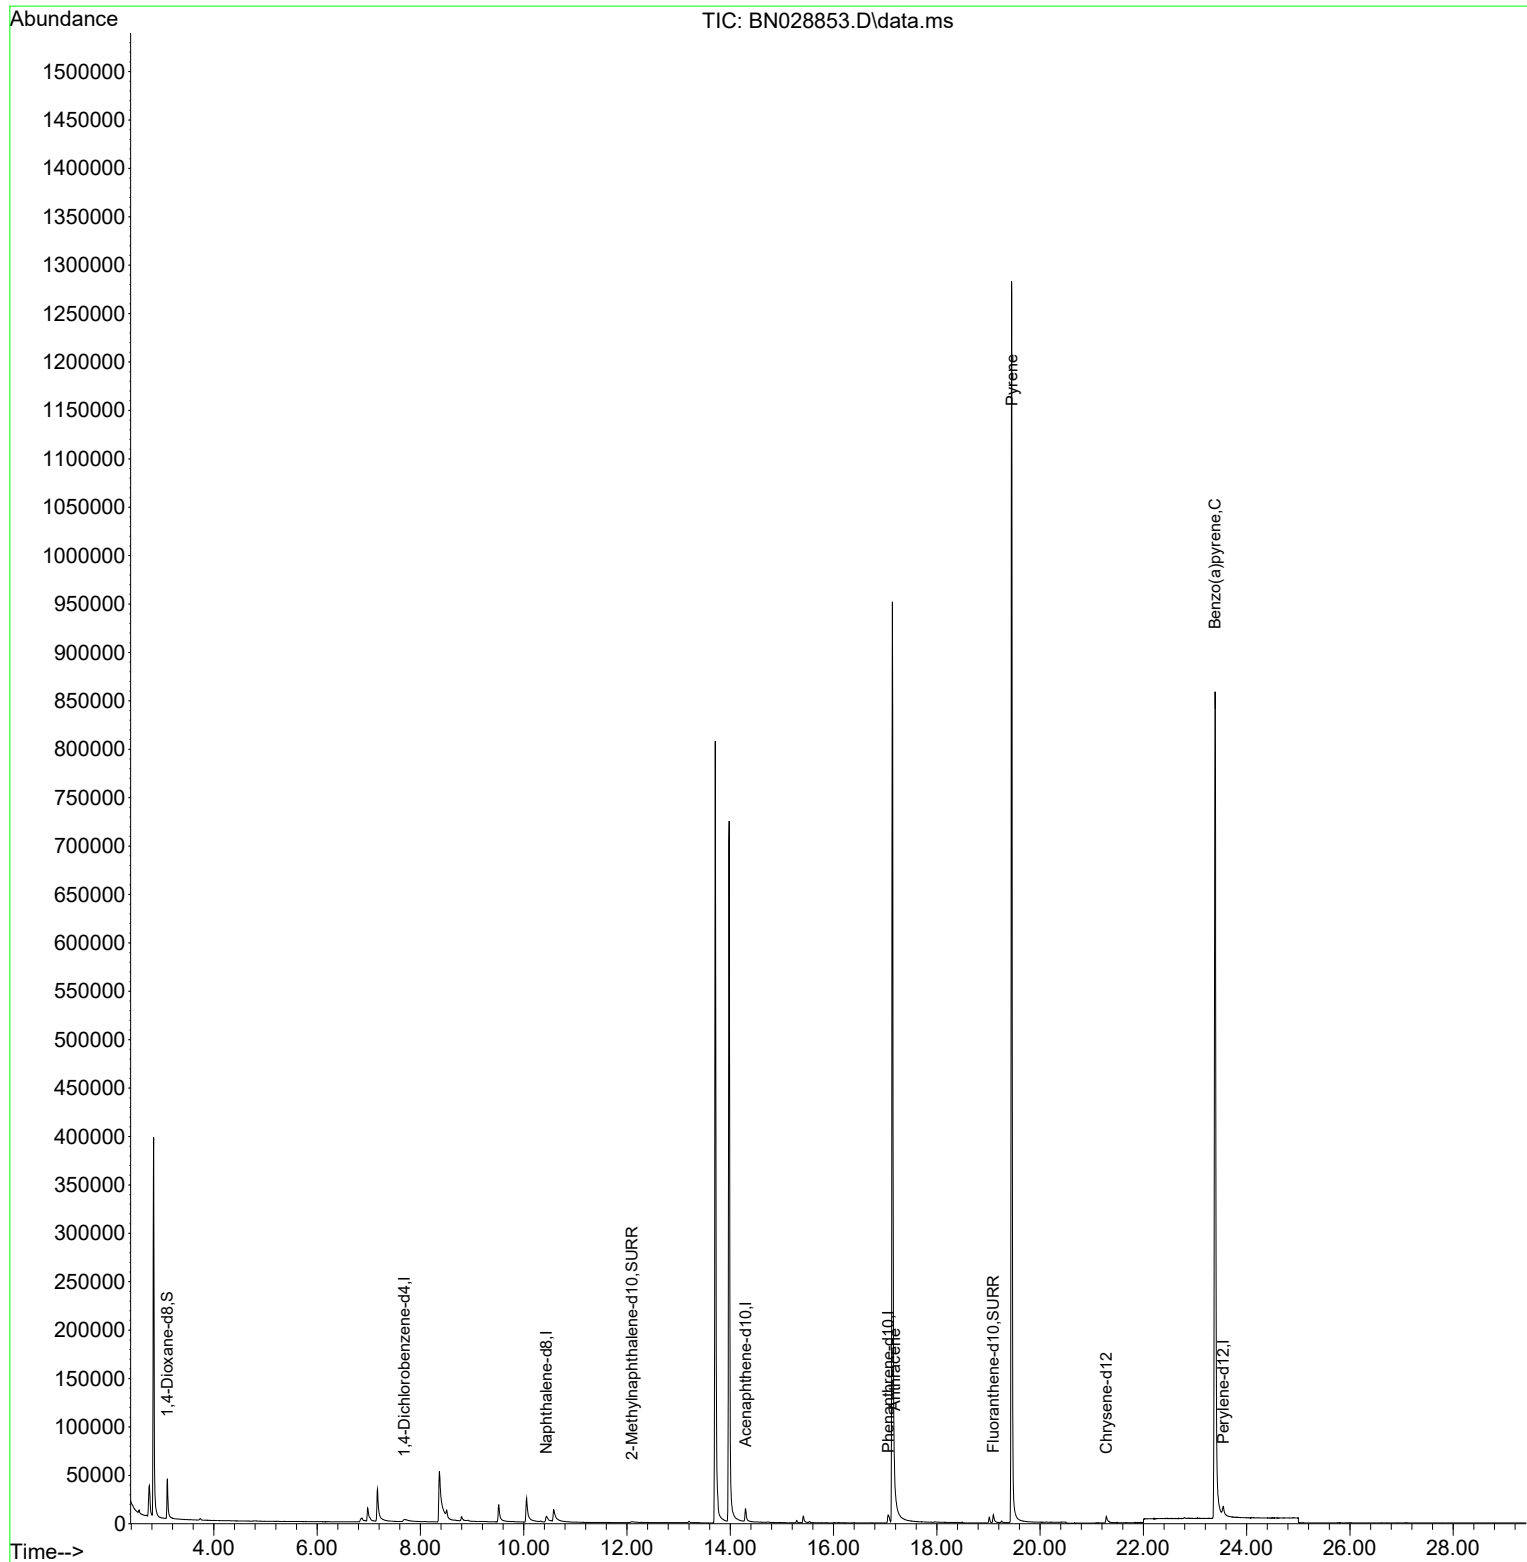


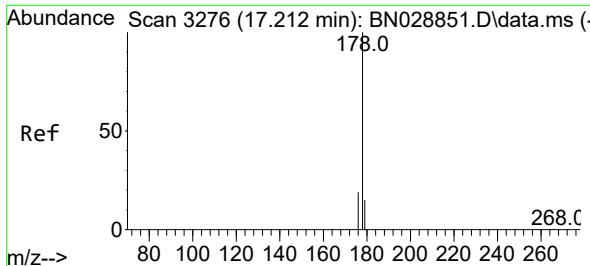

#16
 Anthracene
 Concen: 0.053 ng/ul
 RT: 17.182 min Scan# 31
 Delta R.T. -0.022 min
 Lab File: BN028853.D
 Acq: 24 Nov 2023 11:47




Instrument :
 BNA_N
 ClientSampleId :
 DCKB7


Tgt Ion:178 Resp: 2451
 Ion Ratio Lower Upper
 178 100
 179 33.0 12.6 18.8#
 176 31.6 14.9 22.3#

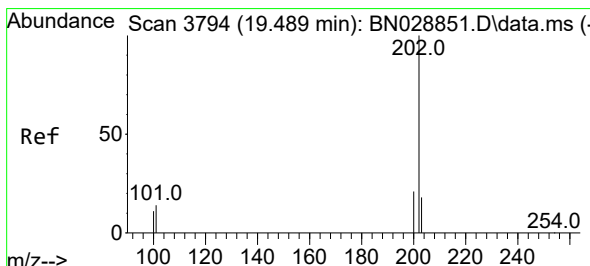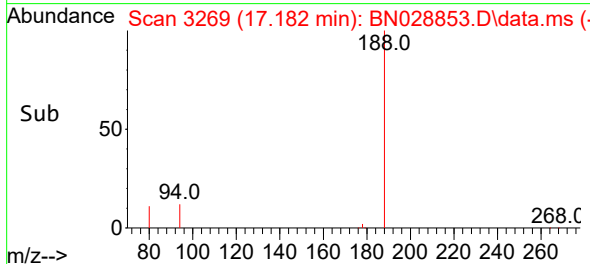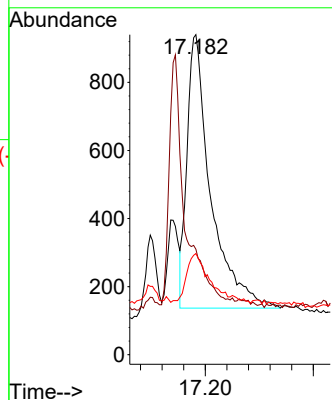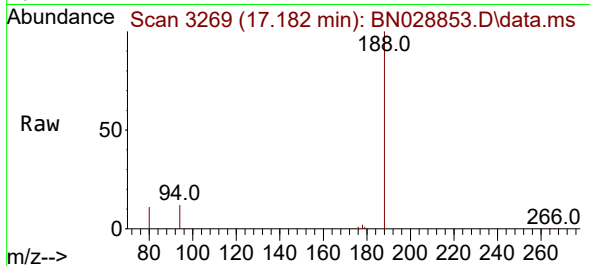

#20
 Pyrene
 Concen: 0.046 ng/ul
 RT: 19.452 min Scan# 3786
 Delta R.T. -0.033 min
 Lab File: BN028853.D
 Acq: 24 Nov 2023 11:47


Tgt Ion:202 Resp: 2283
 Ion Ratio Lower Upper
 202 100
 101 146.0 10.3 15.5#
 100 986.9 8.2 12.2#

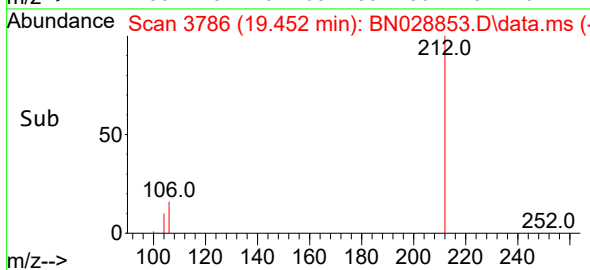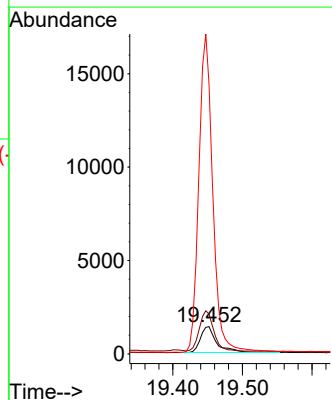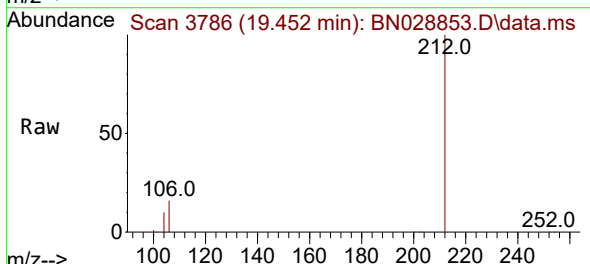

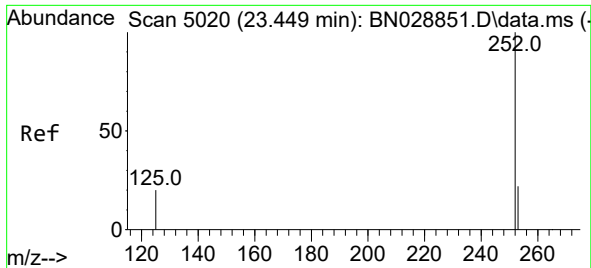

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.388 min Scan# 4999
Delta R.T. -0.056 min
Lab File: BN028853.D
Acq: 24 Nov 2023 11:47

Instrument :
BNA_N
ClientSampleId :
DCKB7

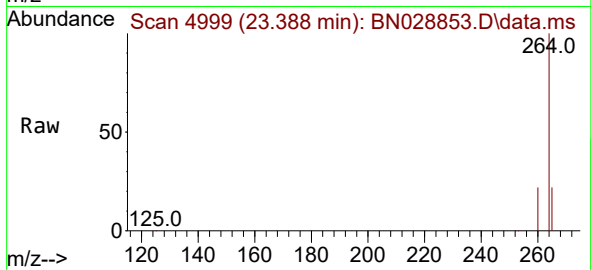

Tgt Ion:252 Resp: 4456
Ion Ratio Lower Upper
252 100
253 53.3 19.0 28.6#
125 48.3 13.2 19.8#

