

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028856.D
 Acq On : 24 Nov 2023 13:34
 Operator : MA/JU
 Sample : 05268-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKE8

Quant Time: Nov 25 01:02:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.706	152	5018	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.439	136	19237	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.292	164	10445	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.051	188	18258	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.271	240	12101	0.400	ng/ul	# 0.00
23) Perylene-d12	23.539	264	14867	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.103	96	27400	4.941	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.067	152	4596	0.159	ng/ul	0.00
18) Fluoranthene-d10	19.088	212	12728	0.327	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.477	128	349239	6.478	ng/ul	99
7) 2-Methylnaphthalene	12.133	142	9268	0.261	ng/ul	100
8) 1-Methylnaphthalene	12.331	142	11509	0.319	ng/ul	100
10) Acenaphthylene	14.005	152	30859	0.592	ng/ul	98
11) Acenaphthene	14.352	153	124791	3.253	ng/ul	99
12) Fluorene	15.347	166	213650	4.787	ng/ul	99
14) Pentachlorophenol	16.701	266	4931	1.125	ng/ul	99
15) Phenanthrene	17.089	178	152158	2.712	ng/ul	100
16) Anthracene	17.178	178	15534	0.302	ng/ul#	93
19) Fluoranthene	19.121	202	5734	0.111	ng/ul#	89
20) Pyrene	19.479	202	3257	0.061	ng/ul#	57
26) Benzo(a)pyrene	23.384	252	4219	0.080	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028856.D
Acq On : 24 Nov 2023 13:34
Operator : MA/JU
Sample : 05268-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCKE8


Quant Time: Nov 25 01:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

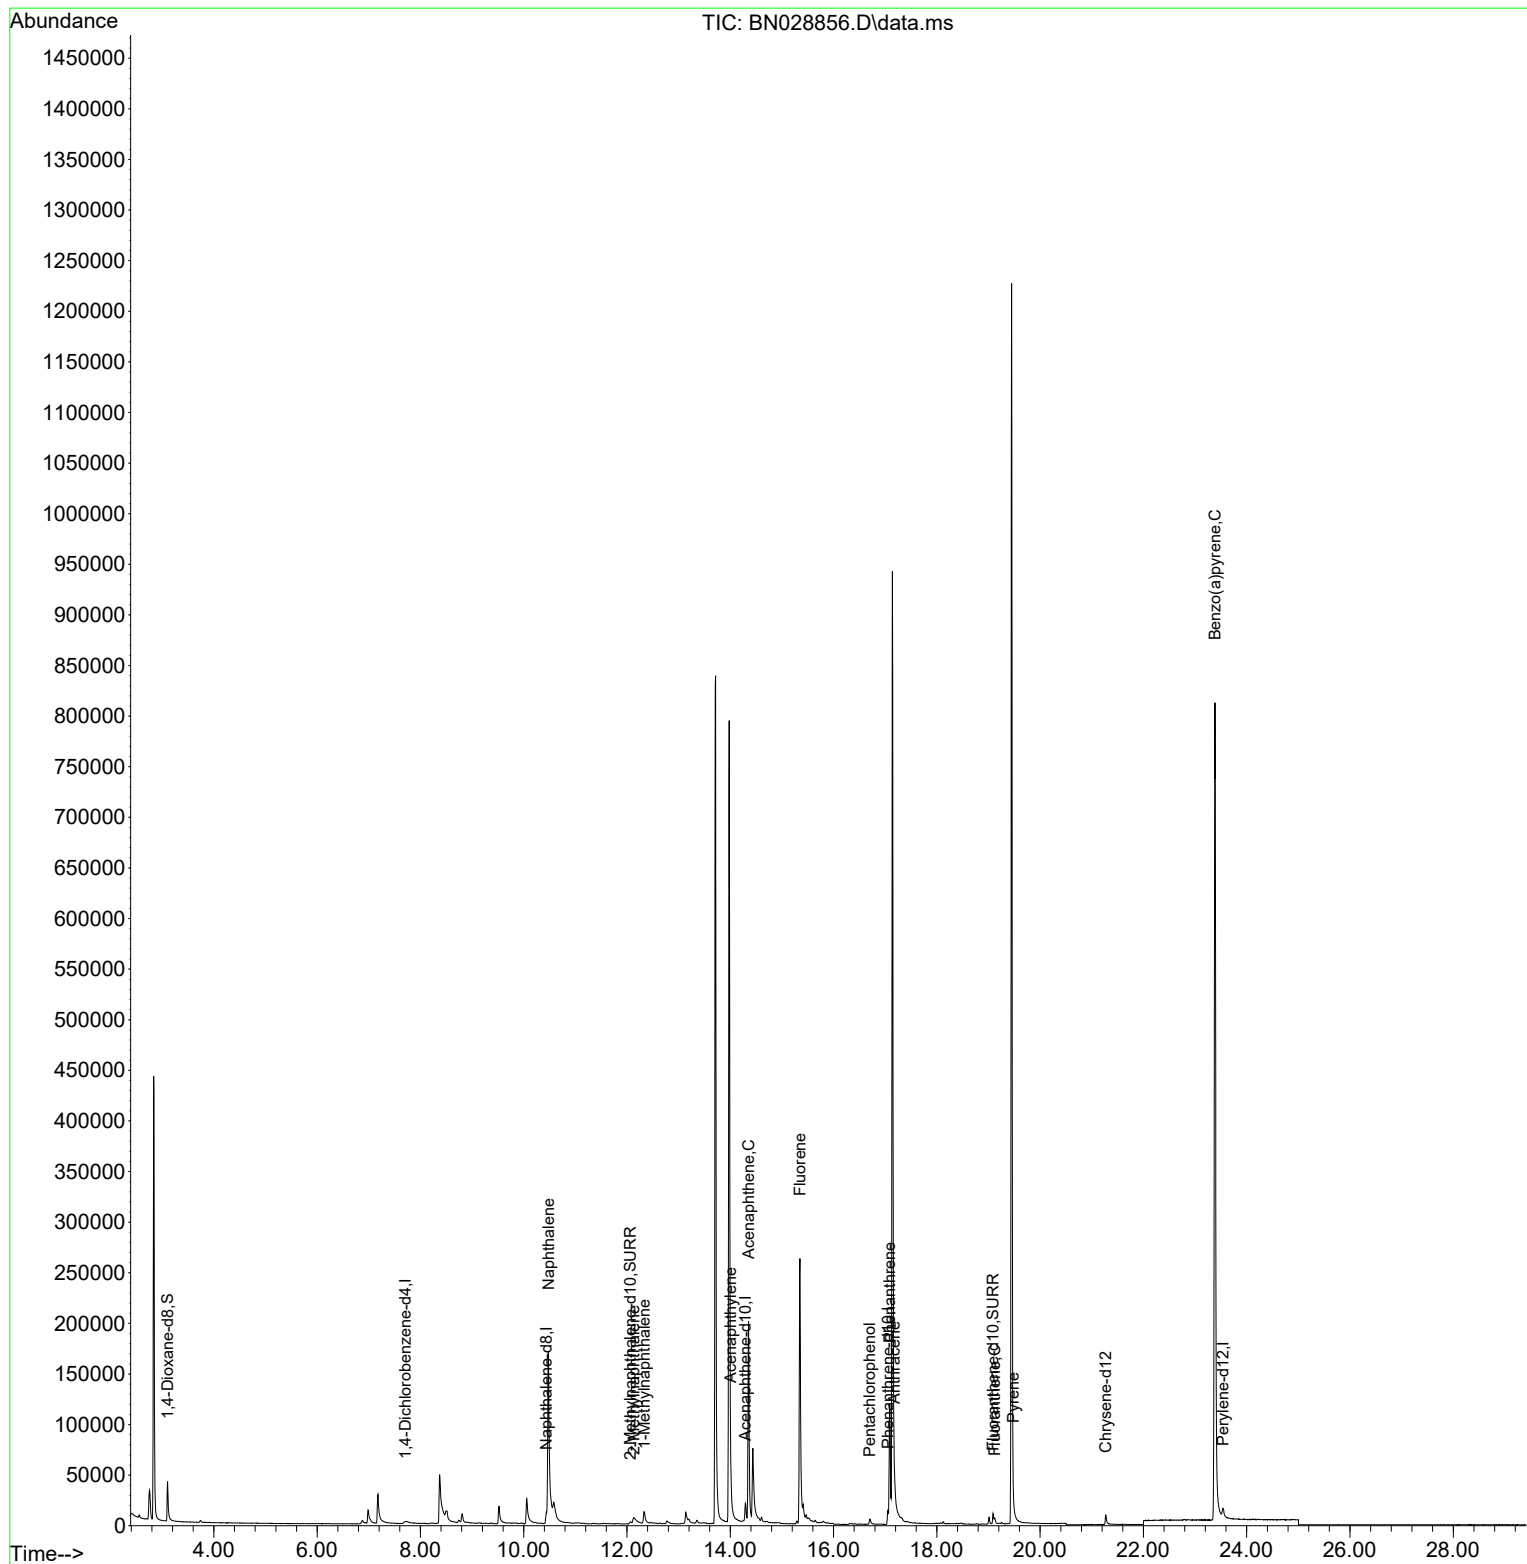






#5
Naphthalene
Concen: 6.478 ng/ul
RT: 10.477 min Scan# 1896
Delta R.T. -0.029 min
Lab File: BN028856.D
Acq: 24 Nov 2023 13:34

Instrument :
BNA_N
ClientSampleId :
DCKE8







Tgt Ion:128 Resp: 349239
Ion Ratio Lower Upper
128 100
129 11.2 9.2 13.8
127 12.8 10.7 16.1

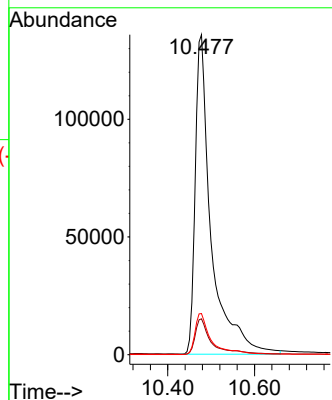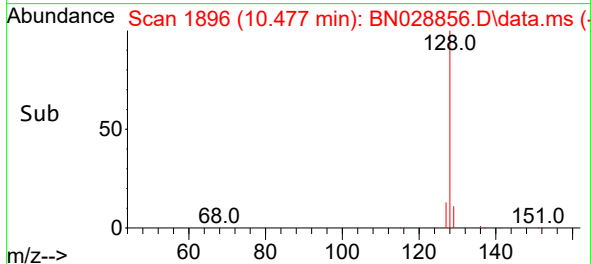

#7
2-Methylnaphthalene
Concen: 0.261 ng/ul
RT: 12.133 min Scan# 2197
Delta R.T. -0.007 min
Lab File: BN028856.D
Acq: 24 Nov 2023 13:34

Tgt Ion:142 Resp: 9268
Ion Ratio Lower Upper
142 100
141 88.8 70.8 106.2

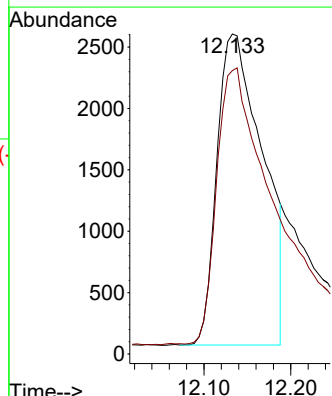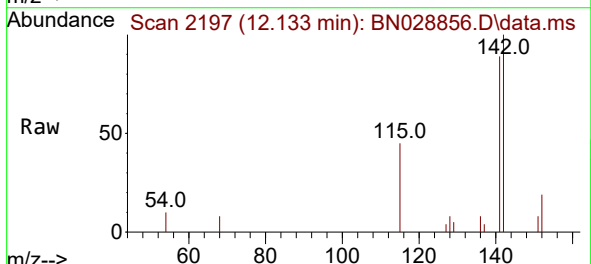

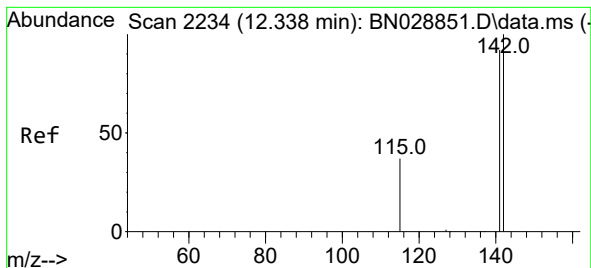

#8

1-Methylnaphthalene

Concen: 0.319 ng/ul

RT: 12.331 min Scan# 21

Delta R.T. -0.007 min

Lab File: BN028856.D

Acq: 24 Nov 2023 13:34

Instrument :

BNA_N

ClientSampleId :





DCKE8

Tgt Ion:142 Resp: 11509

Ion Ratio Lower Upper

142 100

141 92.2 74.1 111.1

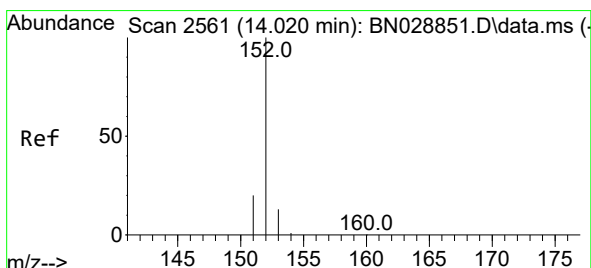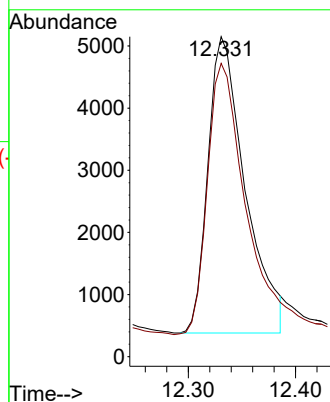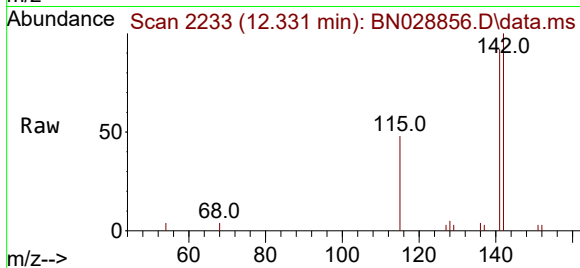

#10

Acenaphthylene

Concen: 0.592 ng/ul

RT: 14.005 min Scan# 2558

Delta R.T. -0.020 min

Lab File: BN028856.D

Acq: 24 Nov 2023 13:34




Tgt Ion:152 Resp: 30859


Ion Ratio Lower Upper

152 100

151 20.4 16.1 24.1

153 14.6 10.6 15.8


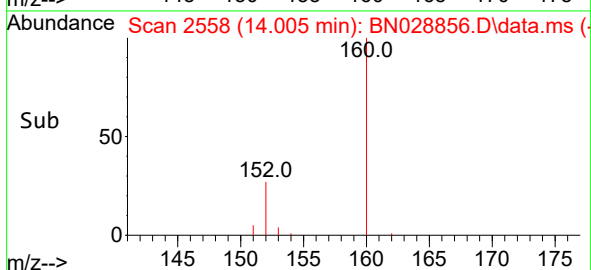
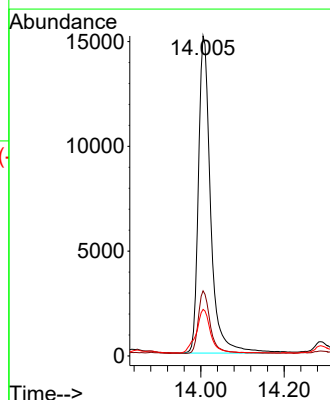
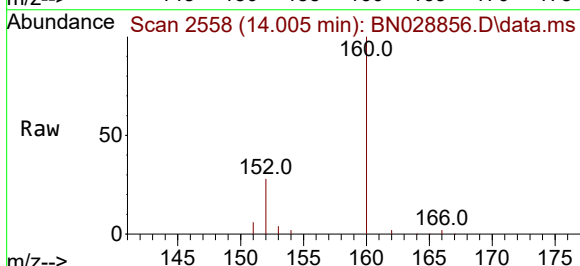




#11
Acenaphthene
Concen: 3.253 ng/ul
RT: 14.352 min Scan# 2084
Delta R.T. -0.011 min
Lab File: BN028856.D
Acq: 24 Nov 2023 13:34




Instrument :
BNA_N
ClientSampleId :
DCKE8


Tgt Ion:153 Resp: 124791
Ion Ratio Lower Upper
153 100
152 48.0 39.6 59.4
154 88.2 71.0 106.6

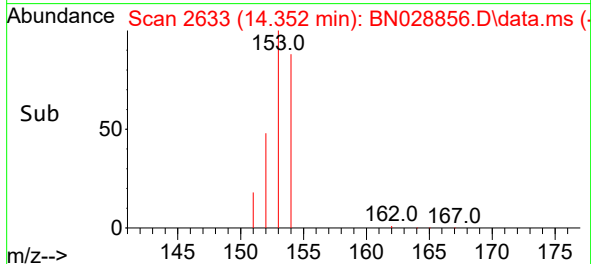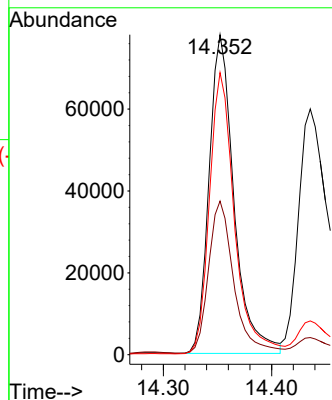

#12
Fluorene
Concen: 4.787 ng/ul
RT: 15.347 min Scan# 2848
Delta R.T. -0.020 min
Lab File: BN028856.D
Acq: 24 Nov 2023 13:34

Tgt Ion:166 Resp: 213650
Ion Ratio Lower Upper
166 100
165 97.6 78.6 118.0
167 13.8 11.0 16.6


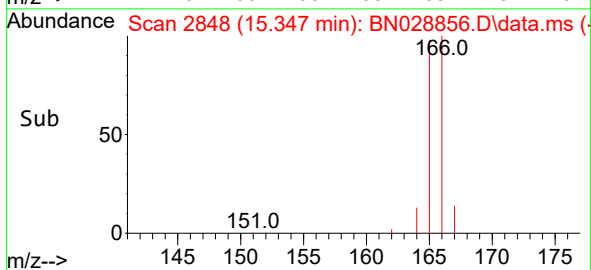
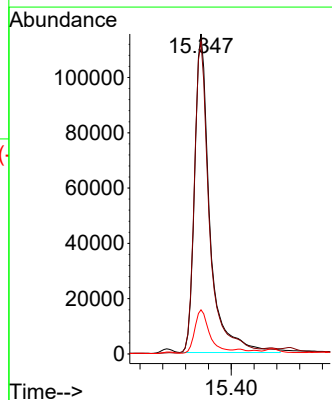
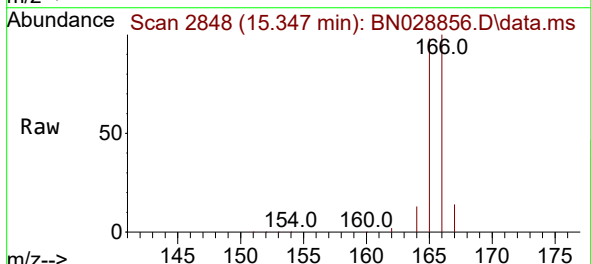




#14
 Pentachlorophenol
 Concen: 1.125 ng/ul
 RT: 16.701 min Scan# 3161
 Delta R.T. -0.023 min
 Lab File: BN028856.D
 Acq: 24 Nov 2023 13:34




Instrument :
 BNA_N
 ClientSampleId :
 DCKE8


Tgt Ion:266 Resp: 4931
 Ion Ratio Lower Upper
 266 100
 264 63.3 50.1 75.1
 268 64.2 50.6 75.8

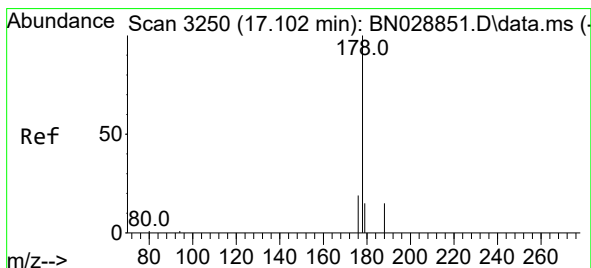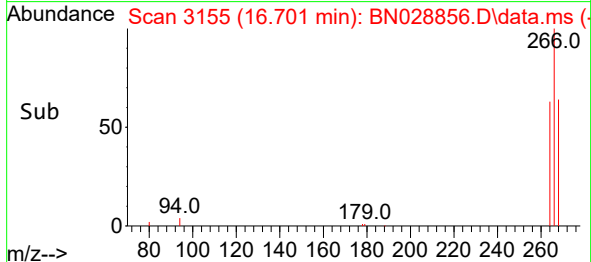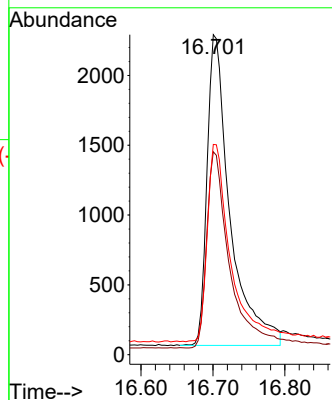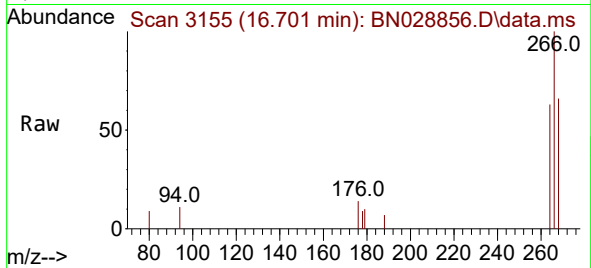

#15
 Phenanthrene
 Concen: 2.712 ng/ul
 RT: 17.089 min Scan# 3247
 Delta R.T. -0.014 min
 Lab File: BN028856.D
 Acq: 24 Nov 2023 13:34

Tgt Ion:178 Resp: 152158
 Ion Ratio Lower Upper
 178 100
 179 15.5 12.4 18.6
 176 19.2 15.4 23.2


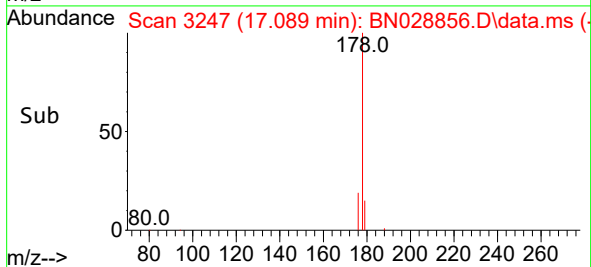
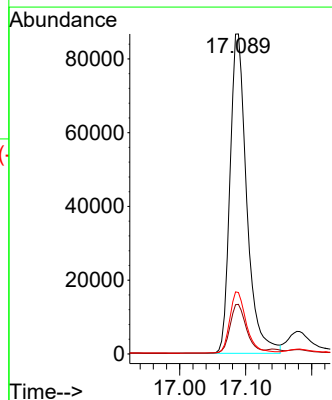
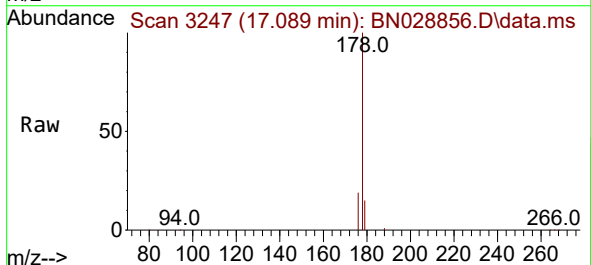


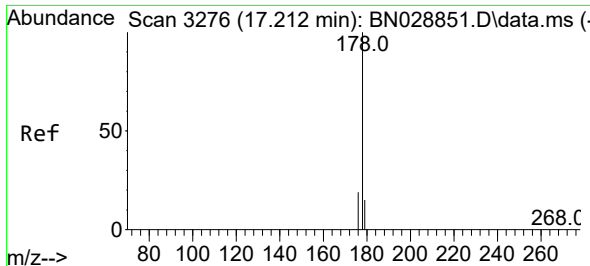

#16
 Anthracene
 Concen: 0.302 ng/ul
 RT: 17.178 min Scan# 31
 Delta R.T. -0.027 min
 Lab File: BN028856.D
 Acq: 24 Nov 2023 13:34




Instrument :
 BNA_N
 ClientSampleId :
 DCKE8


Tgt Ion:178 Resp: 15534
 Ion Ratio Lower Upper
 178 100
 179 19.1 12.6 18.8#
 176 21.5 14.9 22.3

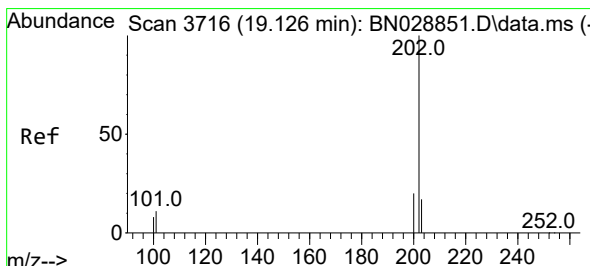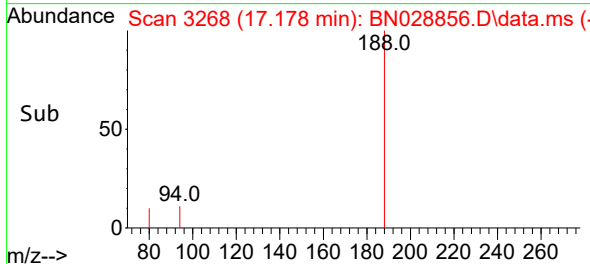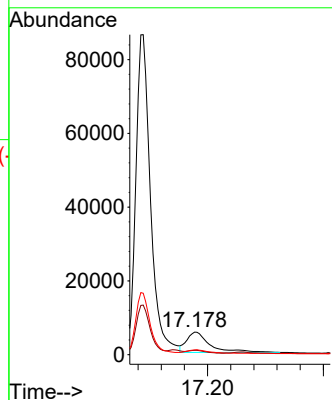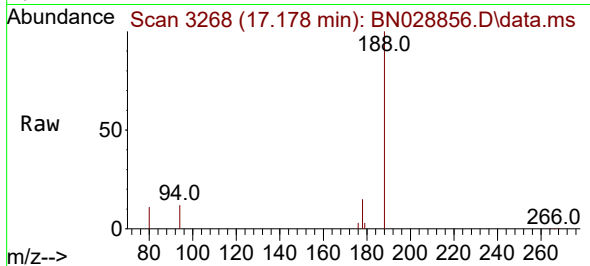

#19
 Fluoranthene
 Concen: 0.111 ng/ul
 RT: 19.121 min Scan# 3715
 Delta R.T. -0.002 min
 Lab File: BN028856.D
 Acq: 24 Nov 2023 13:34

Tgt Ion:202 Resp: 5734
 Ion Ratio Lower Upper
 202 100
 101 15.8 9.5 14.3#
 100 13.0 7.2 10.8#


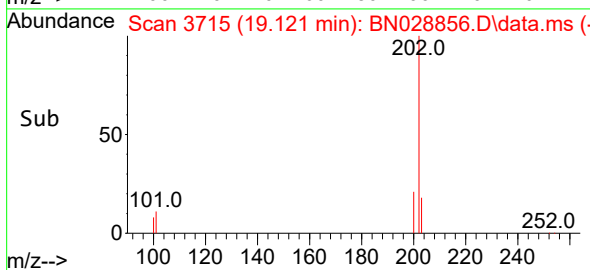
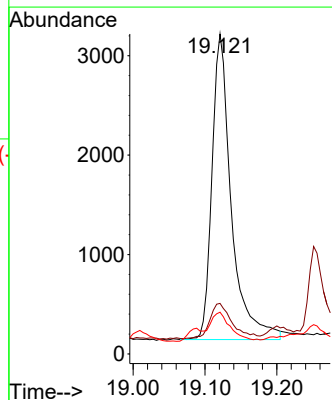
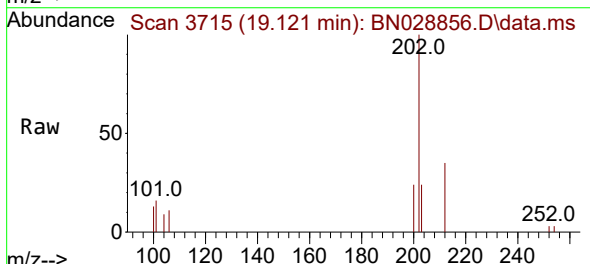




#20
Pyrene
Concen: 0.061 ng/ul
RT: 19.479 min Scan# 31
Delta R.T. -0.006 min
Lab File: BN028856.D
Acq: 24 Nov 2023 13:34

Instrument :
BNA_N
ClientSampleId :
DCKE8

Tgt Ion:202 Resp: 3257
Ion Ratio Lower Upper
202 100
101 23.7 10.3 15.5#
100 34.0 8.2 12.2#

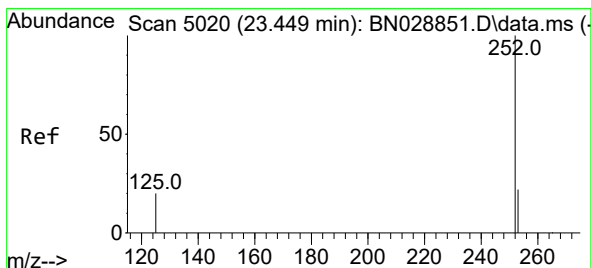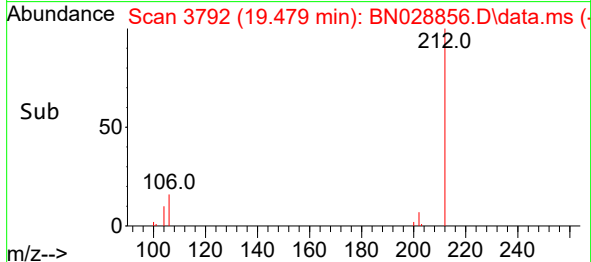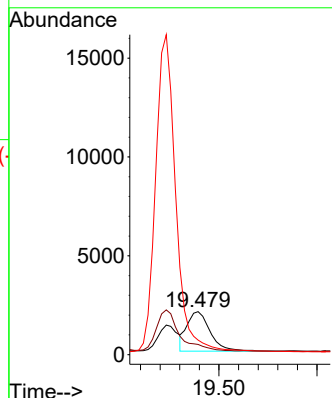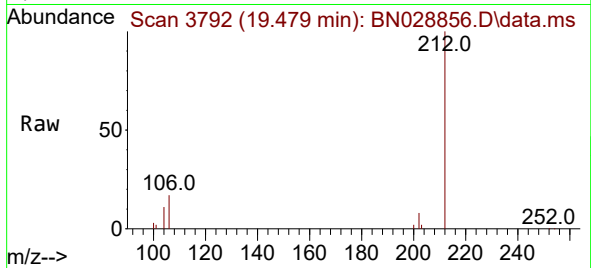

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.384 min Scan# 4998
Delta R.T. -0.060 min
Lab File: BN028856.D
Acq: 24 Nov 2023 13:34

Tgt Ion:252 Resp: 4219
Ion Ratio Lower Upper
252 100
253 54.6 19.0 28.6#
125 49.8 13.2 19.8#

