

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
 Data File : BN028857.D
 Acq On : 24 Nov 2023 14:34
 Operator : MA/JU
 Sample : 05268-21
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKB6

Quant Time: Nov 25 01:02:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.690	152	5335	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.440	136	21568	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.293	164	11803	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.056	188	21609	0.400	ng/ul	0.00
17) Chrysene-d12	21.281	240	11836	0.400	ng/ul	# 0.01
23) Perylene-d12	23.549	264	14042	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	32364	5.489	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.090	152	3704	0.114	ng/ul	0.02
18) Fluoranthene-d10	19.094	212	18940	0.497	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	16.710	266	2876	0.555	ng/ul	100
20) Pyrene	19.452	202	2924	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.388	252	4795	0.096	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112423\
Data File : BN028857.D
Acq On : 24 Nov 2023 14:34
Operator : MA/JU
Sample : 05268-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCKB6

Quant Time: Nov 25 01:02:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration




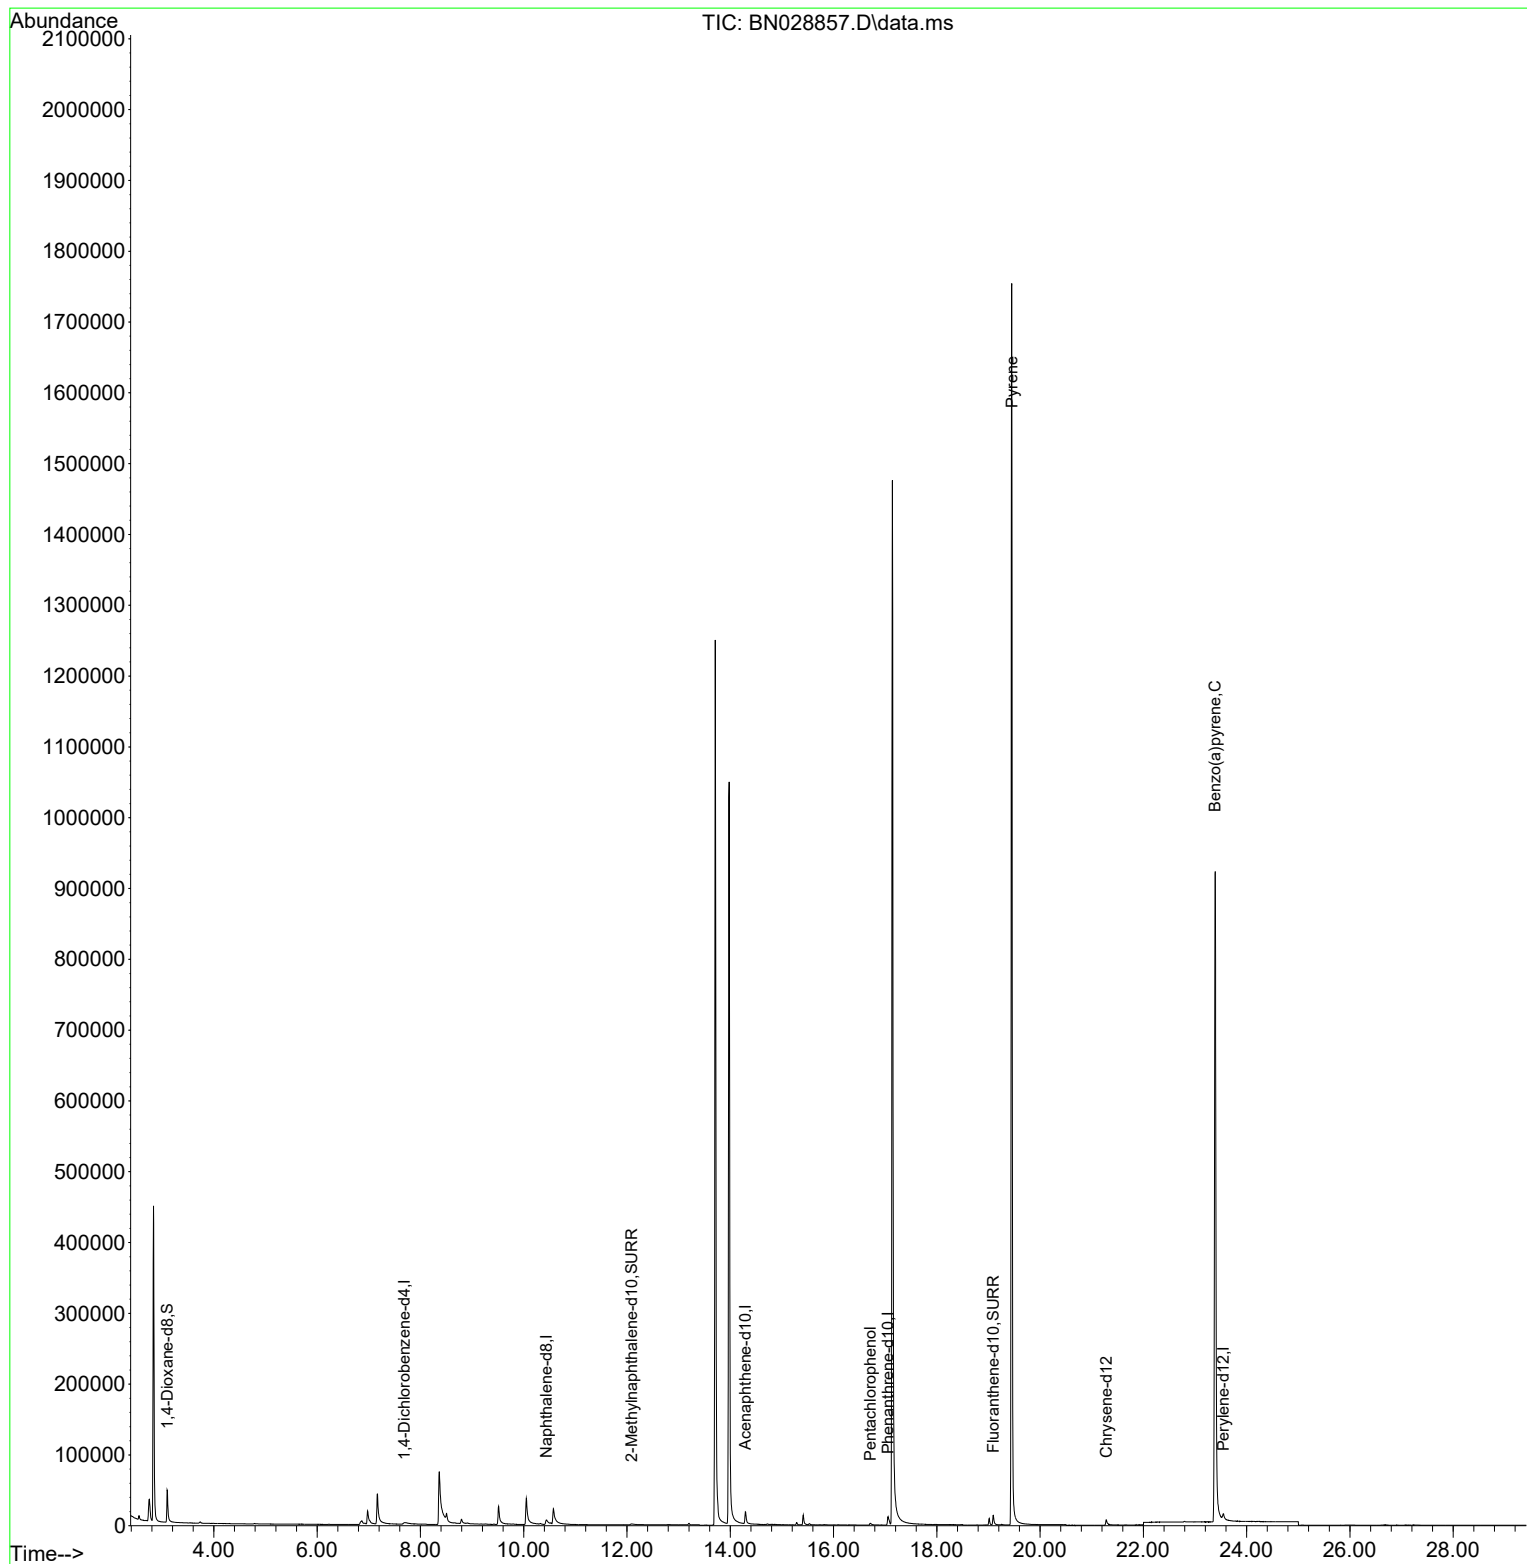


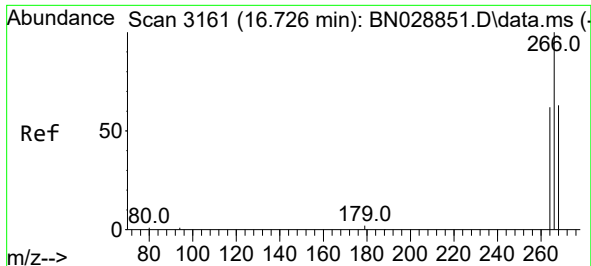

#14
 Pentachlorophenol
 Concen: 0.555 ng/ul
 RT: 16.710 min Scan# 3161
 Delta R.T. -0.014 min
 Lab File: BN028857.D
 Acq: 24 Nov 2023 14:34




Instrument :
 BNA_N
 ClientSampleId :
 DCKB6


Tgt Ion:266 Resp: 2876
 Ion Ratio Lower Upper
 266 100
 264 62.9 50.1 75.1
 268 63.4 50.6 75.8

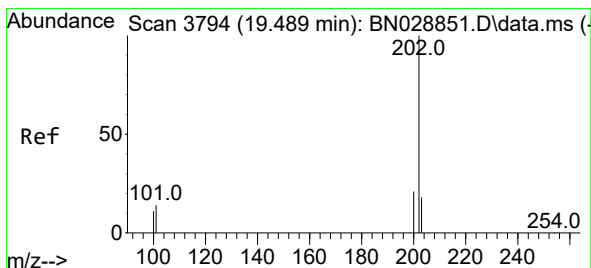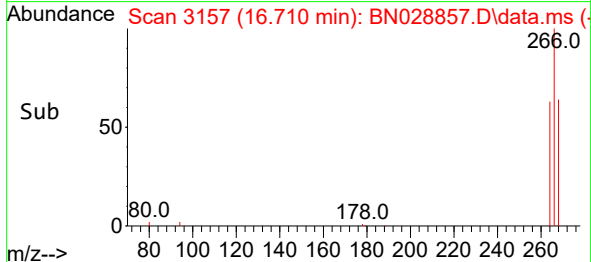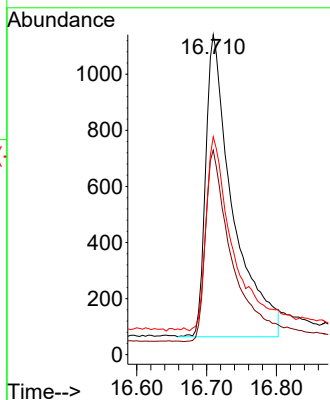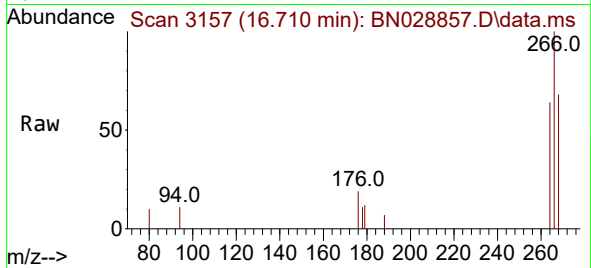

#20
 Pyrene
 Concen: 0.056 ng/ul
 RT: 19.452 min Scan# 3786
 Delta R.T. -0.033 min
 Lab File: BN028857.D
 Acq: 24 Nov 2023 14:34


Tgt Ion:202 Resp: 2924
 Ion Ratio Lower Upper
 202 100
 101 152.2 10.3 15.5#
 100 1061.9 8.2 12.2#

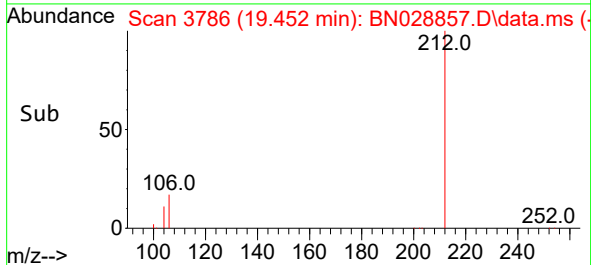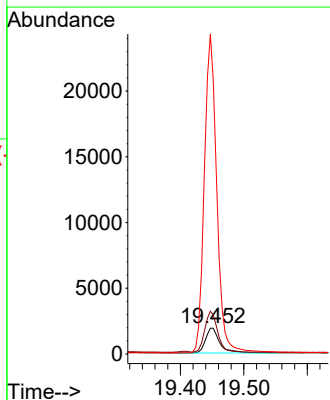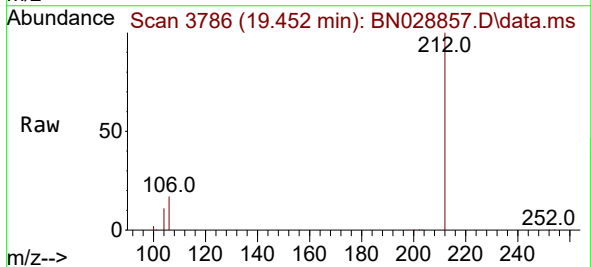

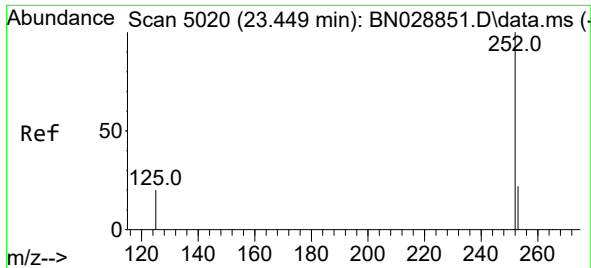

#26
 Benzo(a)pyrene
 Concen: 0.096 ng/ul
 RT: 23.388 min Scan# 4999
 Delta R.T. -0.056 min
 Lab File: BN028857.D
 Acq: 24 Nov 2023 14:34

Instrument :
 BNA_N
 ClientSampleId :
 DCKB6

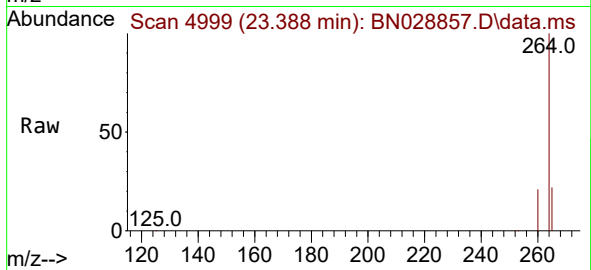

Tgt Ion:252 Resp: 4795
 Ion Ratio Lower Upper
 252 100
 253 48.3 19.0 28.6#
 125 44.3 13.2 19.8#

